

Data Path : P:\HPCHEM1\FID_E\Data\FE012718\
Data File : FE025892.D
Signal(s) : FID1B.CH
Acq On : 27 Jan 2018 21:57
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 27 23:44:04 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Sat Jan 27 14:10:49 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.772	3107954	19.732 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.963	236608	1.325 ug/ml
13) N-TRIACONTANE	17.826	157704	1.038 ug/ml
14) N-DOTRIACONTANE	18.657	258808	1.690 ug/ml
15) N-TETRATRIACONTANE	19.441	200599	1.537 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_E\Data\FE012718\
Data File : FE025892.D
Signal(s) : FID1B.CH
Acq On : 27 Jan 2018 21:57
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 27 23:44:04 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Sat Jan 27 14:10:49 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

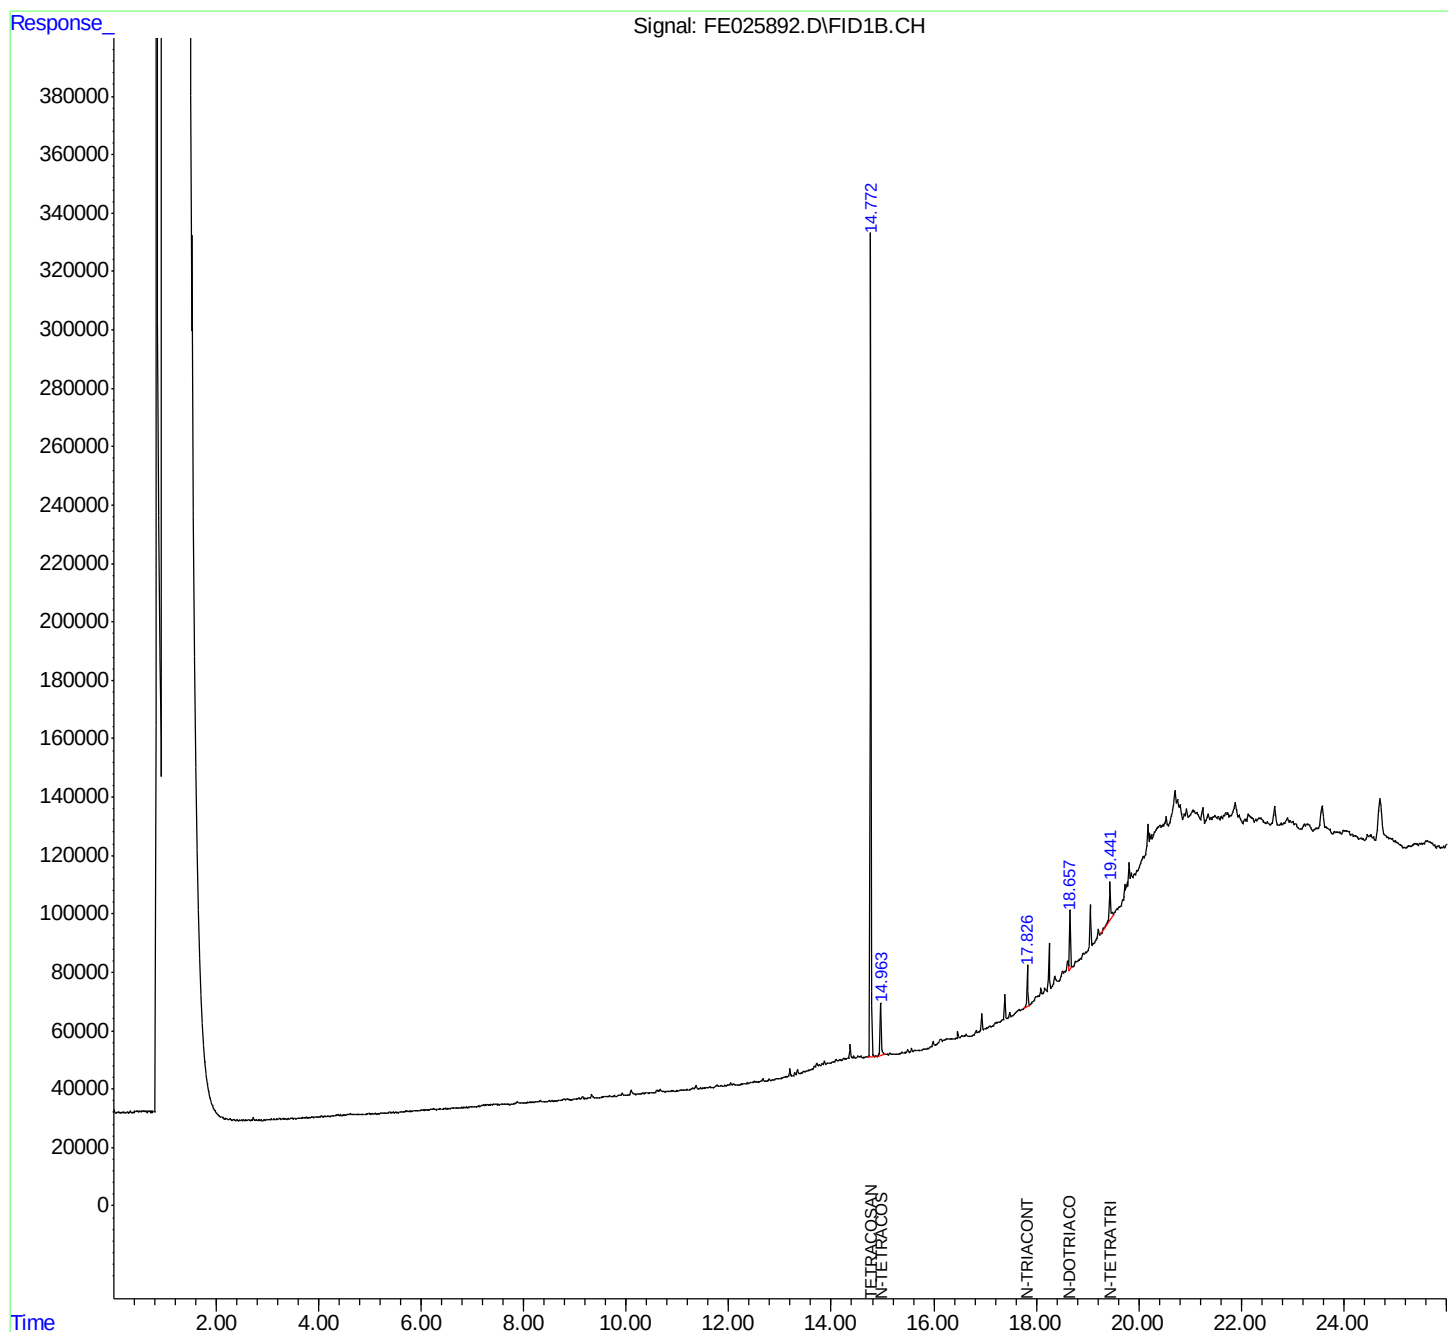

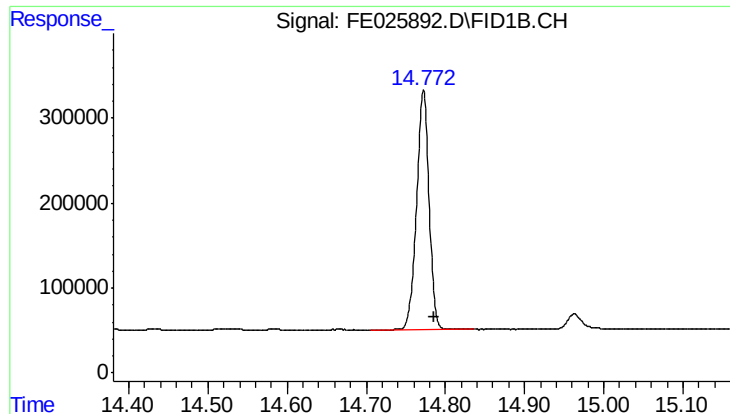


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.772 min
Delta R.T.: -0.013 min
Response: 3107954
Conc: 19.73 ug/ml

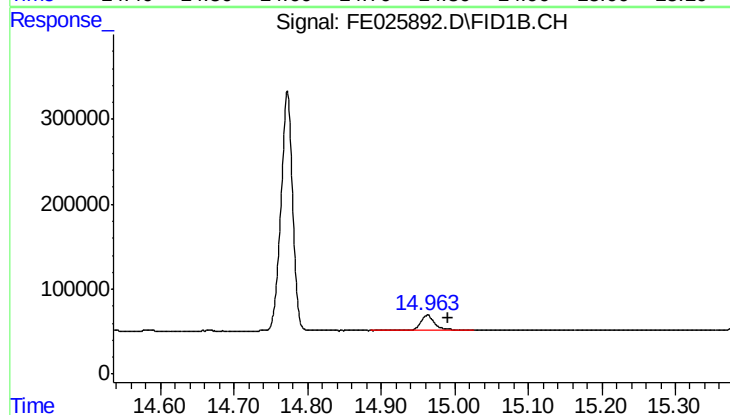


#10 N-TETRACOSANE

R.T.: 14.963 min
Delta R.T.: -0.028 min
Response: 236608
Conc: 1.33 ug/ml

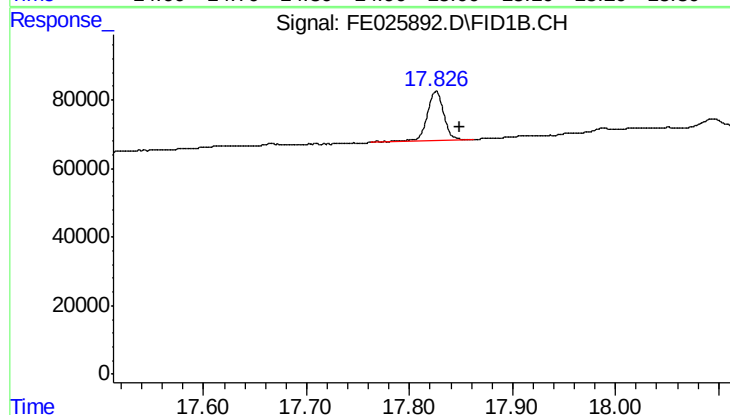


#13 N-TRIACONTANE

R.T.: 17.826 min
Delta R.T.: -0.022 min
Response: 157704
Conc: 1.04 ug/ml

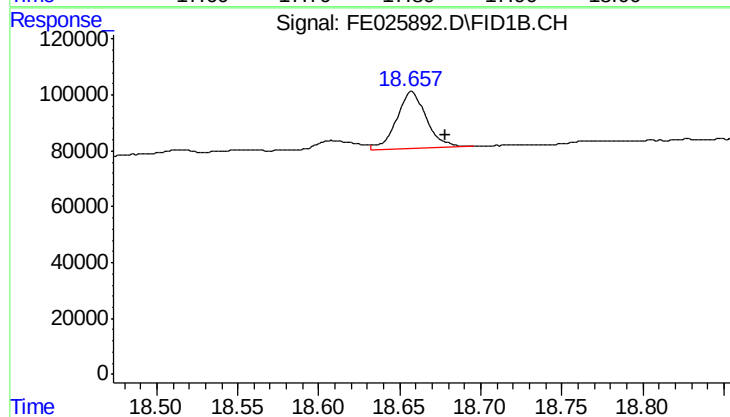

#14 N-DOTRIACONTANE

R.T.: 18.657 min
Delta R.T.: -0.021 min
Response: 258808
Conc: 1.69 ug/ml

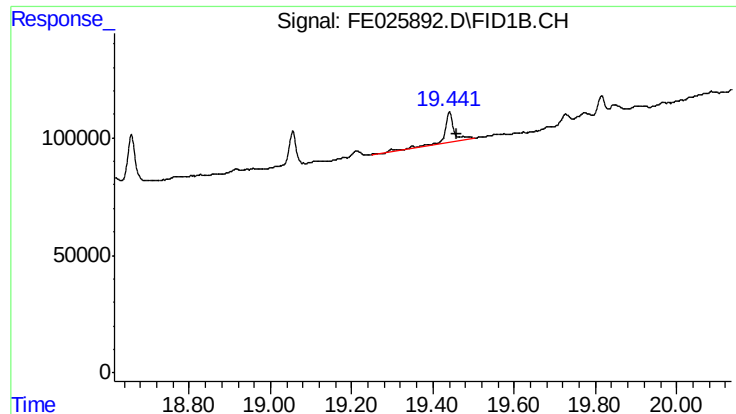

#15 N-TETRATRIACONTANE

R.T.: 19.441 min
Delta R.T.: -0.019 min
Response: 200599
Conc: 1.54 ug/ml