

Data Path : P:\HPCHEM1\FID E\Data\FE013018\
 Data File : FE025991.D
 Signal(s) : FID1B.CH
 Acq On : 30 Jan 2018 19:47
 Operator : UA/AJ
 Sample : PB106140BS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 31 05:48:15 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
 Quant Title :
 QLast Update : Tue Jan 30 11:45:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.757	3054117	19.255 ug/ml
Target Compounds			
2) N-DECANE	4.509	3404179	21.541 ug/ml
3) N-DODECANE	6.524	3939429	23.040 ug/ml
4) N-TETRADECANE	8.318	4444171	23.713 ug/ml
5) N-HEXADECANE	9.917	4828649	24.316 ug/ml
6) N-OCTADECANE	11.358	5023308	23.801 ug/ml
7) N-EICOSANE	12.665	4963313	24.026 ug/ml
8) N-DOCOSANE	13.862	4827838	24.686 ug/ml
10) N-TETRACOSANE	14.963	4556670	24.975 ug/ml
11) N-HEXACOSANE	15.981	4160111	25.414 ug/ml
12) N-OCTACOSANE	16.930	3851909	25.374 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE013018\
Data File : FE025991.D
Signal(s) : FID1B.CH
Acq On : 30 Jan 2018 19:47
Operator : UA/AJ
Sample : PB106140BS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 31 05:48:15 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Tue Jan 30 11:45:47 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

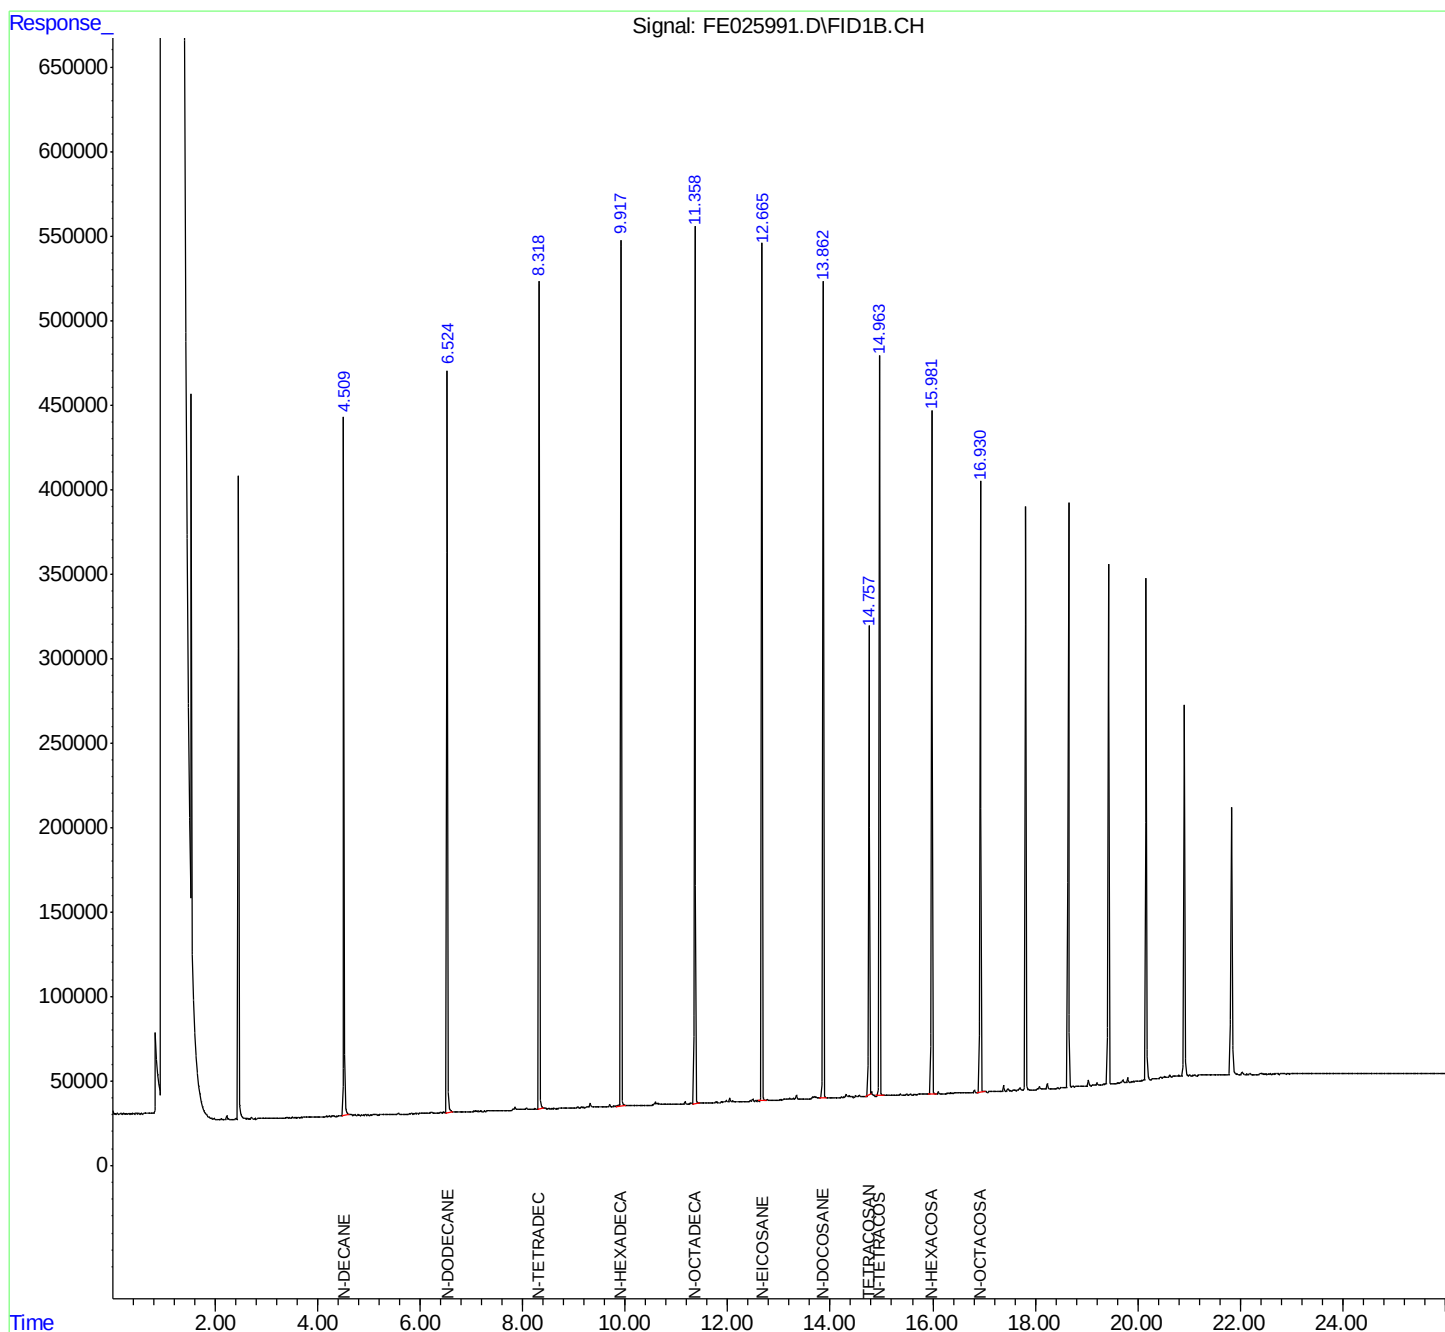


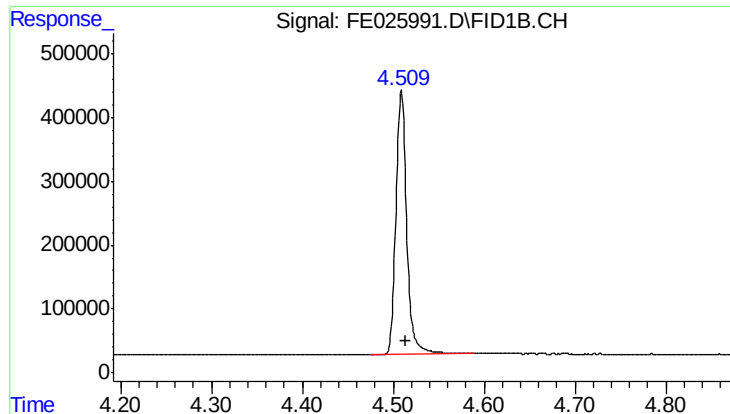

#2 N-DECANE


R.T.: 4.509 min
Delta R.T.: -0.005 min
Response: 3404179
Conc: 21.54 ug/ml

Instrument :
FID_E
ClientSampleId :

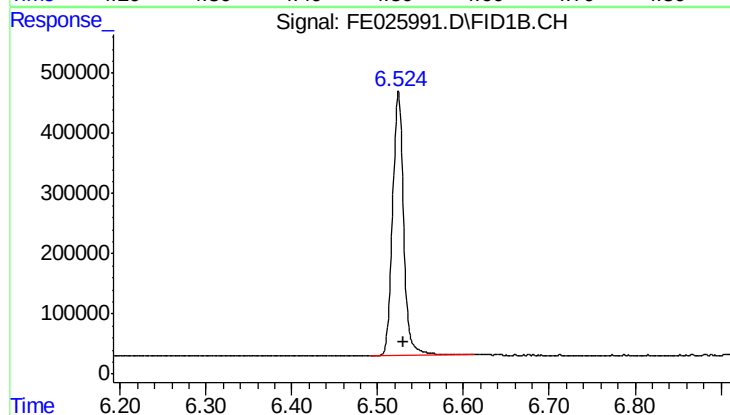


#3 N-DODECANE

R.T.: 6.524 min
Delta R.T.: -0.006 min
Response: 3939429
Conc: 23.04 ug/ml

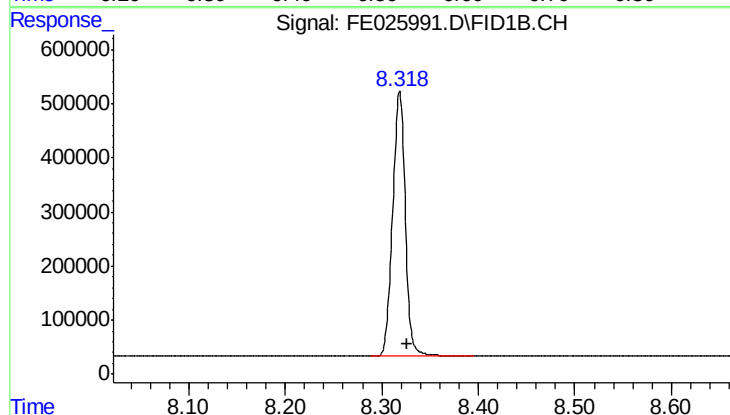


#4 N-TETRADECANE

R.T.: 8.318 min
Delta R.T.: -0.008 min
Response: 4444171
Conc: 23.71 ug/ml

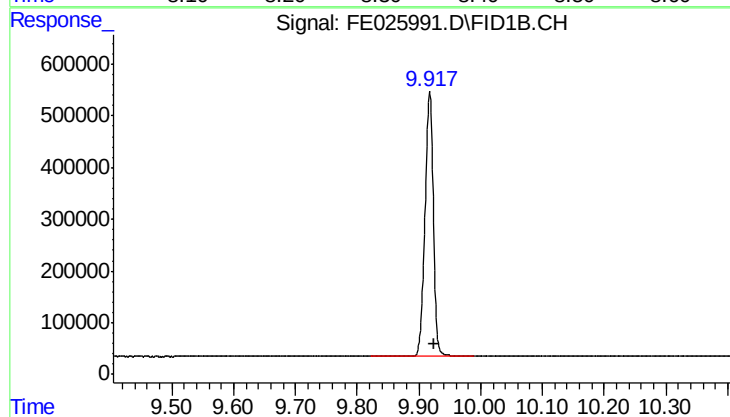

#5 N-HEXADECANE


R.T.: 9.917 min
Delta R.T.: -0.008 min
Response: 4828649
Conc: 24.32 ug/ml

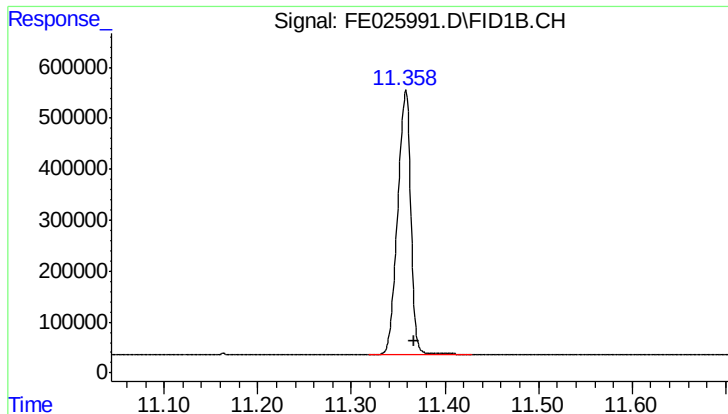

#6 N-OCTADECANE


R.T.: 11.358 min
Delta R.T.: -0.009 min
Response: 5023308
Conc: 23.80 ug/ml

Instrument :
FID_E
ClientSampleId :

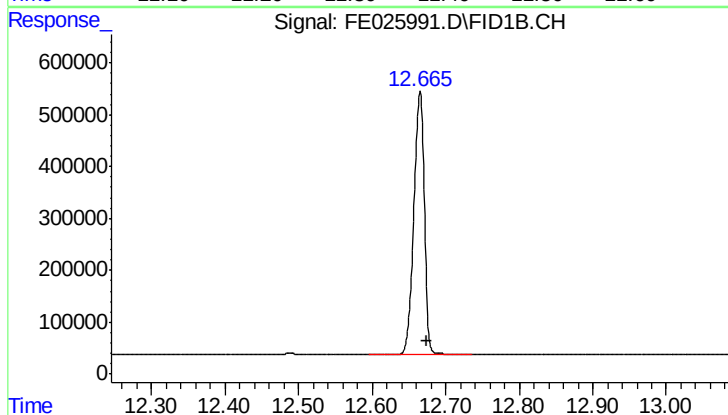


#7 N-EICOSANE

R.T.: 12.665 min
Delta R.T.: -0.009 min
Response: 4963313
Conc: 24.03 ug/ml

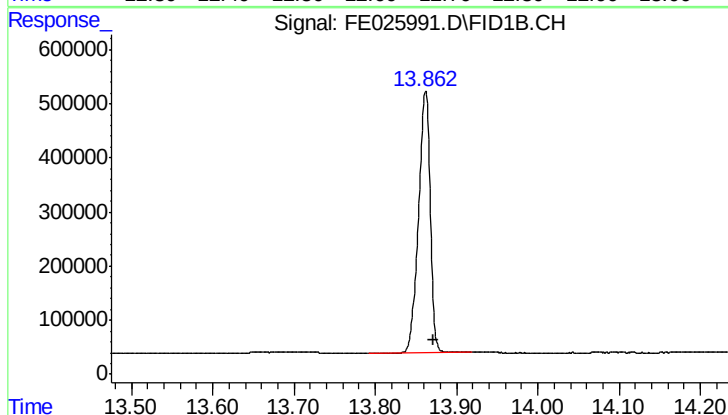


#8 N-DOCOSANE

R.T.: 13.862 min
Delta R.T.: -0.009 min
Response: 4827838
Conc: 24.69 ug/ml

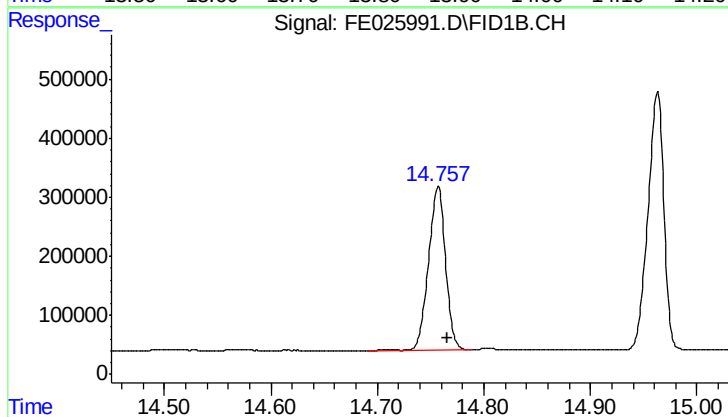

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.757 min
Delta R.T.: -0.009 min
Response: 3054117
Conc: 19.25 ug/ml

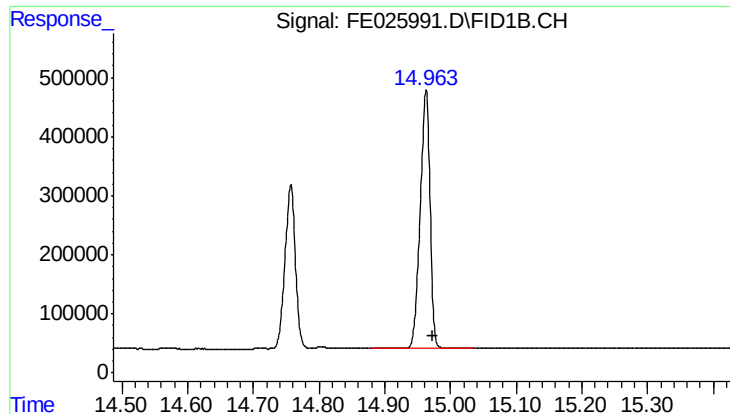

#10 N-TETRACOSANE


R.T.: 14.963 min
Delta R.T.: -0.010 min
Response: 4556670
Conc: 24.98 ug/ml

Instrument :
FID_E
ClientSampleId :

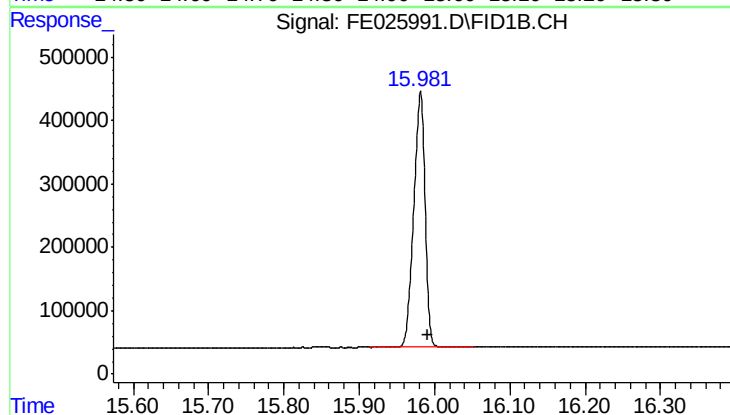

#11 N-HEXACOSANE

R.T.: 15.981 min
Delta R.T.: -0.010 min
Response: 4160111
Conc: 25.41 ug/ml

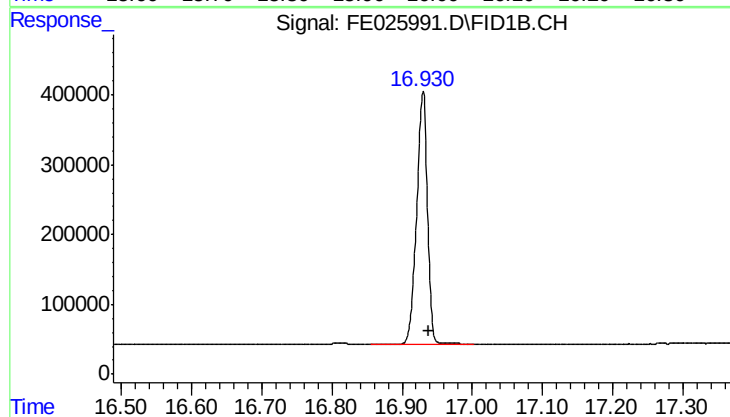

#12 N-OCTACOSANE

R.T.: 16.930 min
Delta R.T.: -0.010 min
Response: 3851909
Conc: 25.37 ug/ml