

Data Path : P:\HPCHEM1\FID E\Data\FE013018\
 Data File : FE026001.D
 Signal(s) : FID1B.CH
 Acq On : 31 Jan 2018 1:39
 Operator : UA/AJ
 Sample : J1353-11MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 31 05:49:37 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
 Quant Title :
 QLast Update : Tue Jan 30 11:45:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.755	3234377	20.391 ug/ml
Target Compounds				
2)	N-DECANE	4.509	4267384	27.003 ug/ml
3)	N-DODECANE	6.524	5008321	29.292 ug/ml
4)	N-TETRADECANE	8.318	5701163	30.420 ug/ml
5)	N-HEXADECANE	9.918	6469231	32.578 ug/ml
6)	N-OCTADECANE	11.357	6176370	29.265 ug/ml
7)	N-EICOSANE	12.665	5624307	27.226 ug/ml
8)	N-DOCOSANE	13.860	5122581	26.194 ug/ml
10)	N-TETRACOSANE	14.961	4547522	24.925 ug/ml
11)	N-HEXACOSANE	15.980	4271516	26.095 ug/ml
12)	N-OCTACOSANE	16.929	4332939	28.543 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE013018\
Data File : FE026001.D
Signal(s) : FID1B.CH
Acq On : 31 Jan 2018 1:39
Operator : UA/AJ
Sample : J1353-11MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 31 05:49:37 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Tue Jan 30 11:45:47 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

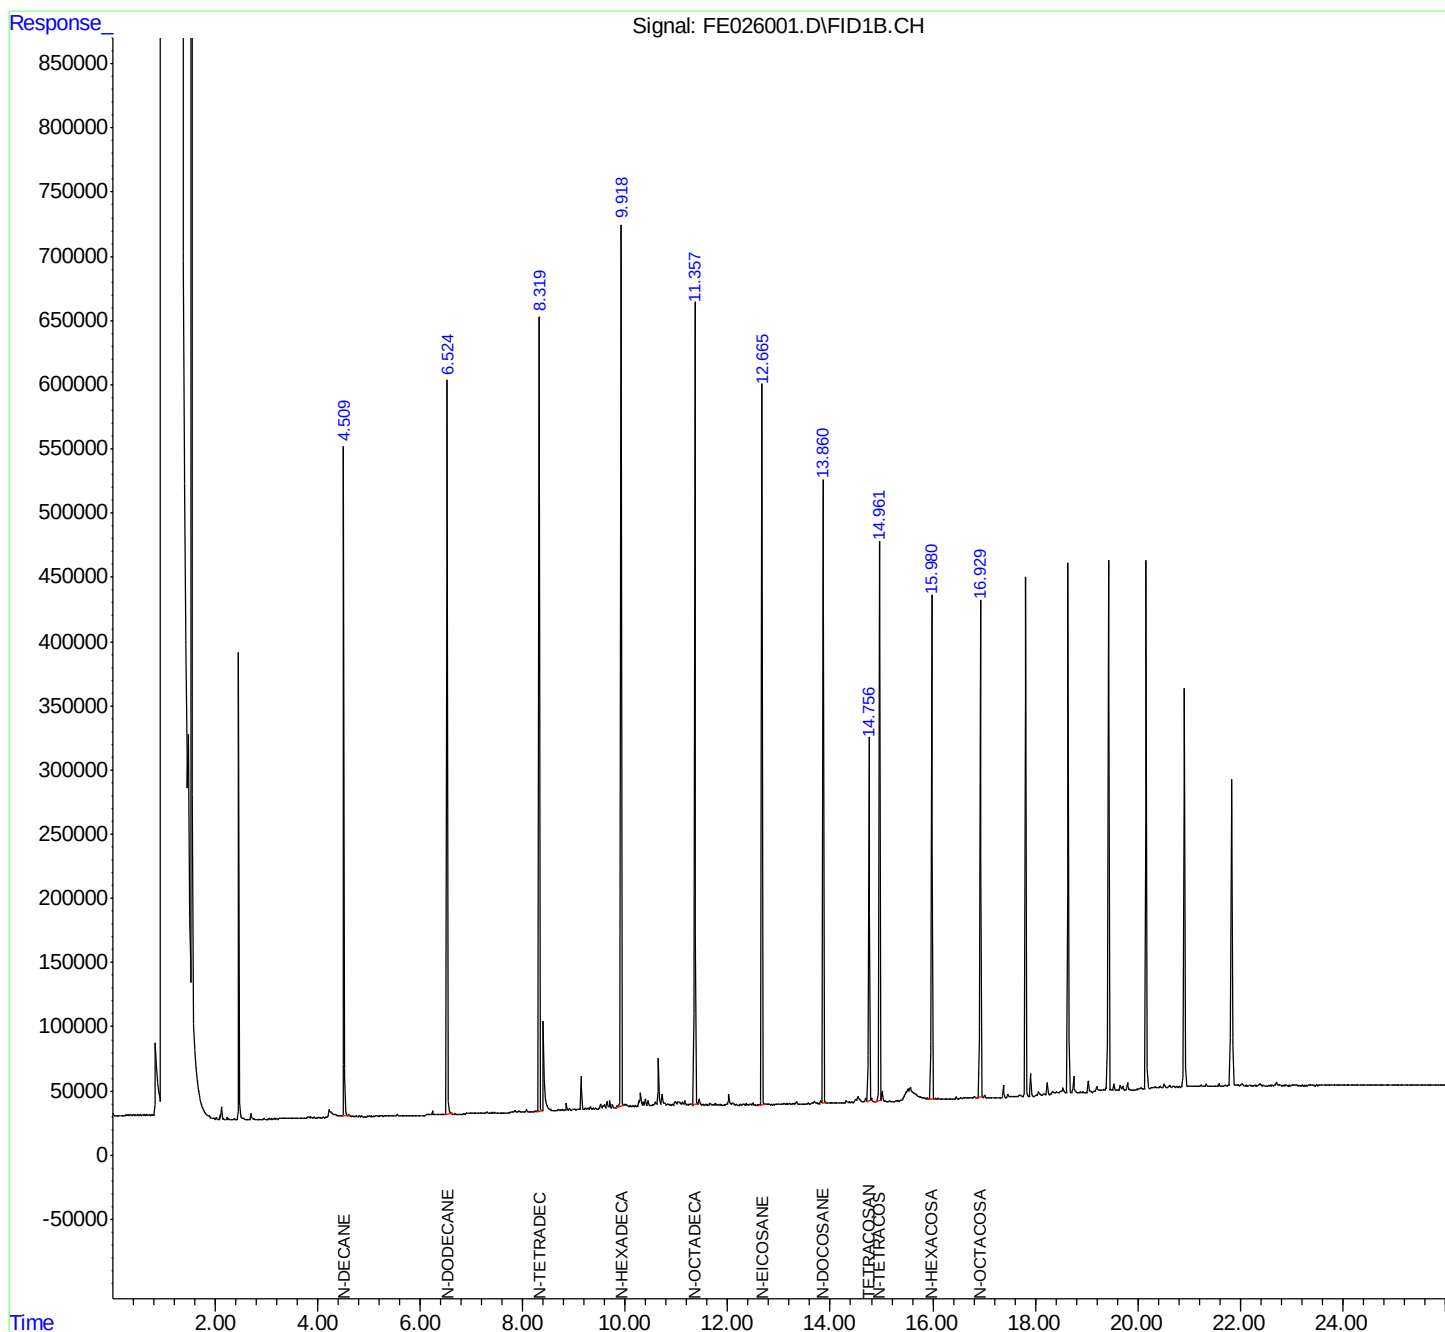


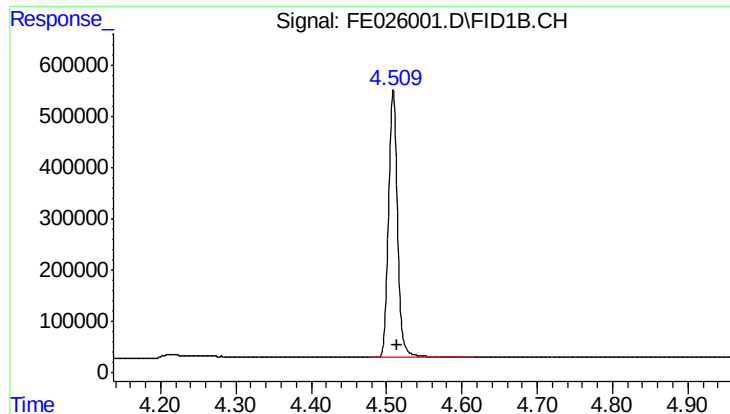

#2 N-DECANE


R.T.: 4.509 min
Delta R.T.: -0.005 min
Response: 4267384
Conc: 27.00 ug/ml

Instrument :
FID_E
ClientSampleId :

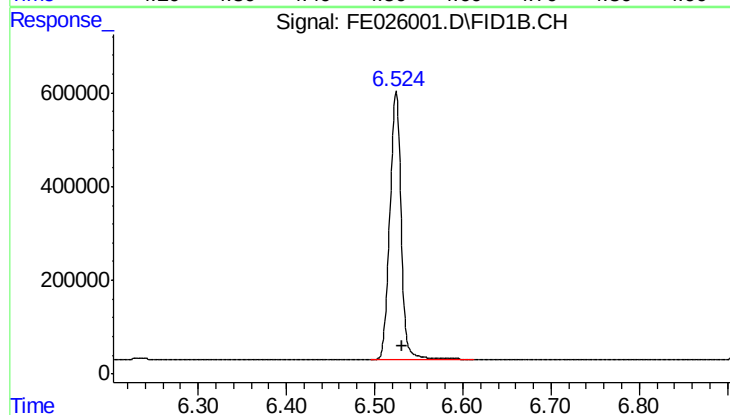


#3 N-DODECANE

R.T.: 6.524 min
Delta R.T.: -0.006 min
Response: 5008321
Conc: 29.29 ug/ml

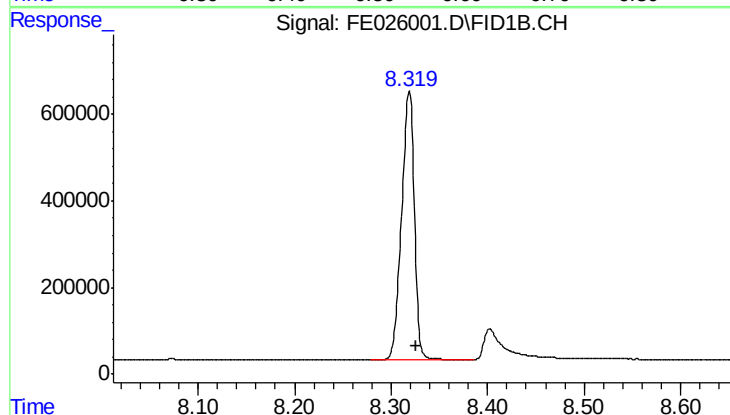


#4 N-TETRADECANE

R.T.: 8.318 min
Delta R.T.: -0.008 min
Response: 5701163
Conc: 30.42 ug/ml

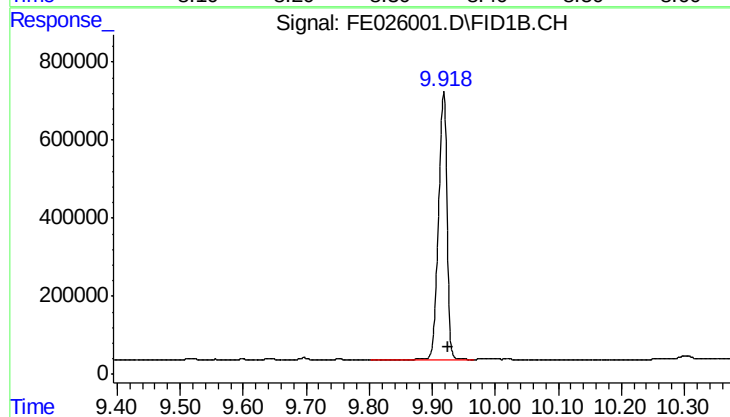

#5 N-HEXADECANE


R.T.: 9.918 min
Delta R.T.: -0.008 min
Response: 6469231
Conc: 32.58 ug/ml

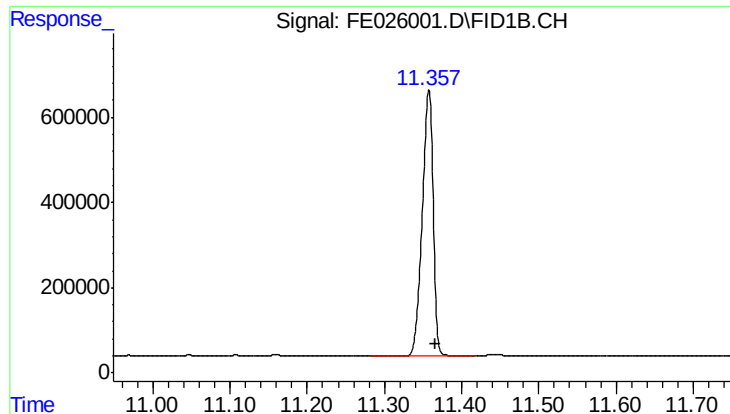

#6 N-OCTADECANE


R.T.: 11.357 min
Delta R.T.: -0.009 min
Response: 6176370
Conc: 29.26 ug/ml

Instrument :
FID_E
ClientSampleId :

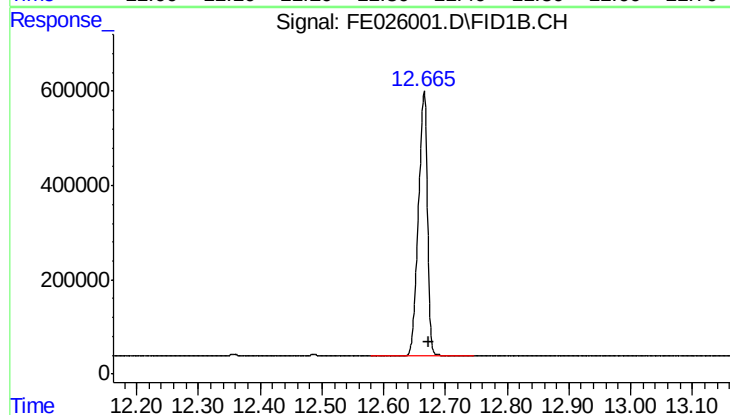


#7 N-EICOSANE

R.T.: 12.665 min
Delta R.T.: -0.009 min
Response: 5624307
Conc: 27.23 ug/ml

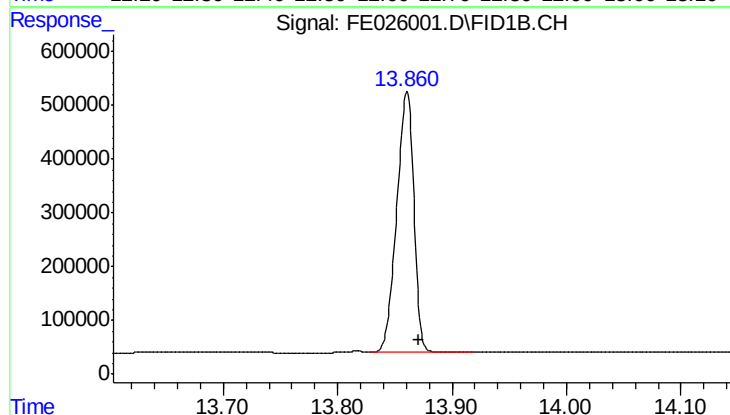


#8 N-DOCOSANE

R.T.: 13.860 min
Delta R.T.: -0.010 min
Response: 5122581
Conc: 26.19 ug/ml

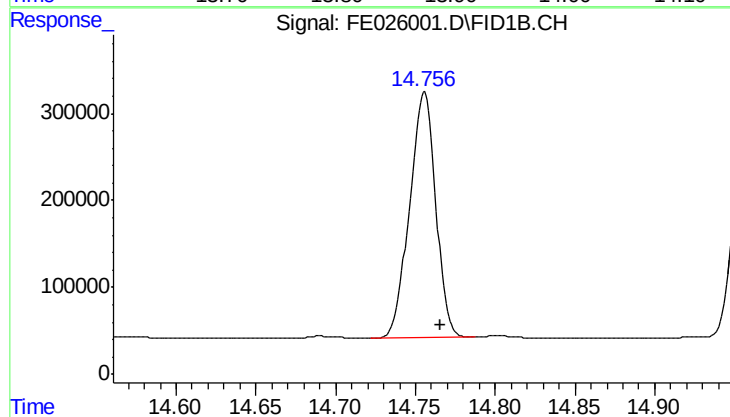

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.755 min
Delta R.T.: -0.010 min
Response: 3234377
Conc: 20.39 ug/ml

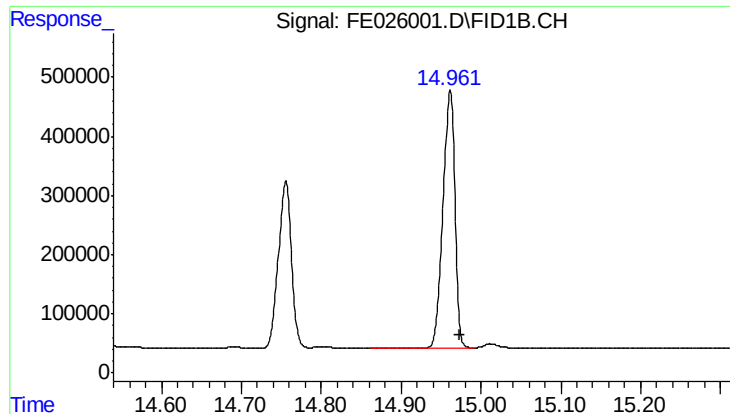

#10 N-TETRACOSANE


R.T.: 14.961 min
Delta R.T.: -0.012 min
Response: 4547522
Conc: 24.93 ug/ml

Instrument :
FID_E
ClientSampleId :

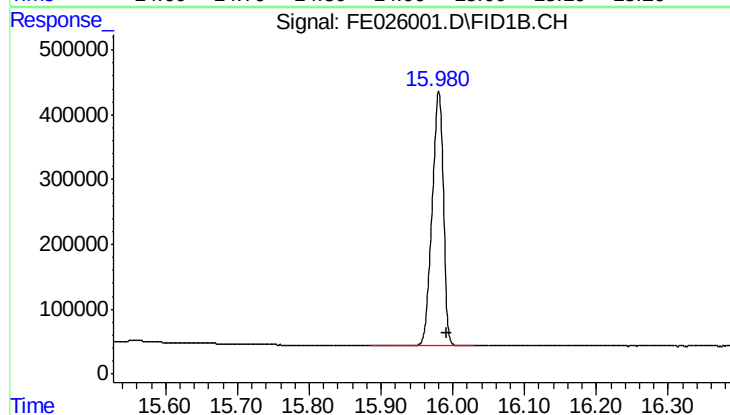

#11 N-HEXACOSANE

R.T.: 15.980 min
Delta R.T.: -0.011 min
Response: 4271516
Conc: 26.09 ug/ml

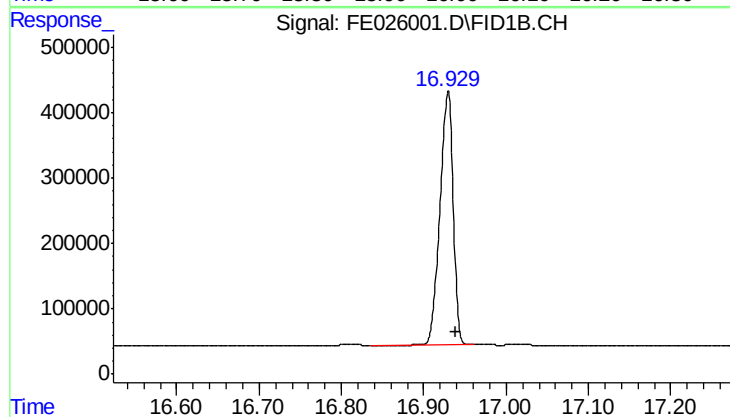

#12 N-OCTACOSANE

R.T.: 16.929 min
Delta R.T.: -0.010 min
Response: 4332939
Conc: 28.54 ug/ml