

Data Path : P:\HPCHEM1\FID E\Data\FE013118\
 Data File : FE026043.D
 Signal(s) : FID1B.CH
 Acq On : 01 Feb 2018 3:52
 Operator : UA/AJ
 Sample : J1016-07 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 01 06:36:37 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
 Quant Title :
 QLast Update : Tue Jan 30 11:45:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.750	241883	1.525 ug/ml
Target Compounds				
7)	N-EICOSANE	12.642	603444	2.921 ug/ml
8)	N-DOCOSANE	13.809f	298334	1.525 ug/ml
10)	N-TETRACOSANE	14.953	994946	5.453 ug/ml
12)	N-OCTACOSANE	16.923	949032	6.252 ug/ml
13)	N-TRIACONTANE	17.812	254693	1.672 ug/ml
14)	N-DOTRIACONTANE	18.645	428155	2.753 ug/ml
15)	N-TETRATRIACONTANE	19.426	155526	1.183 ug/ml
16)	N-HEXATRIACONTANE	20.166	176338	1.671 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE013118\
Data File : FE026043.D
Signal(s) : FID1B.CH
Acq On : 01 Feb 2018 3:52
Operator : UA/AJ
Sample : J1016-07 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Feb 01 06:36:37 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Tue Jan 30 11:45:47 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

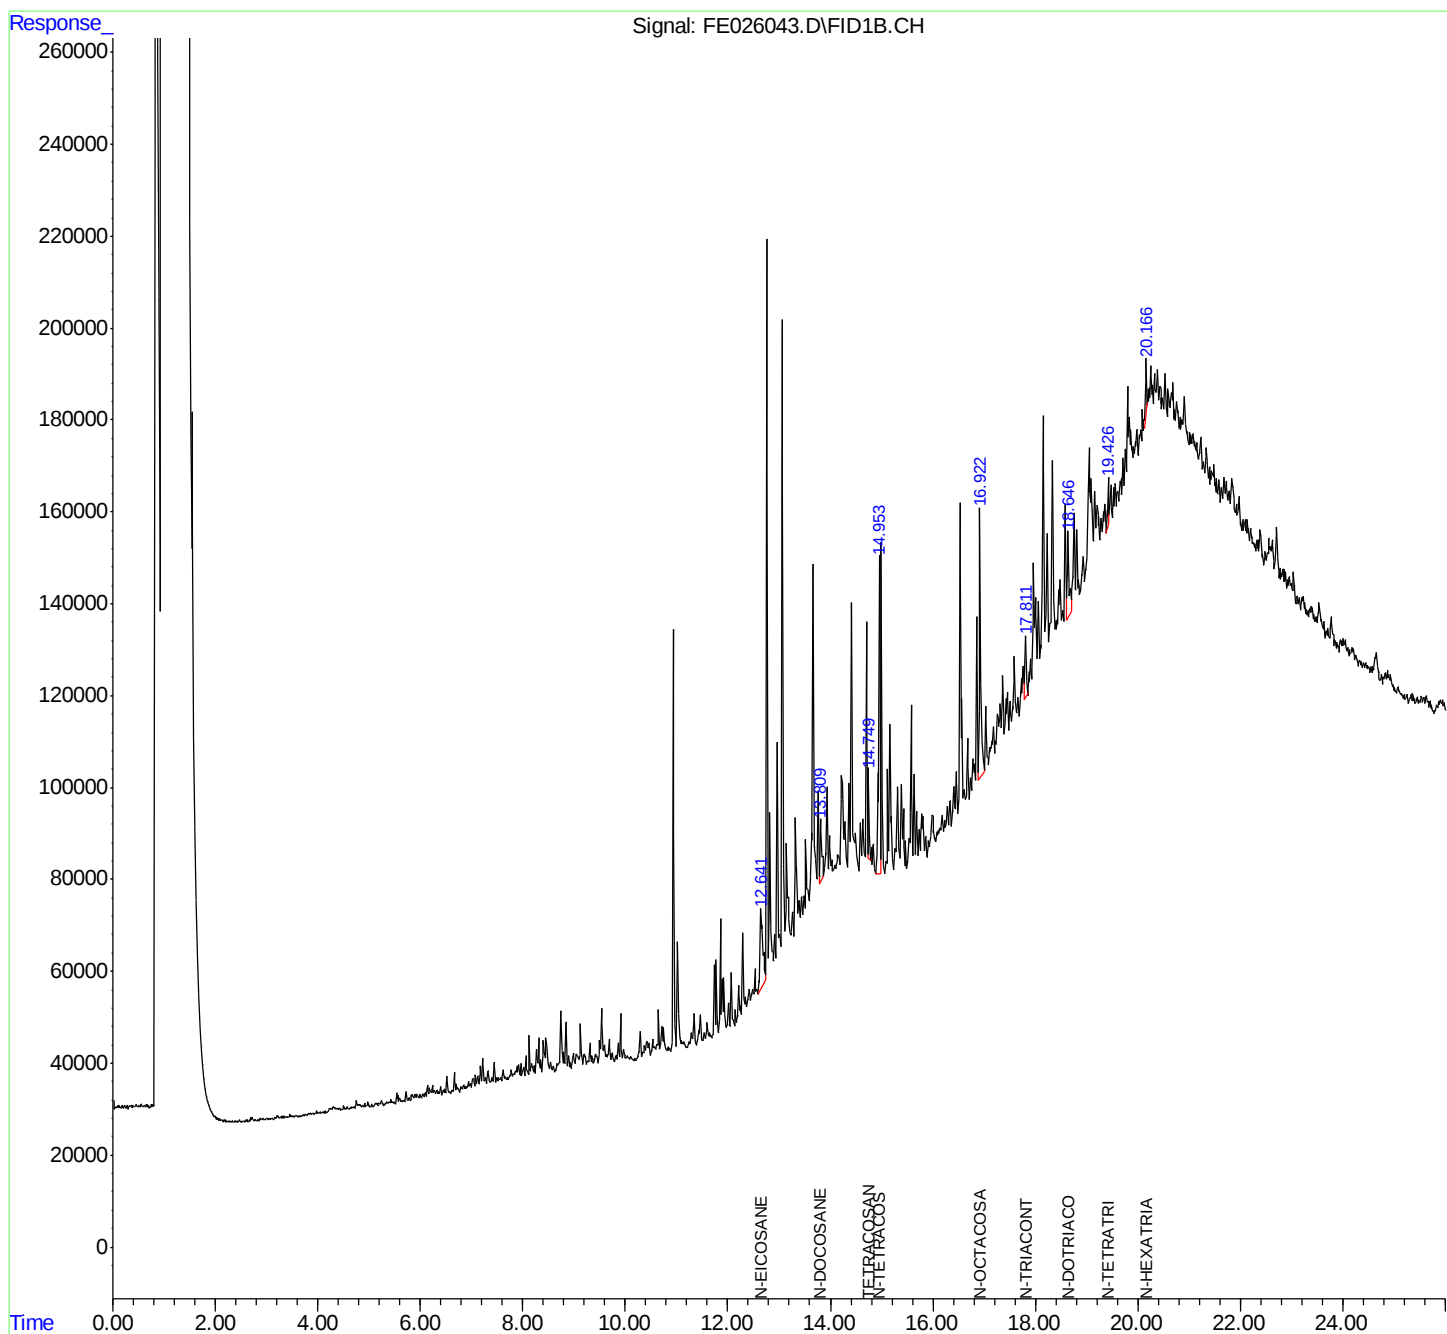


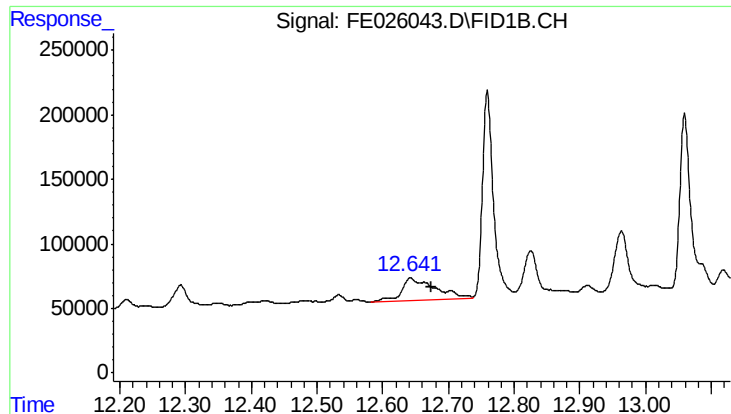

#7 N-EICOSANE


R.T.: 12.642 min
Delta R.T.: -0.032 min
Response: 603444
Conc: 2.92 ug/ml

Instrument :
FID_E
ClientSampleId :

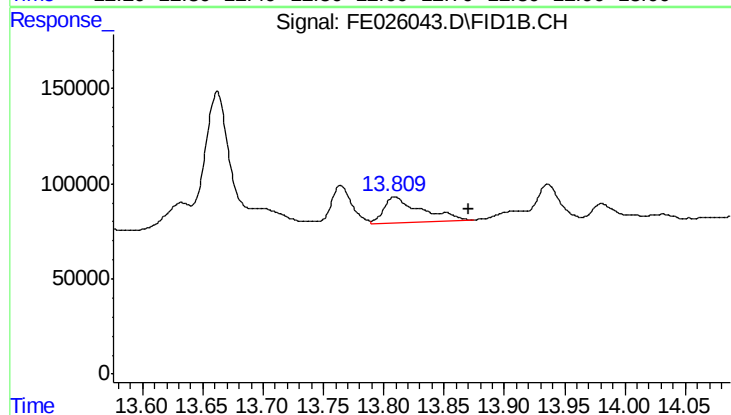


#8 N-DOCOSANE

R.T.: 13.809 min
Delta R.T.: -0.061 min
Response: 298334
Conc: 1.53 ug/ml

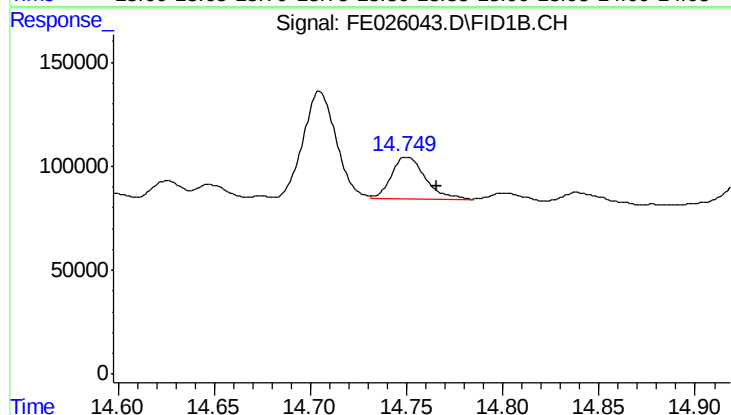


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: -0.015 min
Response: 241883
Conc: 1.52 ug/ml

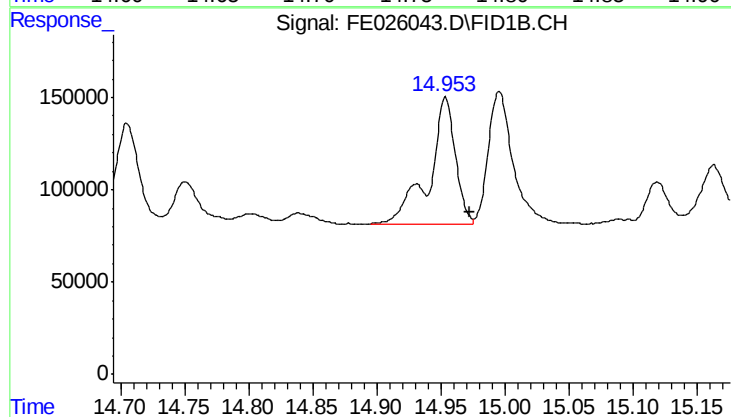

#10 N-TETRACOSANE


R.T.: 14.953 min
Delta R.T.: -0.019 min
Response: 994946
Conc: 5.45 ug/ml

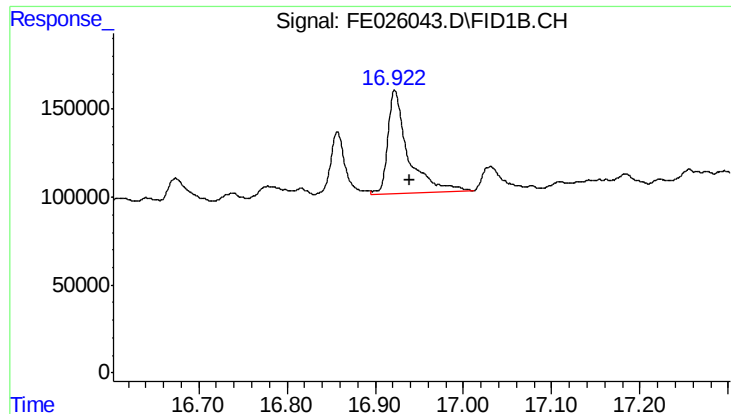

#12 N-OCTACOSANE


R.T.: 16.923 min
Delta R.T.: -0.017 min
Response: 949032
Conc: 6.25 ug/ml

Instrument :
FID_E
ClientSampleId :

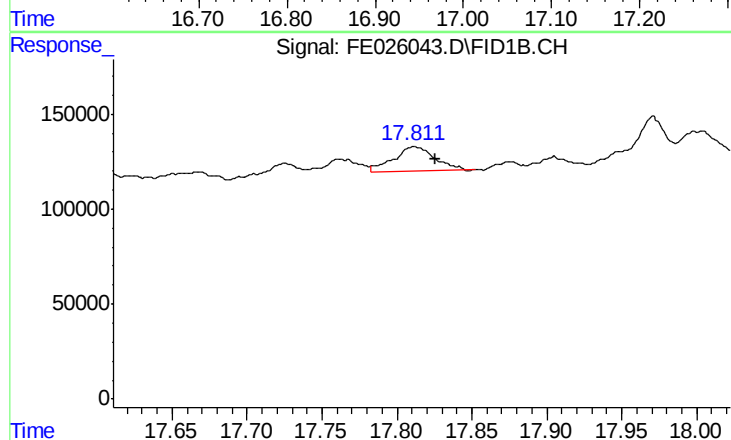


#13 N-TRIACONTANE

R.T.: 17.812 min
Delta R.T.: -0.014 min
Response: 254693
Conc: 1.67 ug/ml

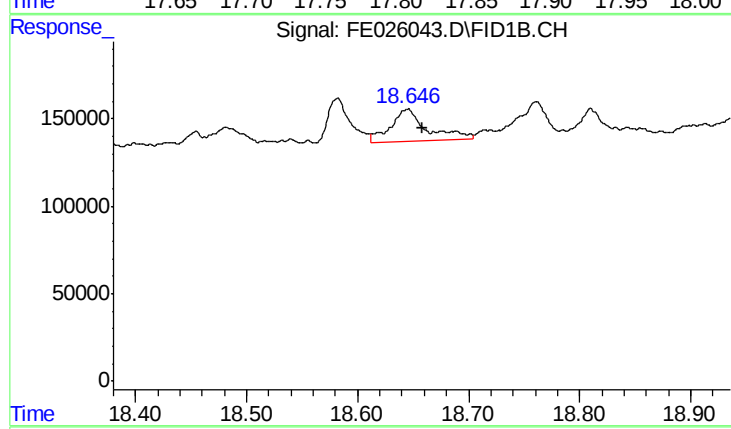


#14 N-DOTRIACONTANE

R.T.: 18.645 min
Delta R.T.: -0.014 min
Response: 428155
Conc: 2.75 ug/ml

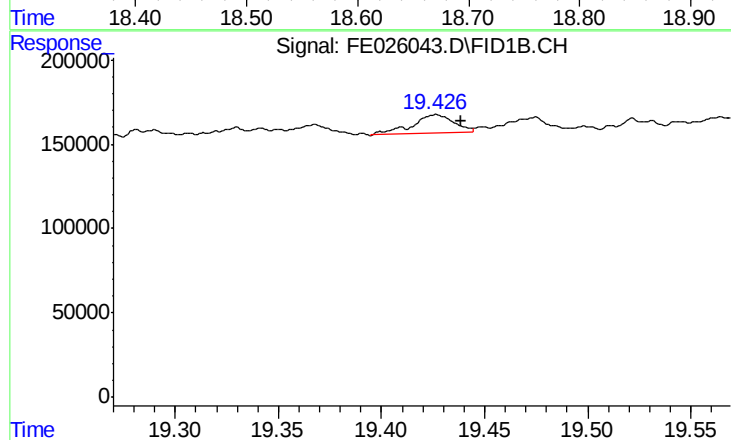

#15 N-TETRATRIACONTANE

R.T.: 19.426 min
Delta R.T.: -0.012 min
Response: 155526
Conc: 1.18 ug/ml

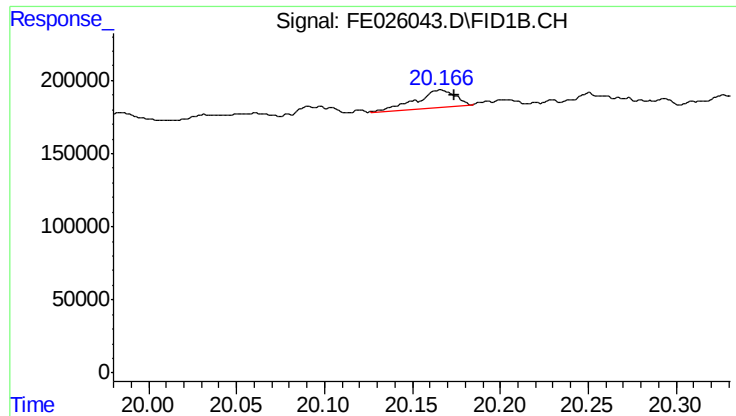

#16 N-HEXATRIACONTANE

R.T.: 20.166 min
Delta R.T.: -0.008 min
Response: 176338
Conc: 1.67 ug/ml

Instrument :
FID_E
ClientSampleId :