

Data Path : P:\HPCHEM1\FID E\Data\FE013118\
 Data File : FE026049.D
 Signal(s) : FID1B.CH
 Acq On : 01 Feb 2018 7:23
 Operator : UA/AJ
 Sample : J1015-24 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 01 08:04:54 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
 Quant Title :
 QLast Update : Tue Jan 30 11:45:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.752	393300	2.480 ug/ml
Target Compounds			
7) N-EICOSANE	12.644	344471	1.668 ug/ml
8) N-DOCOSANE	13.812f	129128	0.660 ug/ml
10) N-TETRACOSANE	14.953	979698	5.370 ug/ml
12) N-OCTACOSANE	16.925	1137516	7.493 ug/ml
13) N-TRIACONTANE	17.818	545679	3.582 ug/ml
14) N-DOTRIACONTANE	18.651	216278	1.391 ug/ml
15) N-TETRATRIACONTANE	19.434	226393	1.722 ug/ml
16) N-HEXATRIACONTANE	20.176	392024	3.714 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE013118\
Data File : FE026049.D
Signal(s) : FID1B.CH
Acq On : 01 Feb 2018 7:23
Operator : UA/AJ
Sample : J1015-24 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :

Integration File: autoint1.e
Quant Time: Feb 01 08:04:54 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Tue Jan 30 11:45:47 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

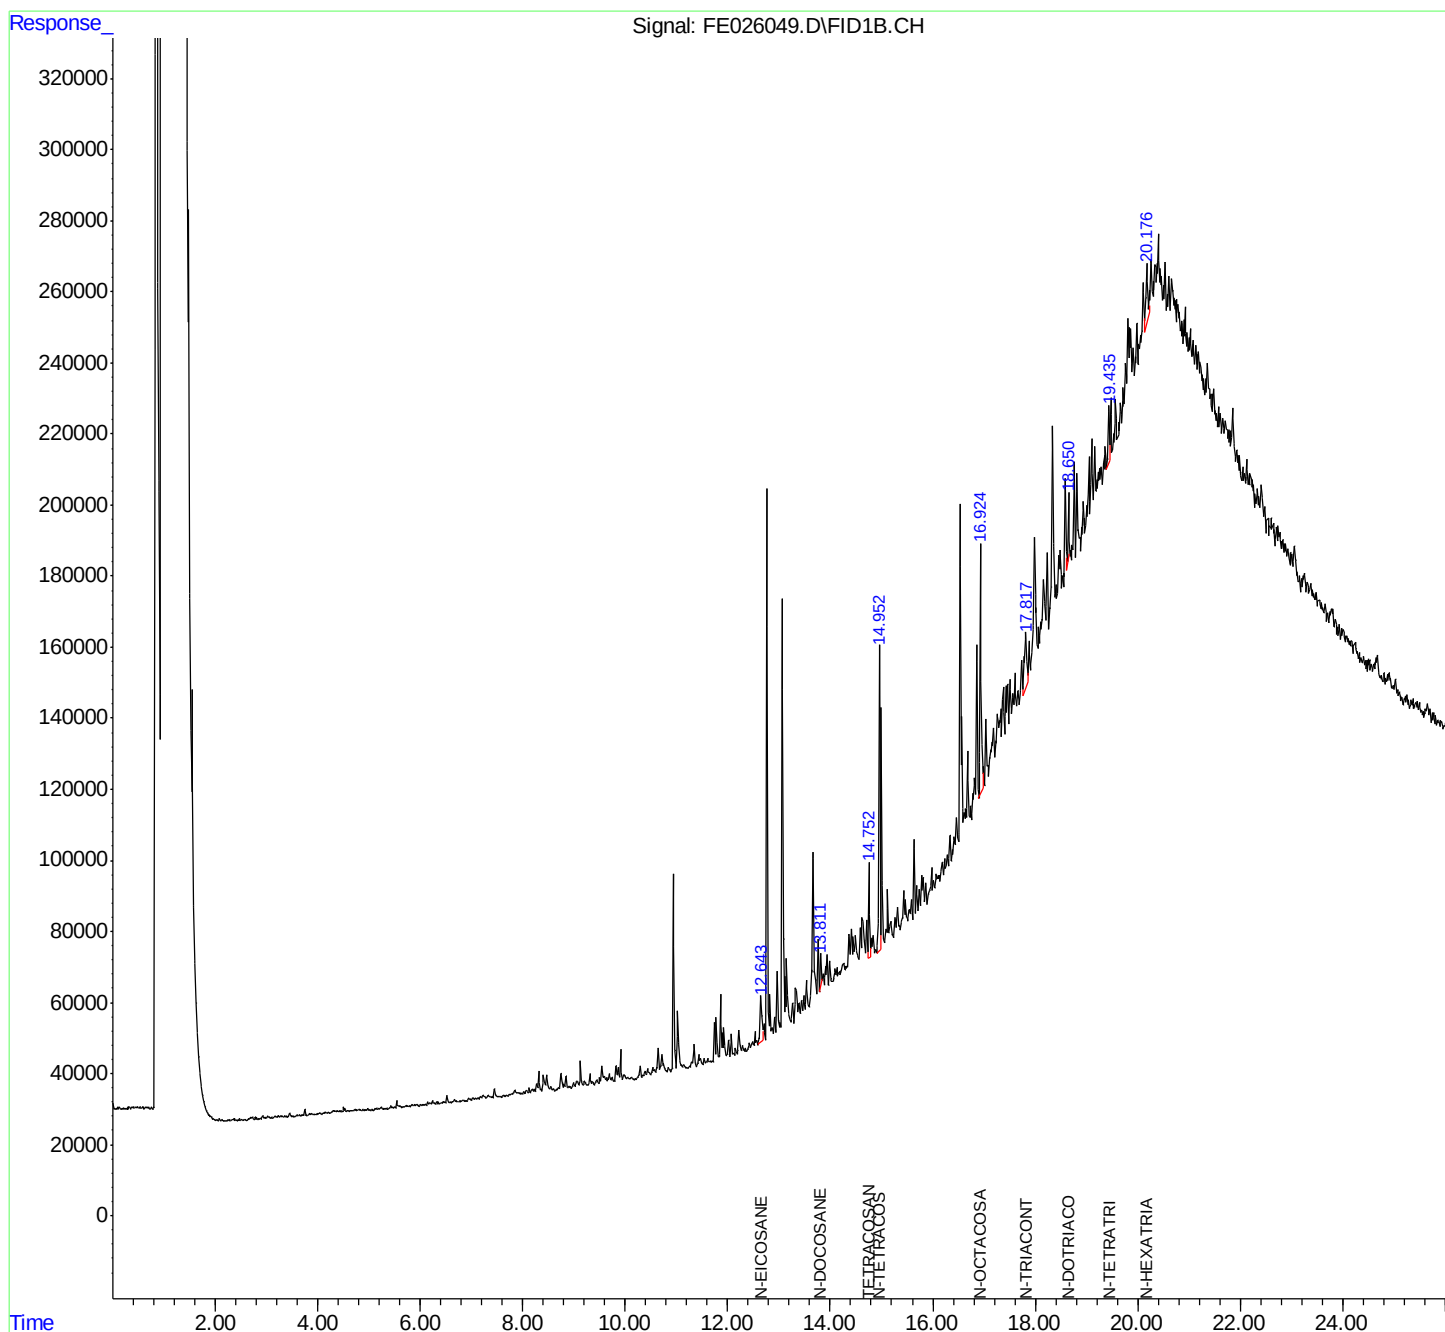


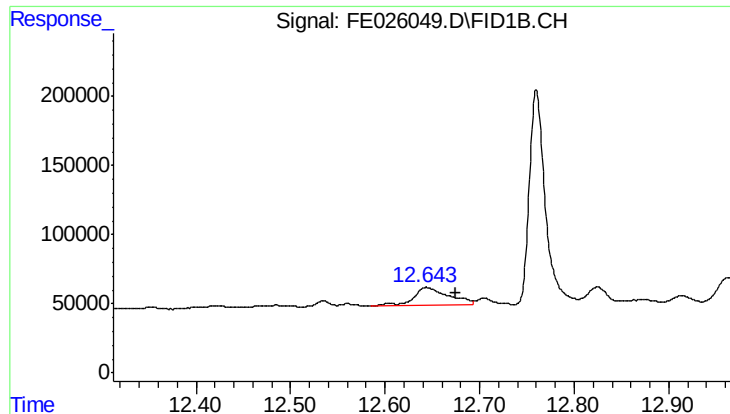

#7 N-EICOSANE


R.T.: 12.644 min
Delta R.T.: -0.030 min
Response: 344471
Conc: 1.67 ug/ml

Instrument :
FID_E
ClientSampleId :

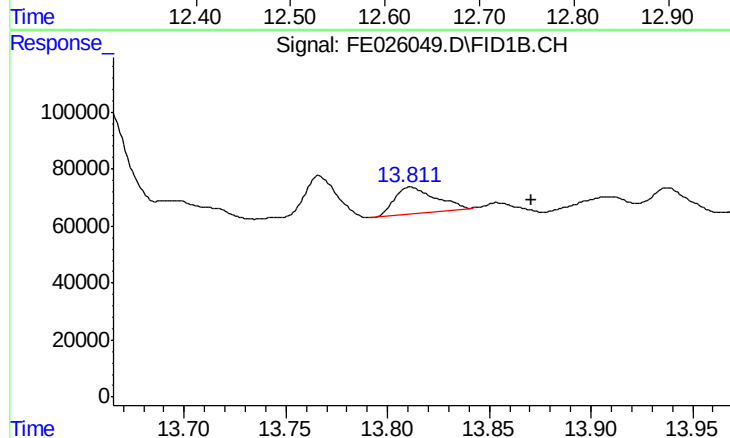


#8 N-DOCOSANE

R.T.: 13.812 min
Delta R.T.: -0.059 min
Response: 129128
Conc: 0.66 ug/ml

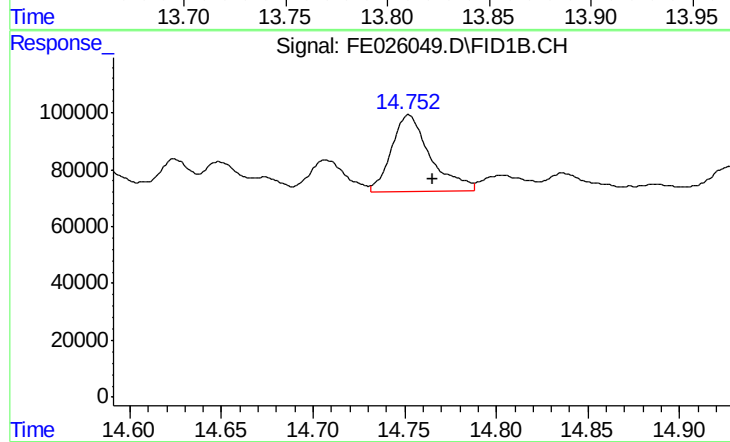


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.752 min
Delta R.T.: -0.013 min
Response: 393300
Conc: 2.48 ug/ml

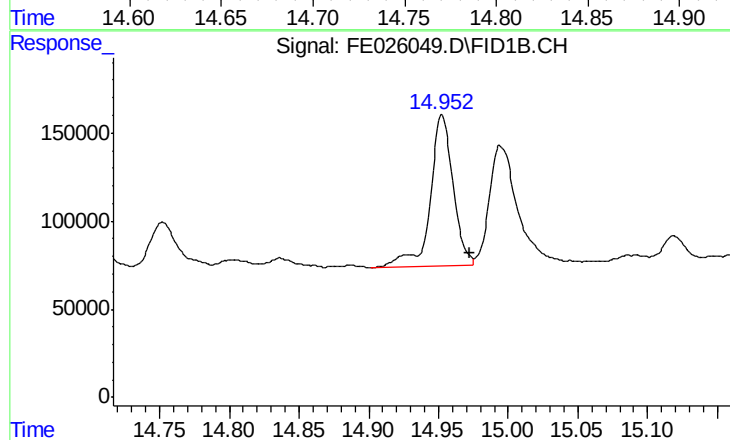

#10 N-TETRACOSANE


R.T.: 14.953 min
Delta R.T.: -0.020 min
Response: 979698
Conc: 5.37 ug/ml

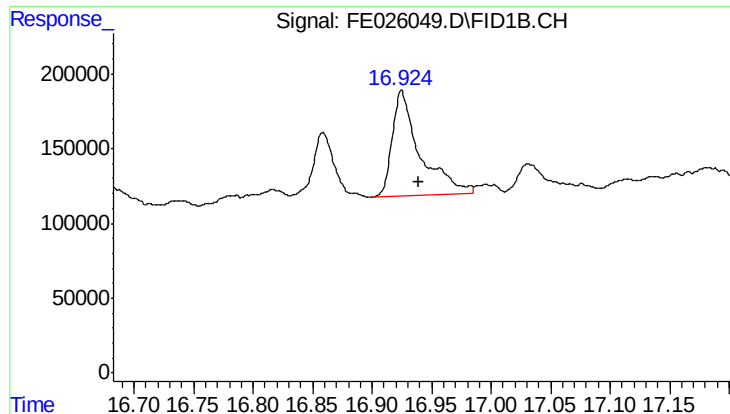

#12 N-OCTACOSANE


R.T.: 16.925 min
Delta R.T.: -0.014 min
Response: 1137516
Conc: 7.49 ug/ml

Instrument :
FID_E
ClientSampleId :

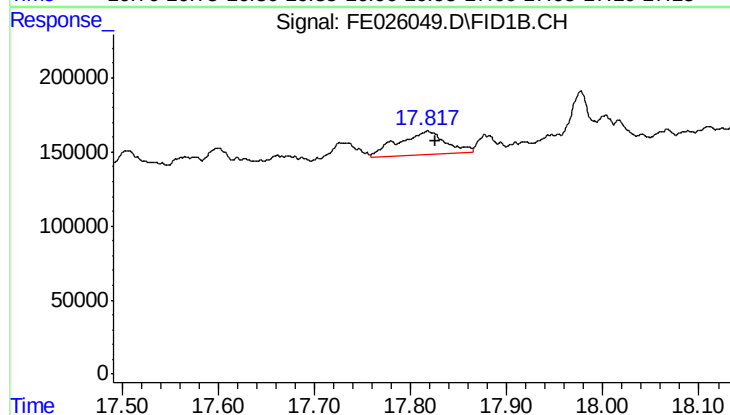


#13 N-TRIACONTANE

R.T.: 17.818 min
Delta R.T.: -0.008 min
Response: 545679
Conc: 3.58 ug/ml

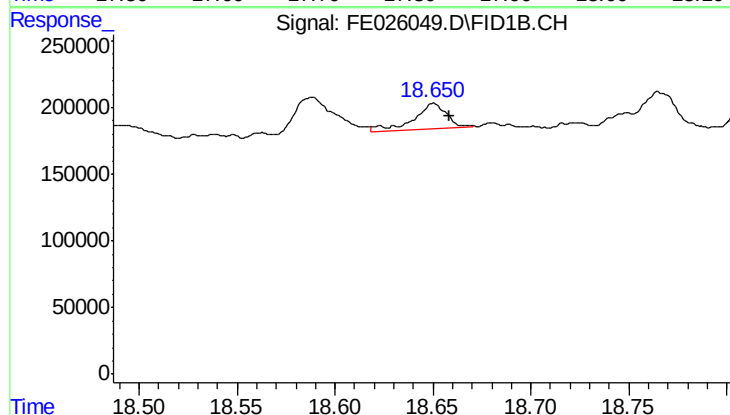


#14 N-DOTRIACONTANE

R.T.: 18.651 min
Delta R.T.: -0.008 min
Response: 216278
Conc: 1.39 ug/ml

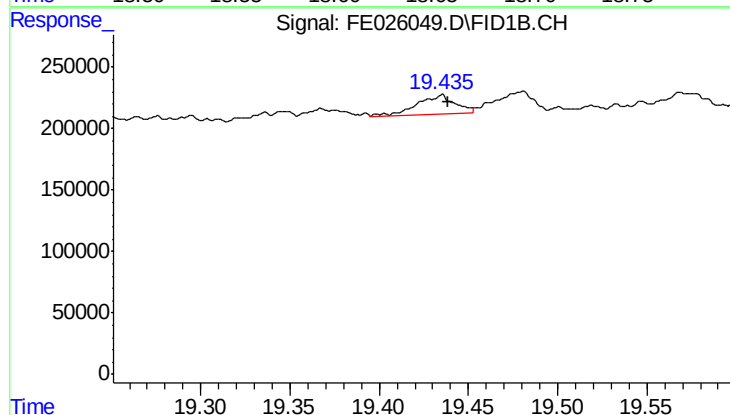

#15 N-TETRATRIACONTANE

R.T.: 19.434 min
Delta R.T.: -0.004 min
Response: 226393
Conc: 1.72 ug/ml

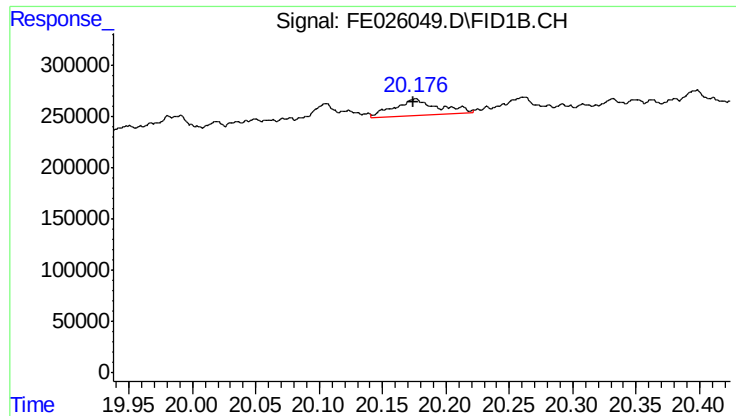

#16 N-HEXATRIACONTANE

R.T.: 20.176 min
Delta R.T.: 0.001 min
Response: 392024
Conc: 3.71 ug/ml

Instrument :
FID_E
ClientSampleId :