

Data Path : P:\HPCHEM1\ECD_L\Data\PL013118\
 Data File : PL032823.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2018 10:37
 Operator : UA\AJ
 Sample : J1333-07DL 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 P-7DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 10:51:14 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 04:03:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.994	35269990	5286716	3.945	4.222
28)	SA Decachlor...	8.116	9.030	19549884	4489128	1.680	2.360 #
Target Compounds							
3)	MA gamma-BHC...	4.171f	0.000	31231007	0	2.419	N.D. #
6)	B beta-BHC	4.338f	0.000	11106373	0	1.945	N.D. #
7)	B delta-BHC	0.000	5.030	0	762340	N.D.	0.343 #
12)	B 4,4'-DDE	5.548	6.316	201.6E6	31640208	15.867	16.591
13)	MA Dieldrin	5.675	6.459	382.1E6	62912194	29.849	32.920
15)	B Endosulfa...	6.141f	6.875	14814993	2108089	1.263	1.197
16)	A 4,4'-DDD	0.000	6.745f	0	3781494	N.D.	2.651 #
17)	MA 4,4'-DDT	6.298	7.097	53978208	9435082	5.106	7.076 #
19)	B Endosulfa...	6.584	7.222	436.8E6	81683616	39.434	50.648 #
20)	A Methoxychlor	0.000	7.500f	0	3380237	N.D.	4.147 #
23)	Chlordane-1	0.000	5.030	0	762340	N.D.	9.859 #
27)	Chlordane-5	6.141	0.000	14814993	0	29.963	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_L\Data\PL013118\
Data File : PL032823.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2018 10:37
Operator : UA\AJ
Sample : J1333-07DL 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :
P-7DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 10:51:14 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 04:03:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

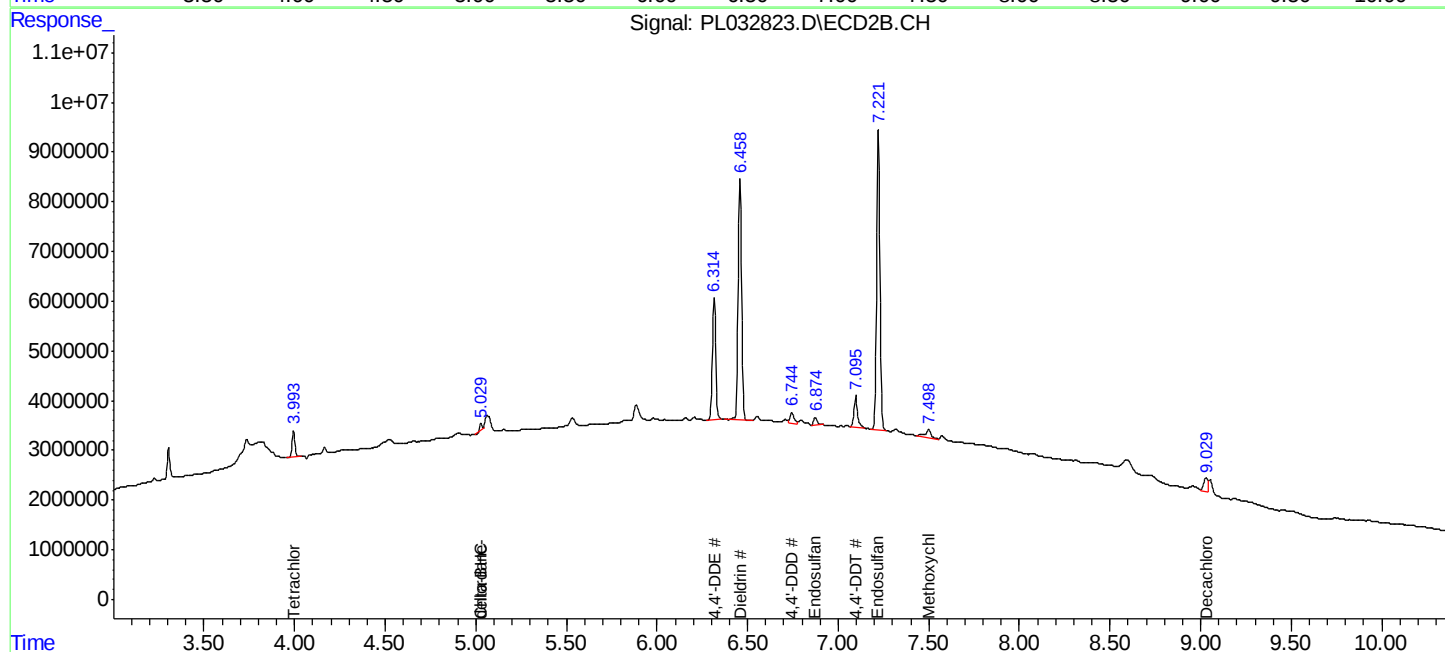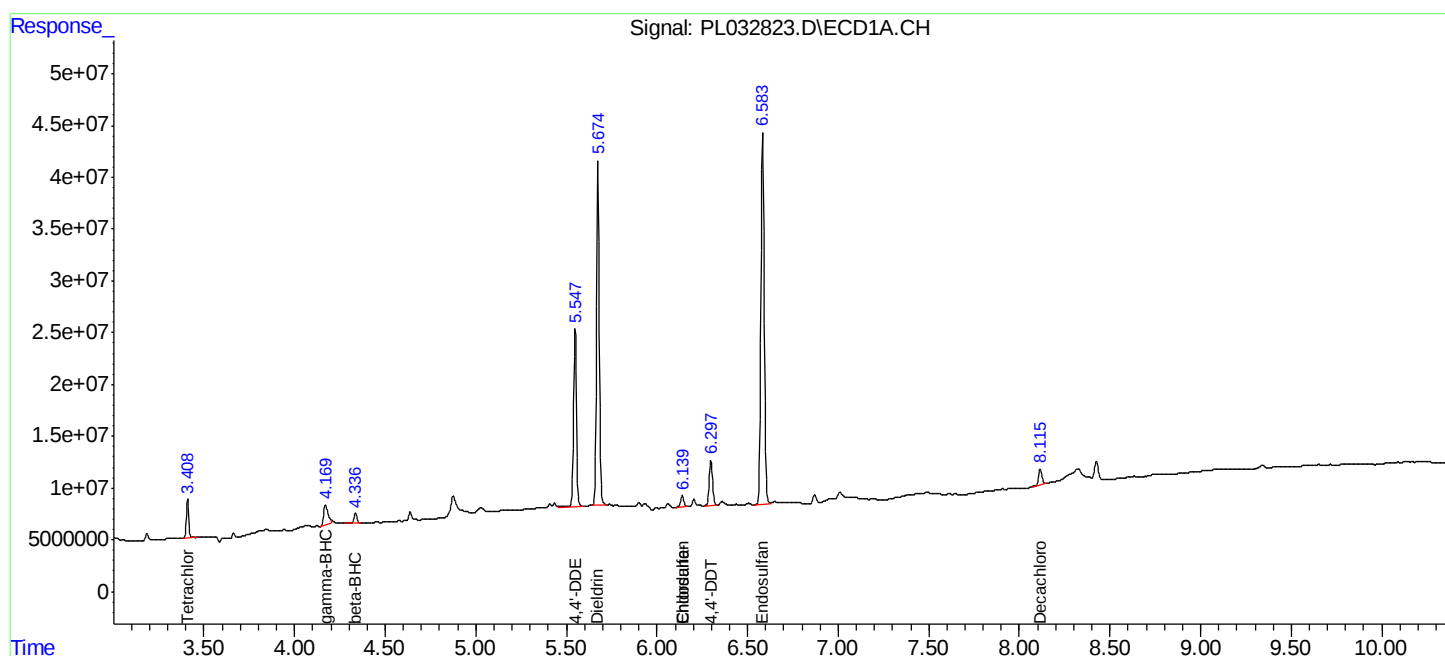


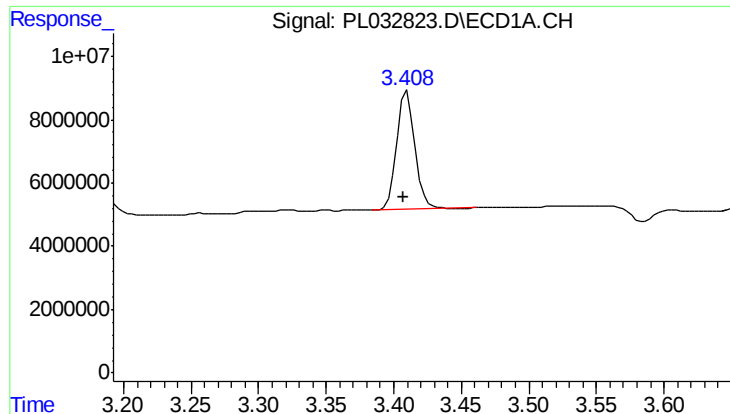

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.002 min
Response: 35269990
Conc: 3.95 ng/ml

Instrument :
FID_E
ClientSampleId :
P-7DL

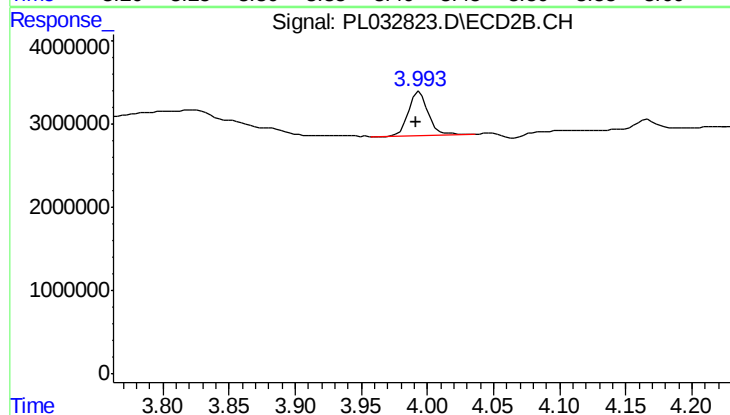


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: 0.003 min
Response: 5286716
Conc: 4.22 ng/ml

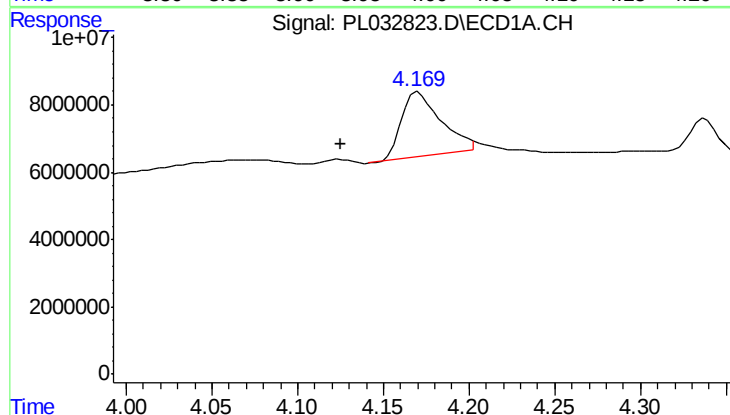


#3 gamma-BHC (Lindane)

R.T.: 4.171 min
Delta R.T.: 0.046 min
Response: 31231007
Conc: 2.42 ng/ml

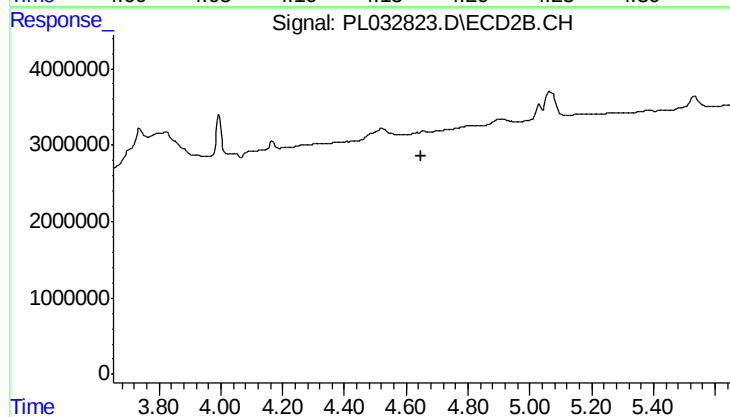

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.650 min
Response: 0
Conc: N.D.

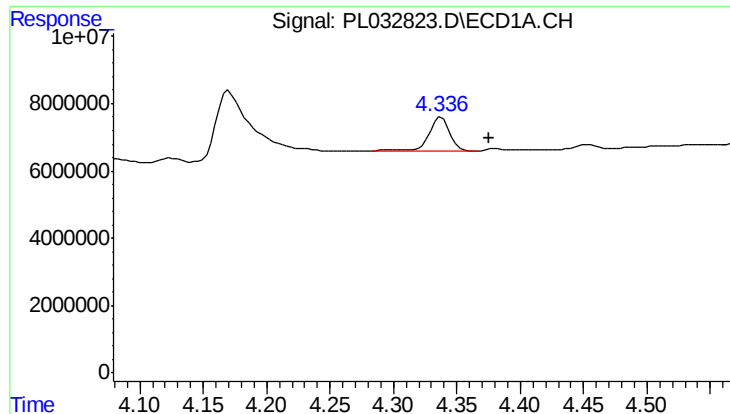

#6 beta-BHC


R.T.: 4.338 min
Delta R.T.: -0.038 min
Response: 11106373
Conc: 1.94 ng/ml

Instrument :
FID_E
ClientSampleId :
P-7DL

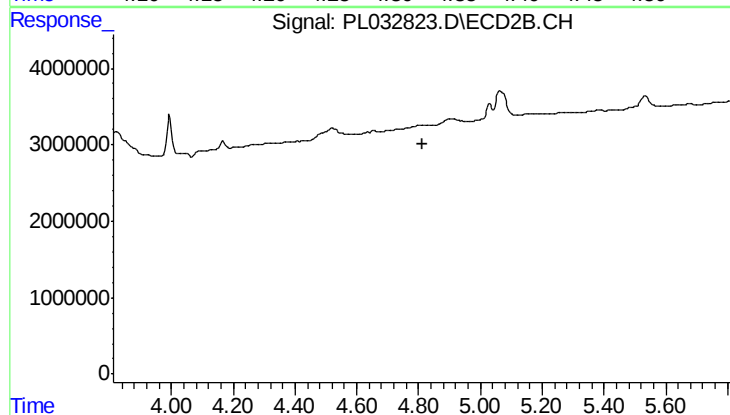


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.811 min
Response: 0
Conc: N.D.

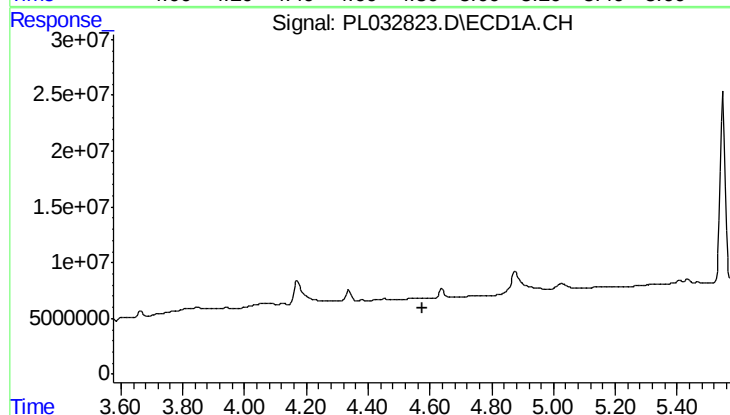


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.574 min
Response: 0
Conc: N.D.

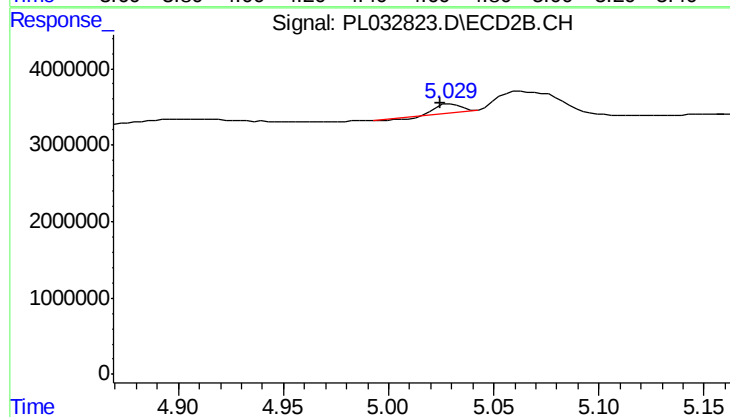

#7 delta-BHC


R.T.: 5.030 min
Delta R.T.: 0.005 min
Response: 762340
Conc: 0.34 ng/ml

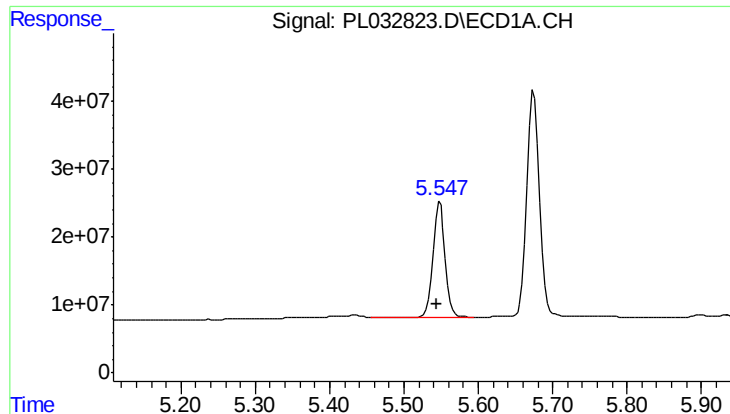

#12 4,4'-DDE


R.T.: 5.548 min
Delta R.T.: 0.004 min
Response: 201599042
Conc: 15.87 ng/ml

Instrument :
FID_E
ClientSampleId :
P-7DL

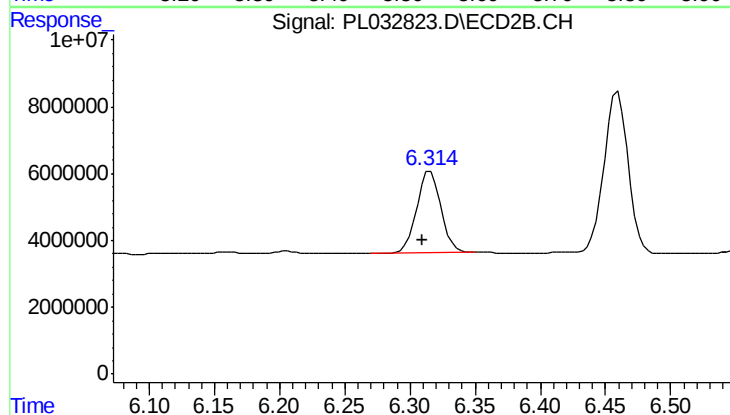


#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: 0.006 min
Response: 31640208
Conc: 16.59 ng/ml

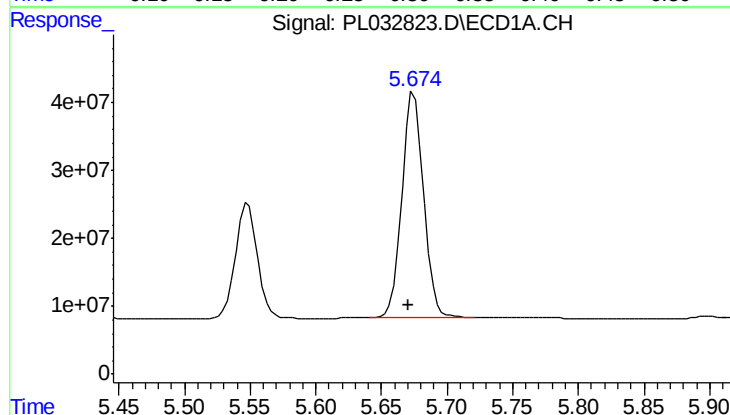


#13 Dieldrin

R.T.: 5.675 min
Delta R.T.: 0.004 min
Response: 382133902
Conc: 29.85 ng/ml

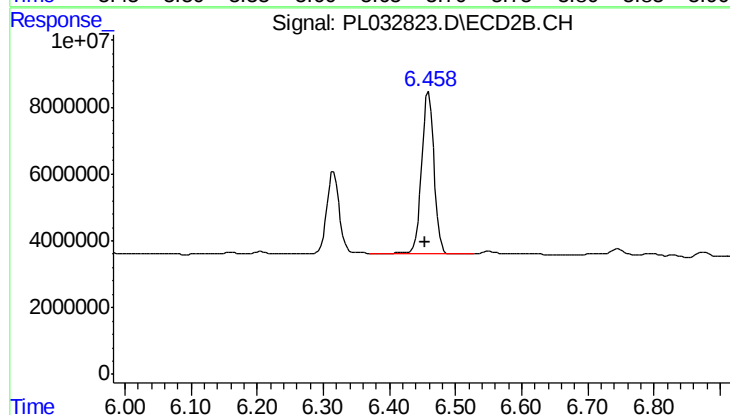

#13 Dieldrin


R.T.: 6.459 min
Delta R.T.: 0.006 min
Response: 62912194
Conc: 32.92 ng/ml

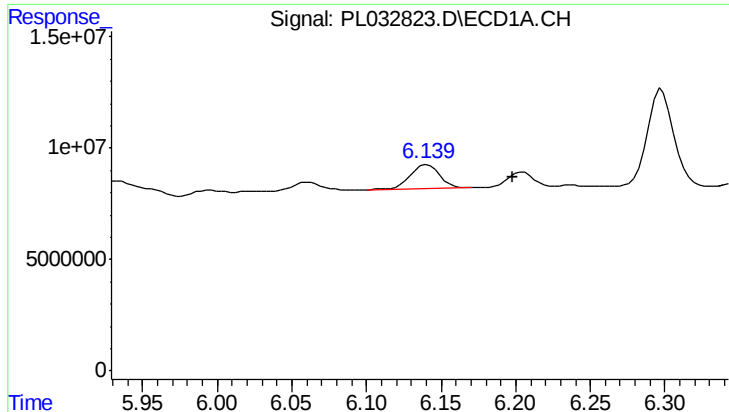

#15 Endosulfan II


R.T.: 6.141 min
Delta R.T.: -0.057 min
Response: 14814993
Conc: 1.26 ng/ml

Instrument :
FID_E
ClientSampleId :
P-7DL

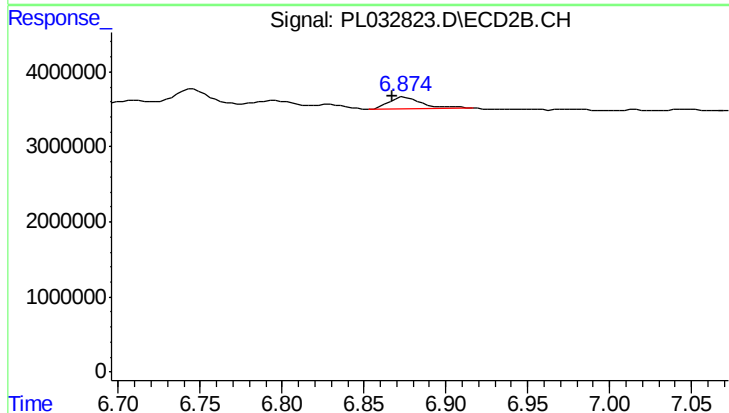


#15 Endosulfan II

R.T.: 6.875 min
Delta R.T.: 0.008 min
Response: 2108089
Conc: 1.20 ng/ml

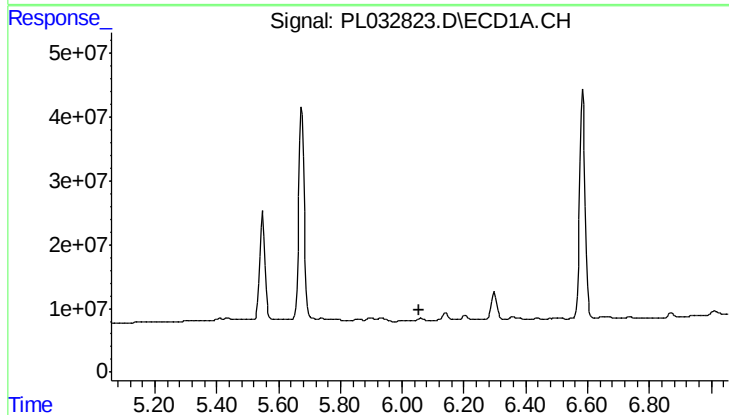


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.057 min
Response: 0
Conc: N.D.

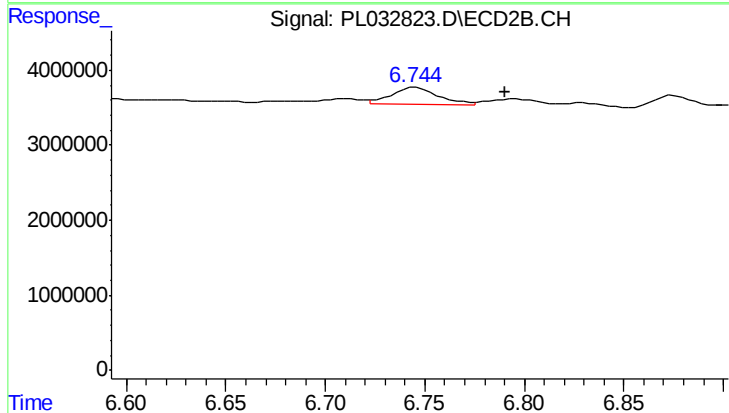

#16 4,4'-DDD


R.T.: 6.745 min
Delta R.T.: -0.045 min
Response: 3781494
Conc: 2.65 ng/ml

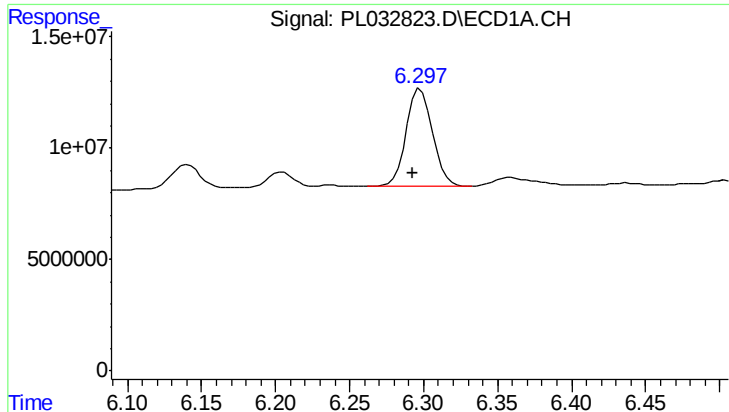

#17 4,4'-DDT


R.T.: 6.298 min
Delta R.T.: 0.005 min
Response: 53978208
Conc: 5.11 ng/ml

Instrument :
FID_E
ClientSampleId :
P-7DL

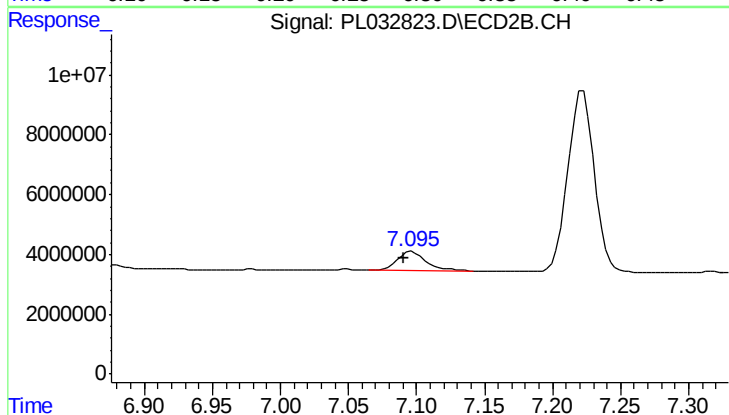


#17 4,4'-DDT

R.T.: 7.097 min
Delta R.T.: 0.006 min
Response: 9435082
Conc: 7.08 ng/ml

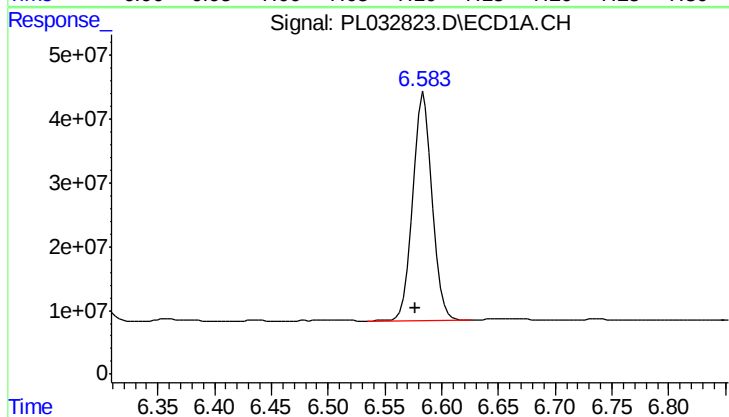


#19 Endosulfan Sulfate

R.T.: 6.584 min
Delta R.T.: 0.007 min
Response: 436812414
Conc: 39.43 ng/ml

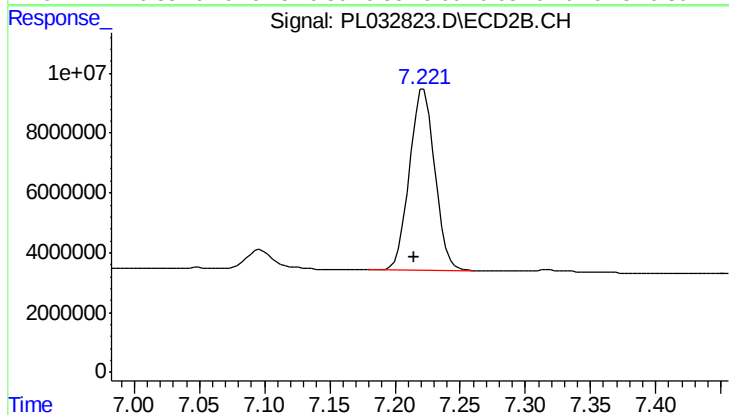

#19 Endosulfan Sulfate

R.T.: 7.222 min
Delta R.T.: 0.007 min
Response: 81683616
Conc: 50.65 ng/ml

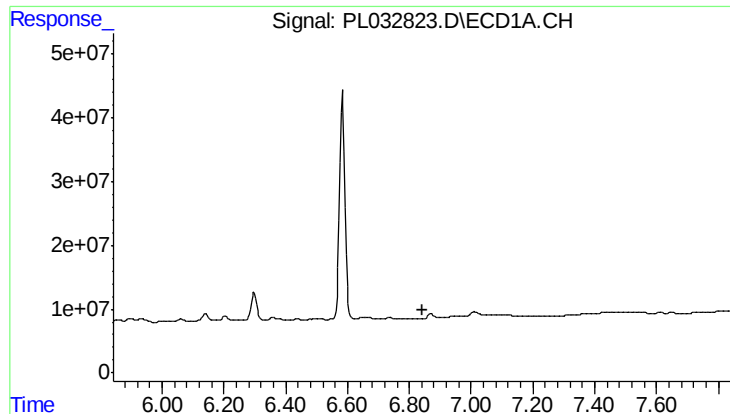


#20 Methoxychlor

+ R.T.: 0.000 min
Exp R.T.: 6.842 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
P-7DL

+

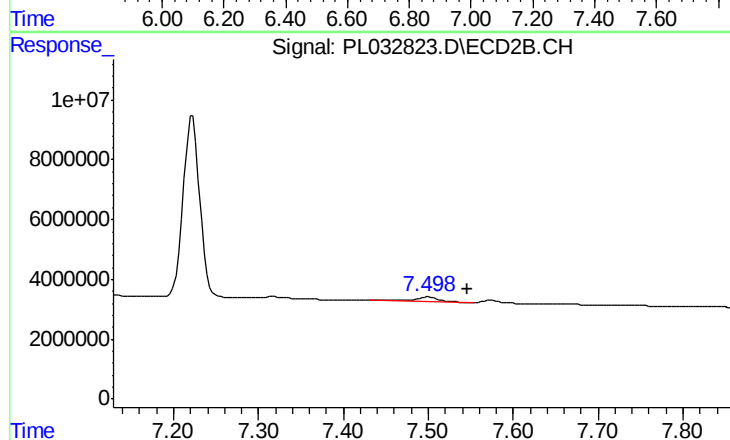

#20 Methoxychlor

R.T.: 7.500 min
Delta R.T.: -0.046 min
Response: 3380237
Conc: 4.15 ng/ml

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.263 min
Response: 0
Conc: N.D.

#27 Chlordane-5

R.T.: 6.141 min
Delta R.T.: -0.065 min
Response: 14814993
Conc: 29.96 ng/ml

Instrument :
FID_E
ClientSampleId :
P-7DL