

Data Path : P:\HPCHEM1\FID E\Data\FE013118\
 Data File : FE026024.D
 Signal(s) : FID1B.CH
 Acq On : 31 Jan 2018 16:41
 Operator : UA/AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Feb 01 03:58:17 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
 Quant Title :
 QLast Update : Tue Jan 30 11:45:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.760	8071592	50.888 ug/ml
Target Compounds			
2) N-DECANE	4.510	8265560	52.303 ug/ml
3) N-DODECANE	6.526	9229642	53.980 ug/ml
4) N-TETRADECANE	8.321	9782435	52.197 ug/ml
5) N-HEXADECANE	9.919	9753043	49.115 ug/ml
6) N-OCTADECANE	11.359	9461066	44.828 ug/ml
7) N-EICOSANE	12.666	8671276	41.976 ug/ml
8) N-DOCOSANE	13.862	7915810	40.476 ug/ml
10) N-TETRACOSANE	14.964	7443322	40.797 ug/ml
11) N-HEXACOSANE	15.983	7339722	44.838 ug/ml
12) N-OCTACOSANE	16.931	7654505	50.423 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE013118\
Data File : FE026024.D
Signal(s) : FID1B.CH
Acq On : 31 Jan 2018 16:41
Operator : UA/AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Sample.e
Quant Time: Feb 01 03:58:17 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Tue Jan 30 11:45:47 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

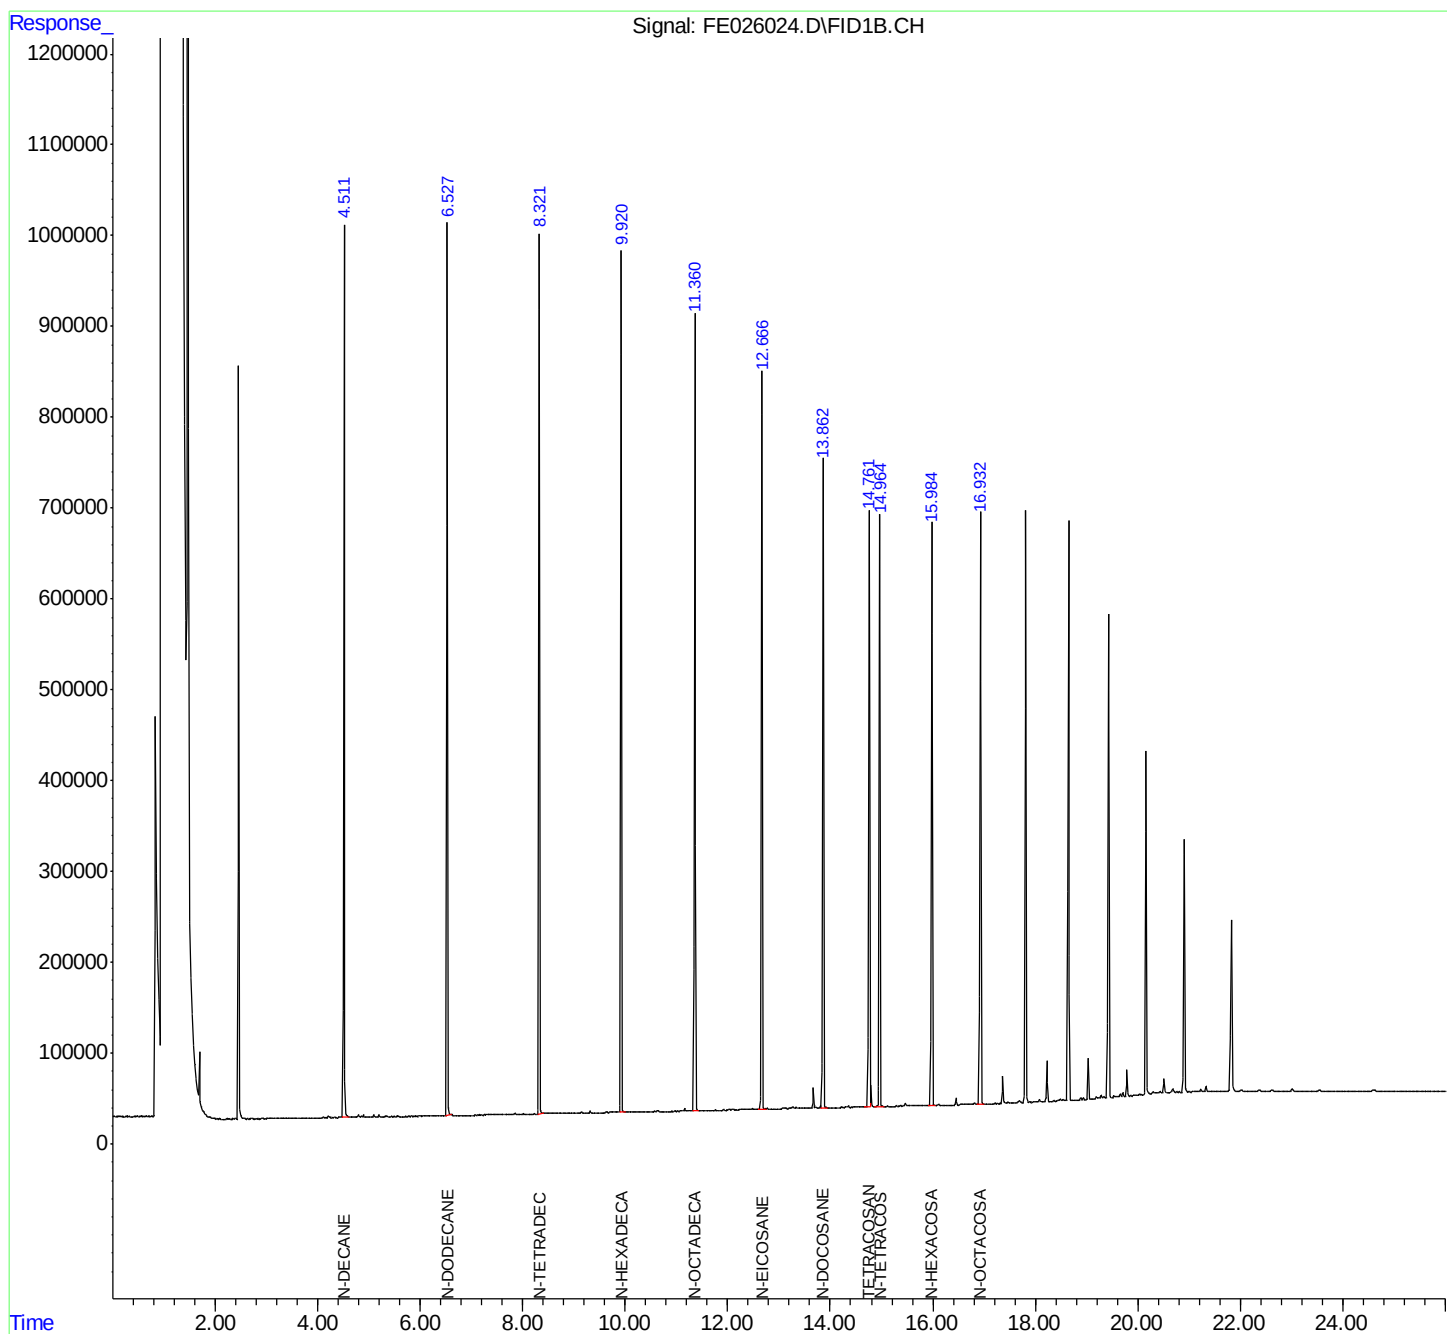


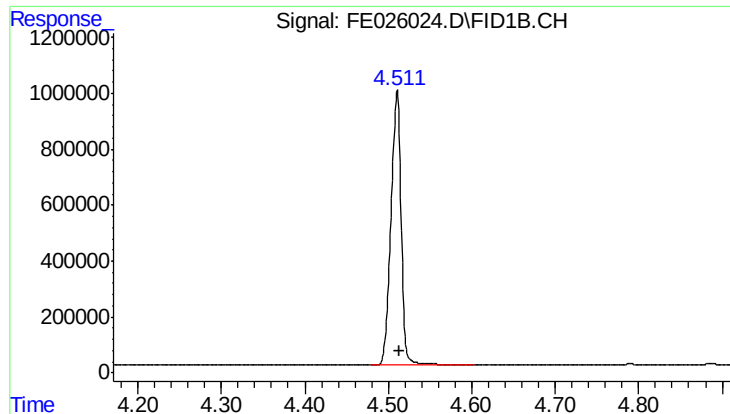

#2 N-DECANE


R.T.: 4.510 min
Delta R.T.: -0.004 min
Response: 8265560
Conc: 52.30 ug/ml

Instrument :
FID_E
ClientSampleId :

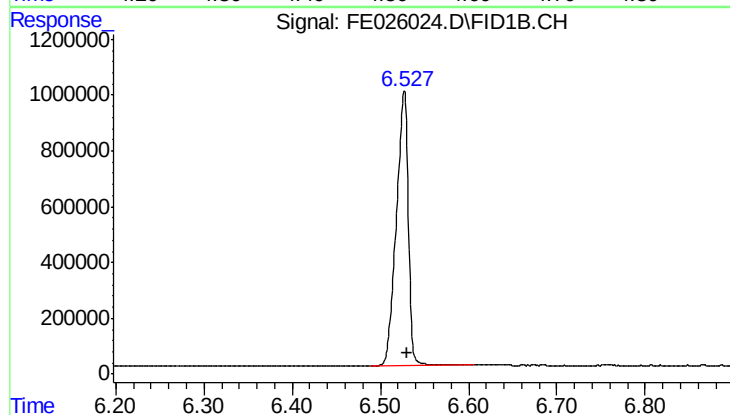


#3 N-DODECANE

R.T.: 6.526 min
Delta R.T.: -0.004 min
Response: 9229642
Conc: 53.98 ug/ml

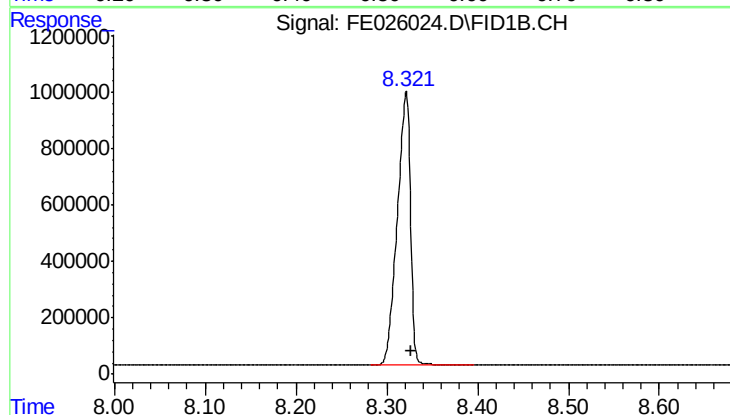


#4 N-TETRADECANE

R.T.: 8.321 min
Delta R.T.: -0.005 min
Response: 9782435
Conc: 52.20 ug/ml

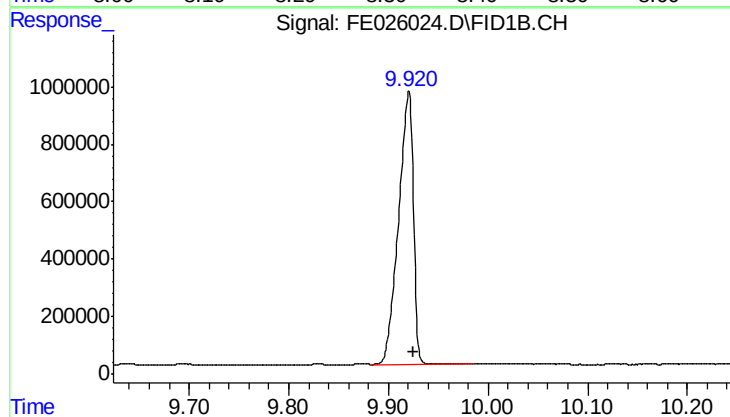

#5 N-HEXADECANE


R.T.: 9.919 min
Delta R.T.: -0.006 min
Response: 9753043
Conc: 49.11 ug/ml

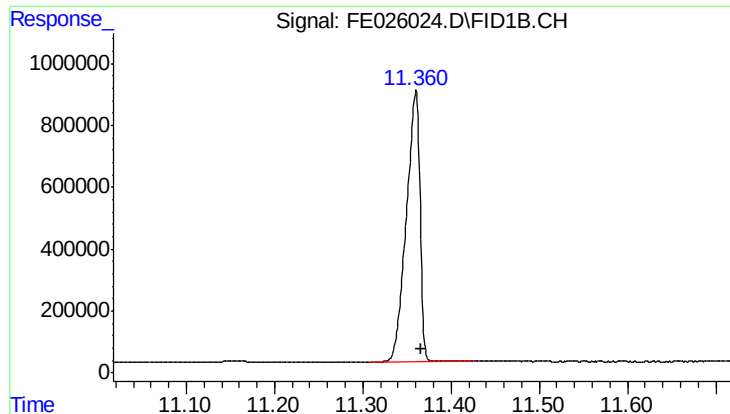

#6 N-OCTADECANE


R.T.: 11.359 min
Delta R.T.: -0.008 min
Response: 9461066
Conc: 44.83 ug/ml

Instrument :
FID_E
ClientSampleId :

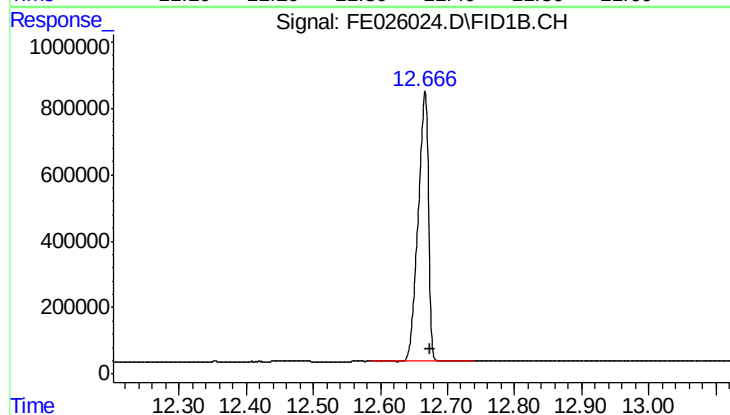


#7 N-EICOSANE

R.T.: 12.666 min
Delta R.T.: -0.008 min
Response: 8671276
Conc: 41.98 ug/ml

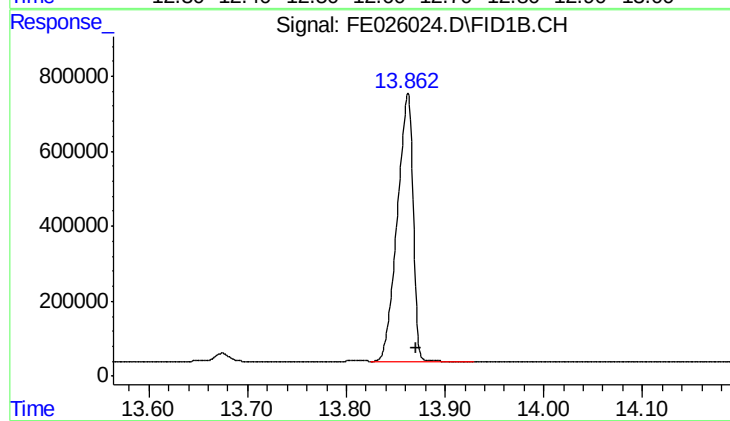


#8 N-DOCOSANE

R.T.: 13.862 min
Delta R.T.: -0.009 min
Response: 7915810
Conc: 40.48 ug/ml

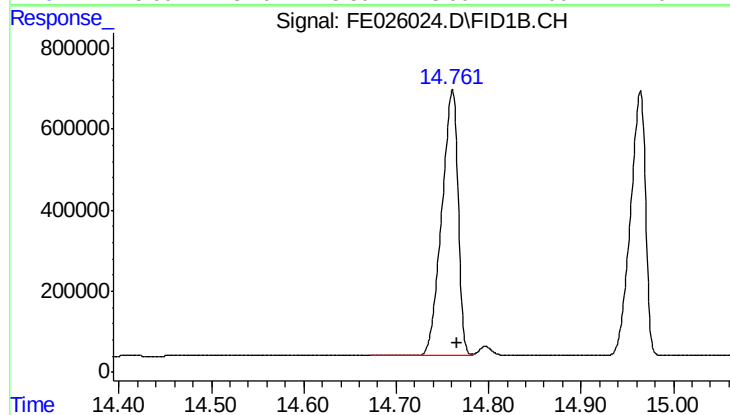

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.760 min
Delta R.T.: -0.005 min
Response: 8071592
Conc: 50.89 ug/ml

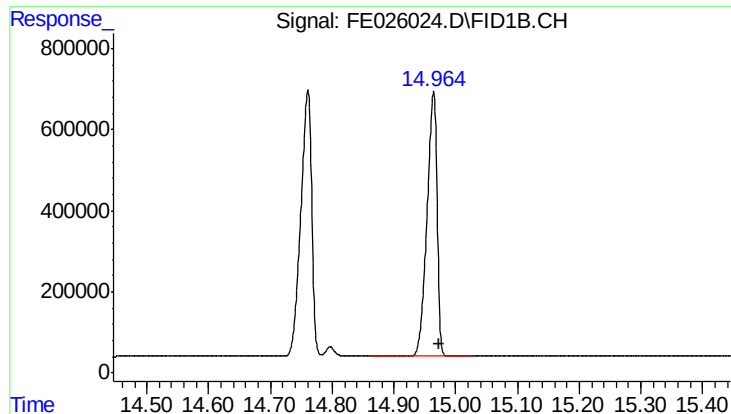

#10 N-TETRACOSANE


R.T.: 14.964 min
Delta R.T.: -0.009 min
Response: 7443322
Conc: 40.80 ug/ml

Instrument :
FID_E
ClientSampleId :

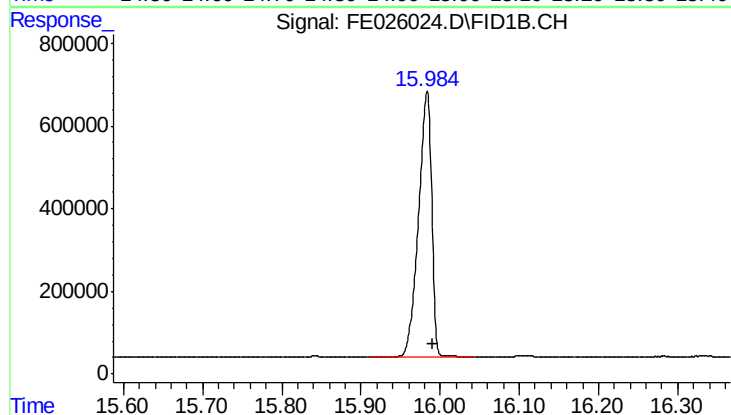

#11 N-HEXACOSANE

R.T.: 15.983 min
Delta R.T.: -0.008 min
Response: 7339722
Conc: 44.84 ug/ml

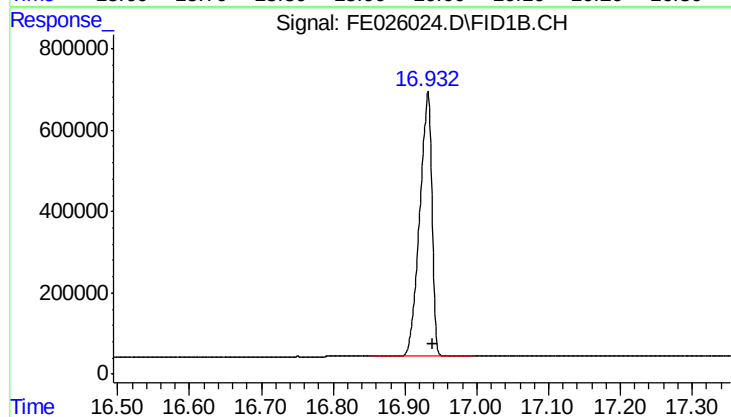

#12 N-OCTACOSANE

R.T.: 16.931 min
Delta R.T.: -0.008 min
Response: 7654505
Conc: 50.42 ug/ml