

Data Path : P:\HPCHEM1\FID E\Data\FE013118\
 Data File : FE026058.D
 Signal(s) : FID1B.CH
 Acq On : 01 Feb 2018 12:41
 Operator : UA/AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Feb 01 13:24:04 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
 Quant Title :
 QLast Update : Tue Jan 30 11:45:47 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.762	8446326	53.250 ug/ml
Target Compounds			
2) N-DECANE	4.510	8884197	56.218 ug/ml
3) N-DODECANE	6.525	9661507	56.506 ug/ml
4) N-TETRADECANE	8.319	9888670	52.764 ug/ml
5) N-HEXADECANE	9.919	9522795	47.955 ug/ml
6) N-OCTADECANE	11.359	8892873	42.136 ug/ml
7) N-EICOSANE	12.666	8141751	39.413 ug/ml
8) N-DOCOSANE	13.863	7777272	39.768 ug/ml
10) N-TETRACOSANE	14.966	7870630	43.139 ug/ml
11) N-HEXACOSANE	15.985	8048958	49.171 ug/ml
12) N-OCTACOSANE	16.935	8294768	54.641 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE013118\
Data File : FE026058.D
Signal(s) : FID1B.CH
Acq On : 01 Feb 2018 12:41
Operator : UA/AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Sample.e
Quant Time: Feb 01 13:24:04 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE012518.M
Quant Title :
QLast Update : Tue Jan 30 11:45:47 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

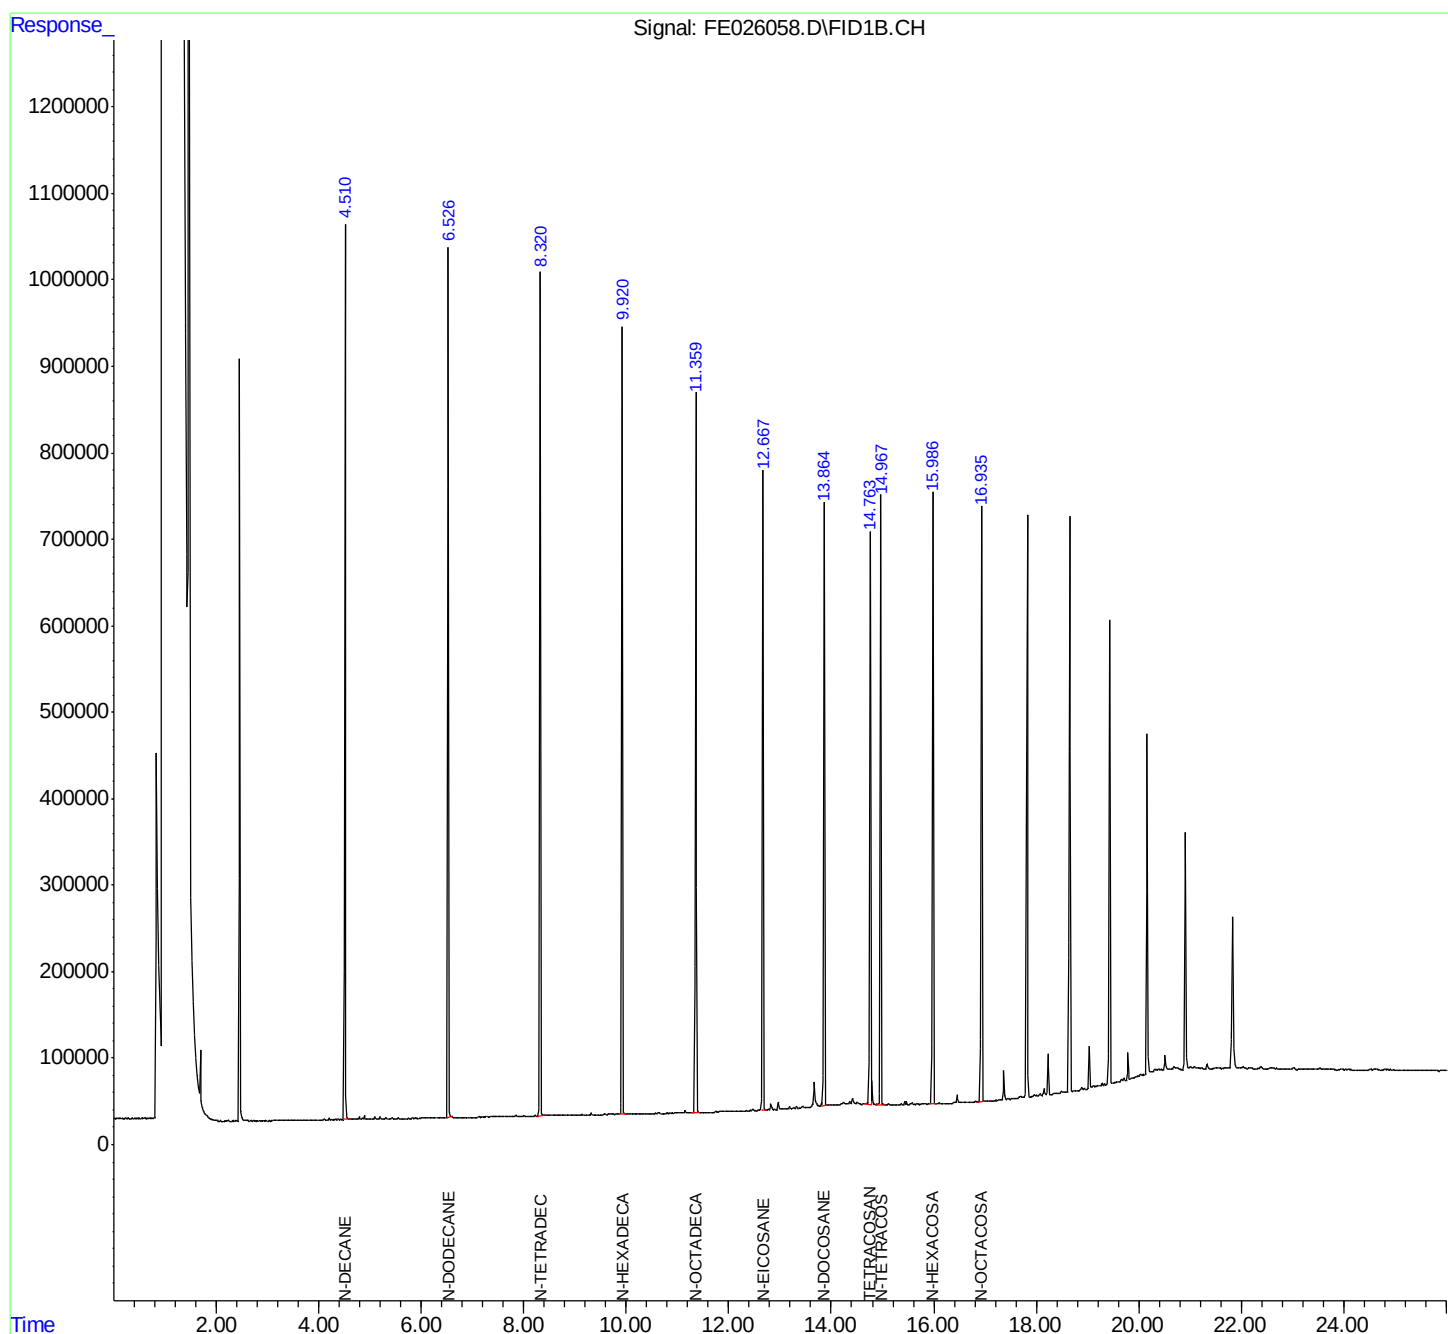


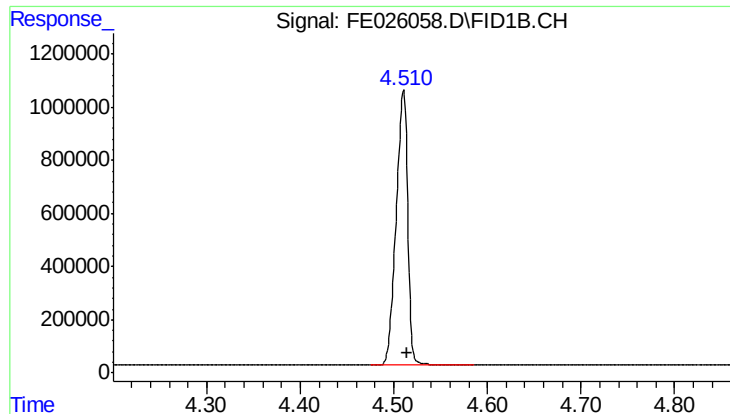

#2 N-DECANE


R.T.: 4.510 min
Delta R.T.: -0.004 min
Response: 8884197
Conc: 56.22 ug/ml

Instrument :
FID_E
ClientSampleId :

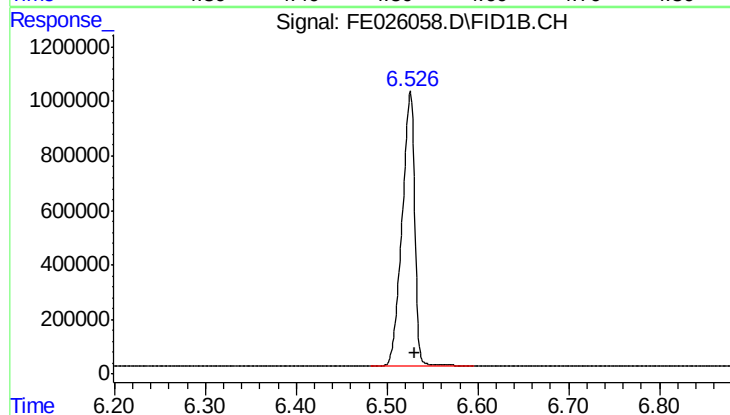


#3 N-DODECANE

R.T.: 6.525 min
Delta R.T.: -0.005 min
Response: 9661507
Conc: 56.51 ug/ml

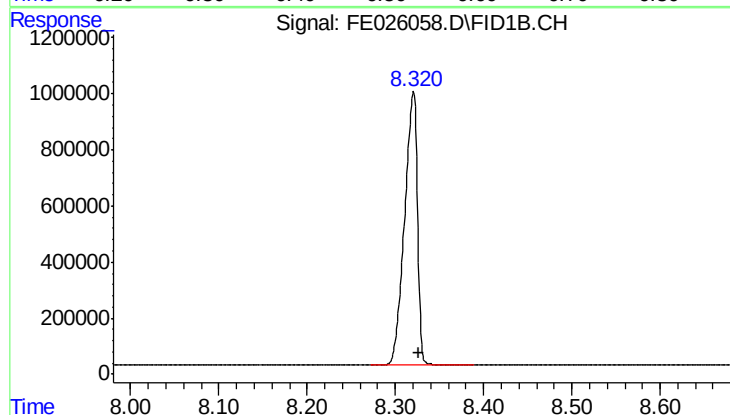


#4 N-TETRADECANE

R.T.: 8.319 min
Delta R.T.: -0.007 min
Response: 9888670
Conc: 52.76 ug/ml

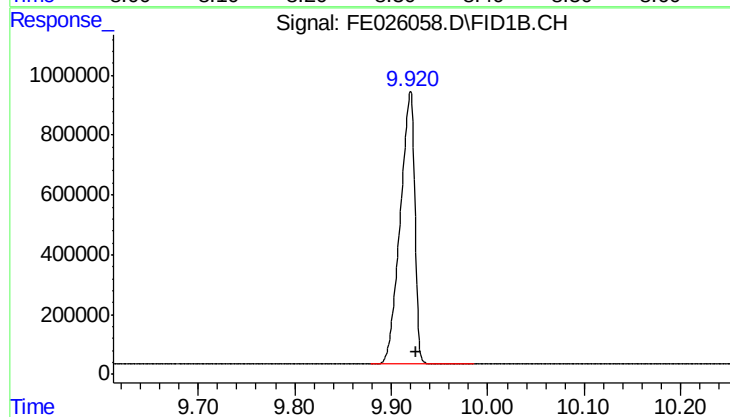

#5 N-HEXADECANE


R.T.: 9.919 min
Delta R.T.: -0.007 min
Response: 9522795
Conc: 47.96 ug/ml

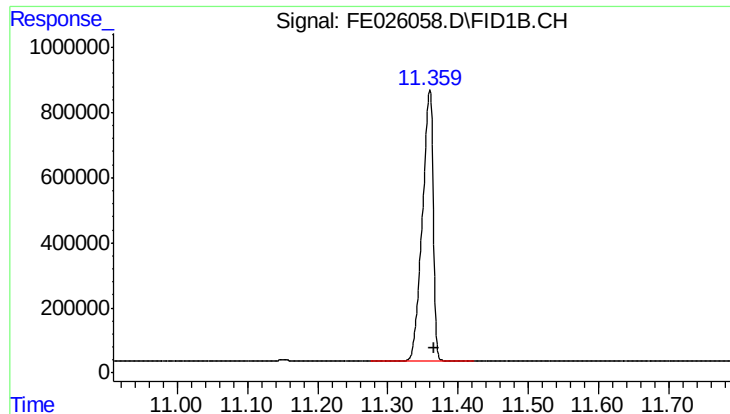

#6 N-OCTADECANE


R.T.: 11.359 min
Delta R.T.: -0.008 min
Response: 8892873
Conc: 42.14 ug/ml

Instrument :
FID_E
ClientSampleId :

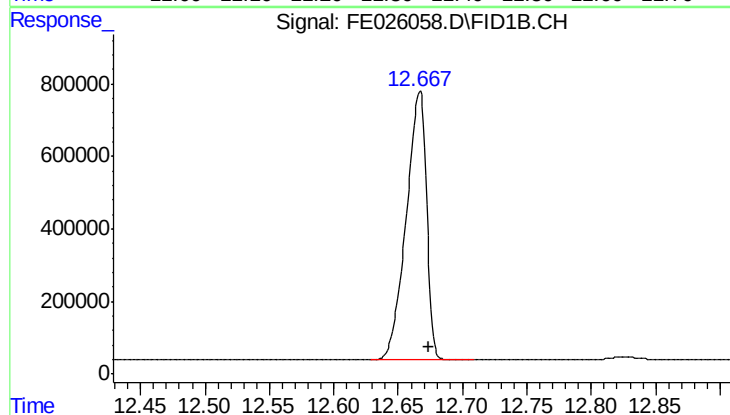


#7 N-EICOSANE

R.T.: 12.666 min
Delta R.T.: -0.008 min
Response: 8141751
Conc: 39.41 ug/ml

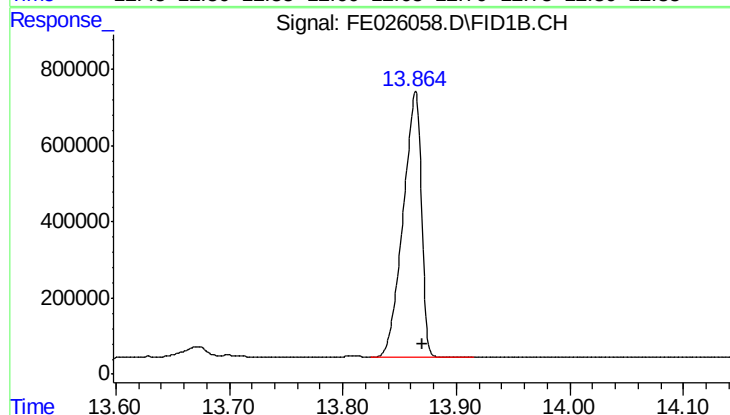


#8 N-DOCOSANE

R.T.: 13.863 min
Delta R.T.: -0.007 min
Response: 7777272
Conc: 39.77 ug/ml

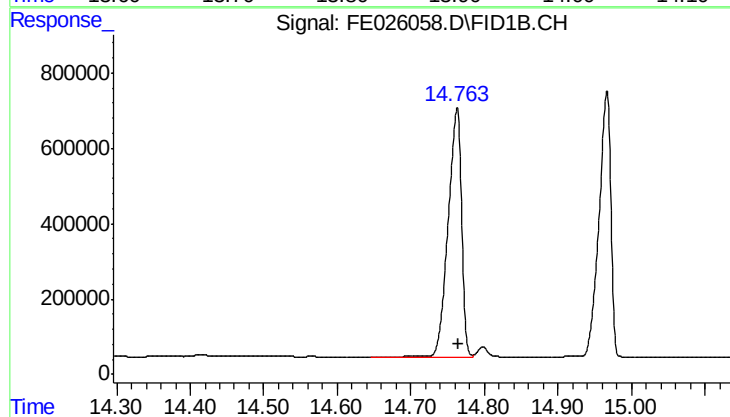

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.762 min
Delta R.T.: -0.003 min
Response: 8446326
Conc: 53.25 ug/ml

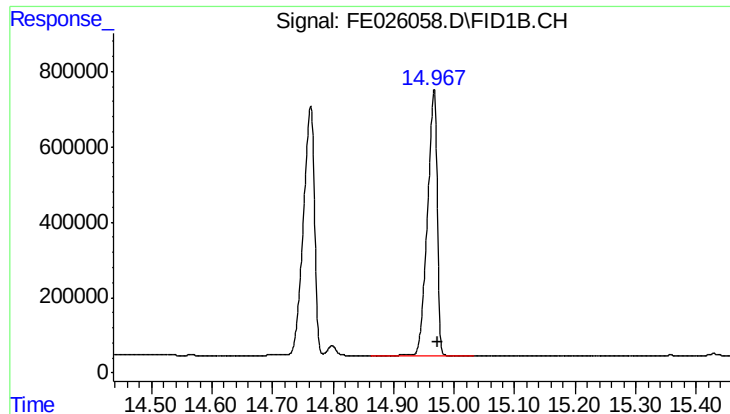

#10 N-TETRACOSANE


R.T.: 14.966 min
Delta R.T.: -0.007 min
Response: 7870630
Conc: 43.14 ug/ml

Instrument :
FID_E
ClientSampleId :

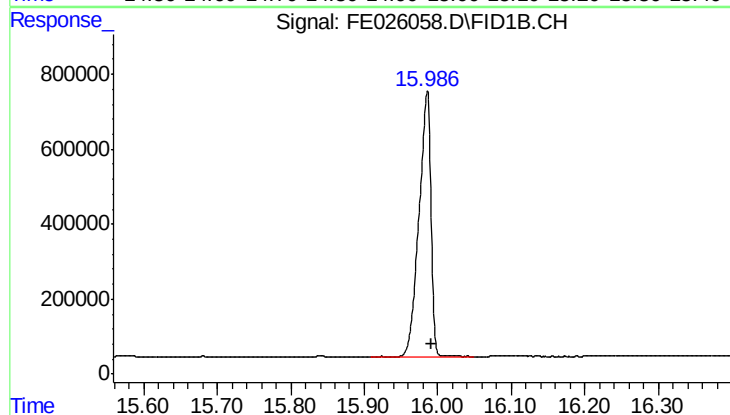

#11 N-HEXACOSANE

R.T.: 15.985 min
Delta R.T.: -0.006 min
Response: 8048958
Conc: 49.17 ug/ml

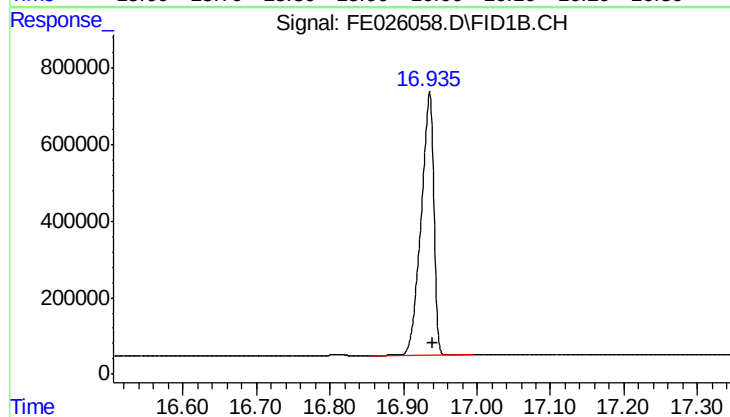

#12 N-OCTACOSANE

R.T.: 16.935 min
Delta R.T.: -0.004 min
Response: 8294768
Conc: 54.64 ug/ml