

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033022\
 Data File : PS018837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 18:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 03:02:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033022.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 02:39:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.811	731.9E6	327.7E6	247.606	479.975 #
Target Compounds							
9) T	2,4-D	8.424f	0.000	11355203	0	2.886	N.D. #
11) T	2,4,5-TP ...	0.000	8.661	0	5650126	N.D.	1.287
12) T	2,4,5-T	9.543f	0.000	13675753	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.506f	0	36085621	N.D.	67.390
14) T	DINOSEB	11.207	0.000	34851084	0	2.108	N.D. #
15) T	Picloram	0.000	10.948f	0	424142	N.D.	<MDL
16) T	DCPA	11.476	0.000	4458498	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033022\
Data File : PS018837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 18:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 03:02:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033022.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 02:39:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

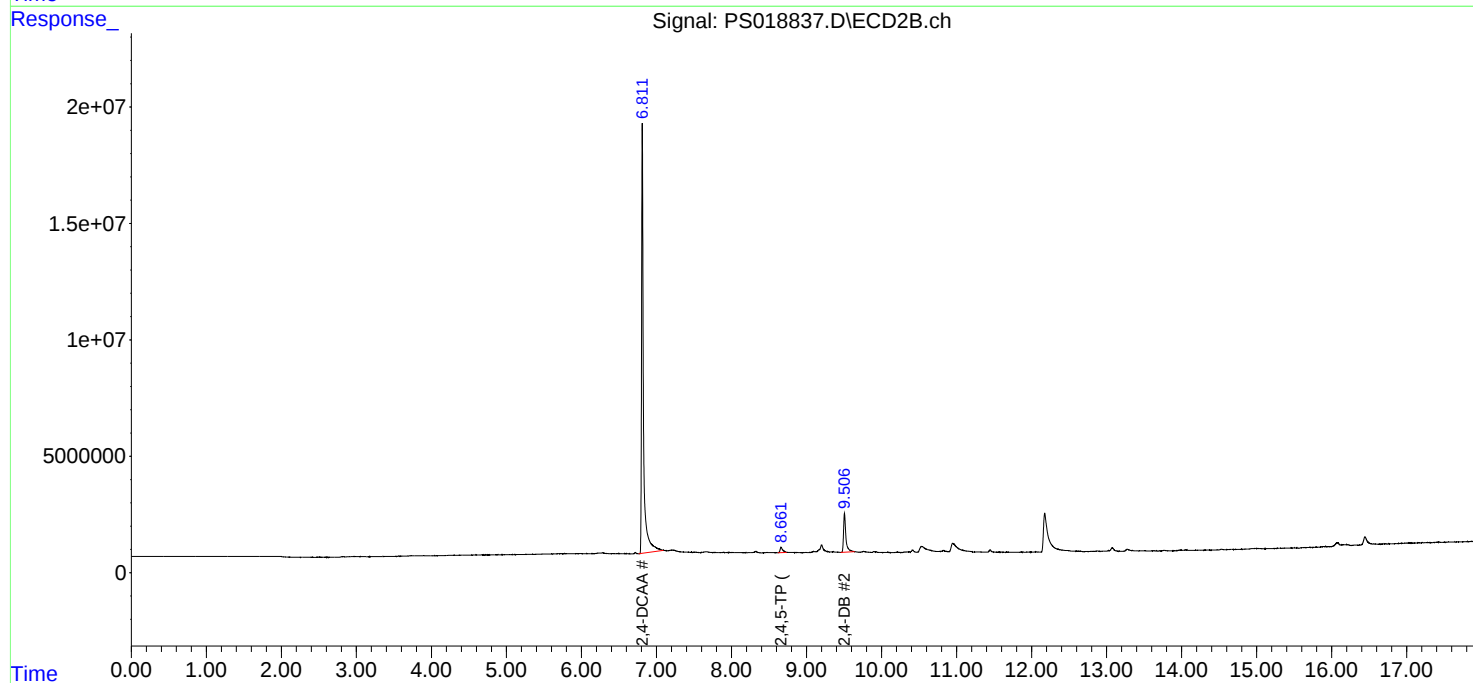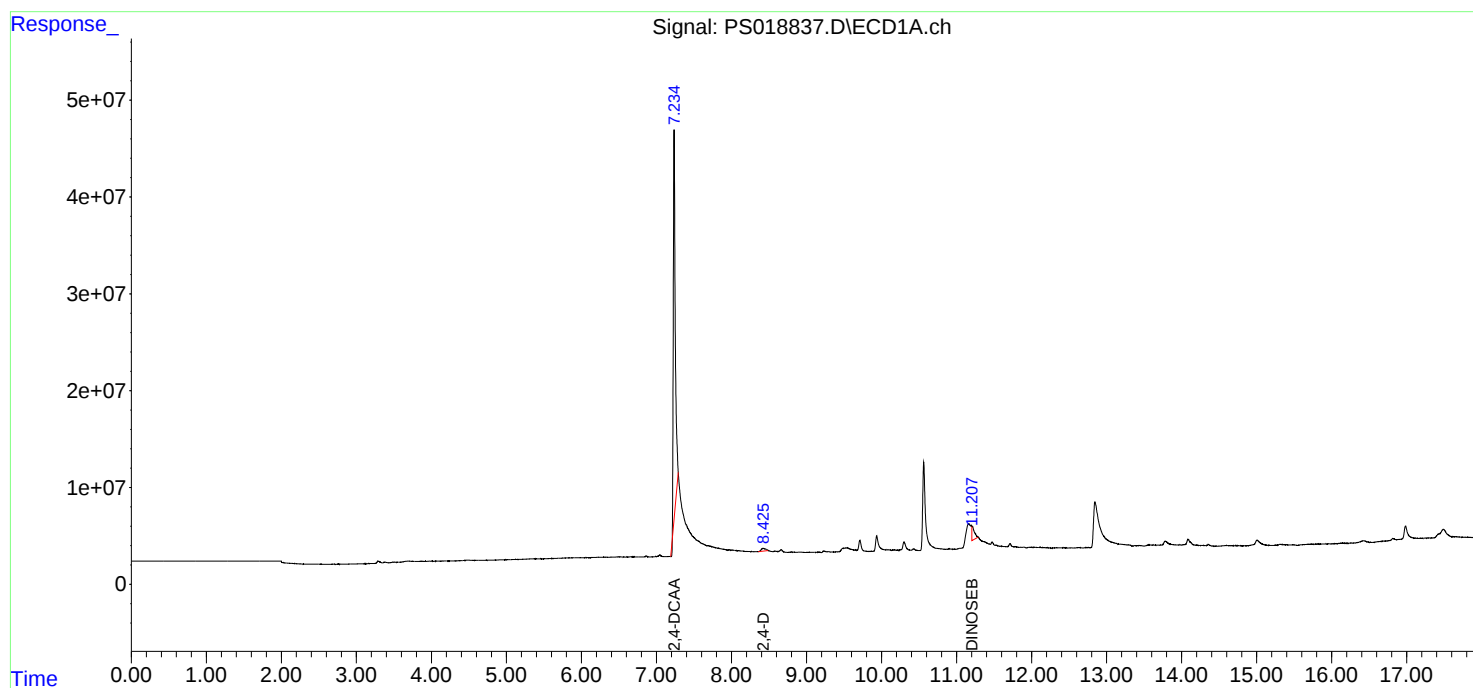


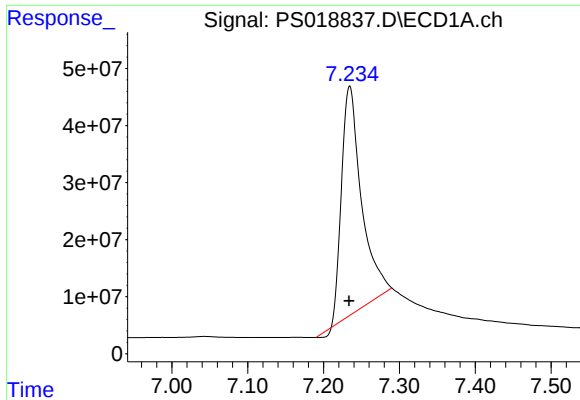

#4 2,4-DCAA


R.T.: 7.235 min
Delta R.T.: 0.001 min
Response: 731945364
Conc: 247.61 ng/ml

Instrument :
FID_E
ClientSampleId :

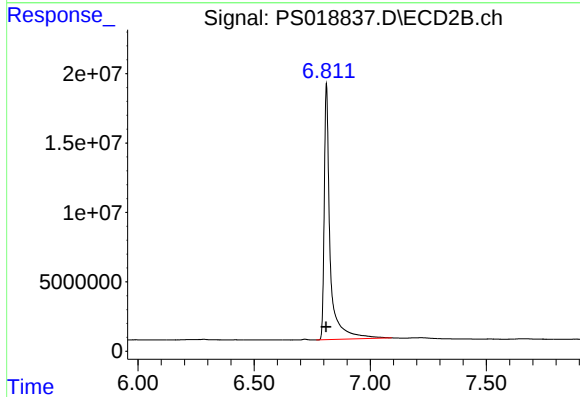


#4 2,4-DCAA

R.T.: 6.811 min
Delta R.T.: 0.000 min
Response: 327737536
Conc: 479.97 ng/ml

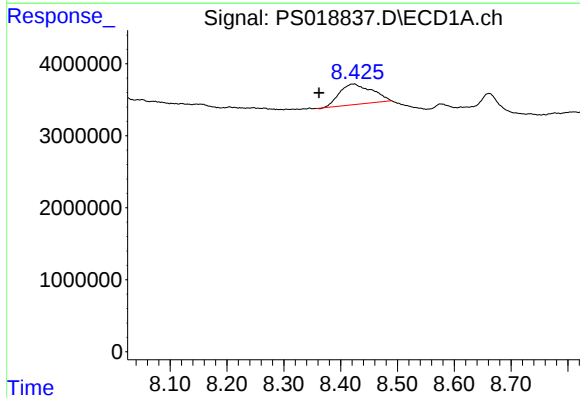


#9 2,4-D

R.T.: 8.424 min
Delta R.T.: 0.063 min
Response: 11355203
Conc: 2.89 ng/ml

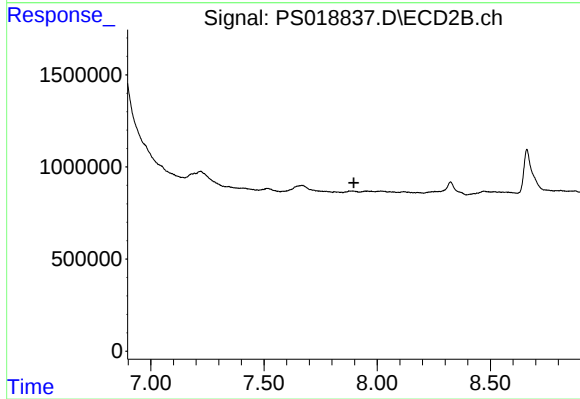

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.897 min
Response: 0
Conc: N.D.

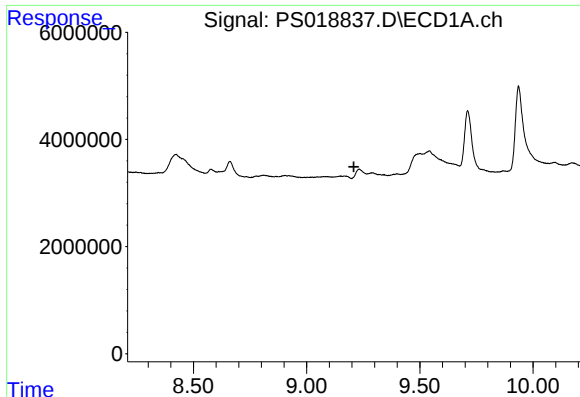

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.209 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

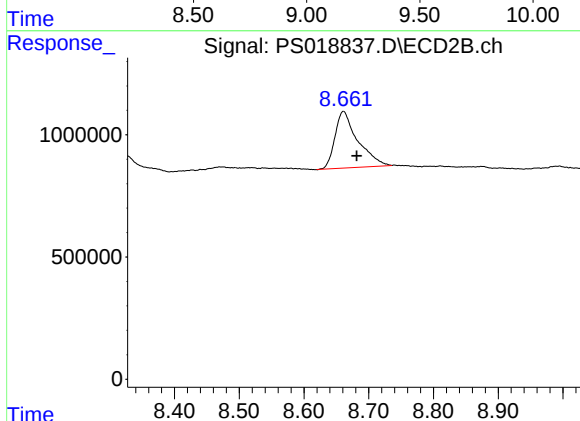


#11 2,4,5-TP (SILVEX)

R.T.: 8.661 min
Delta R.T.: -0.020 min
Response: 5650126
Conc: 1.29 ng/ml

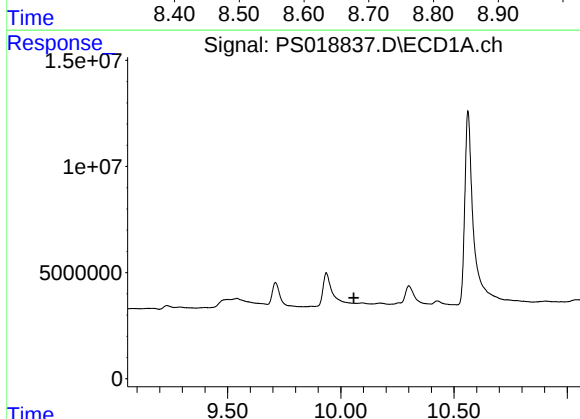


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.058 min
Response: 0
Conc: N.D.

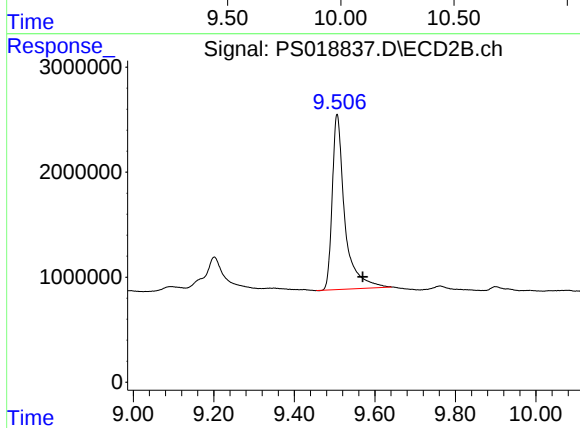

#13 2,4-DB


R.T.: 9.506 min
Delta R.T.: -0.064 min
Response: 36085621
Conc: 67.39 ng/ml

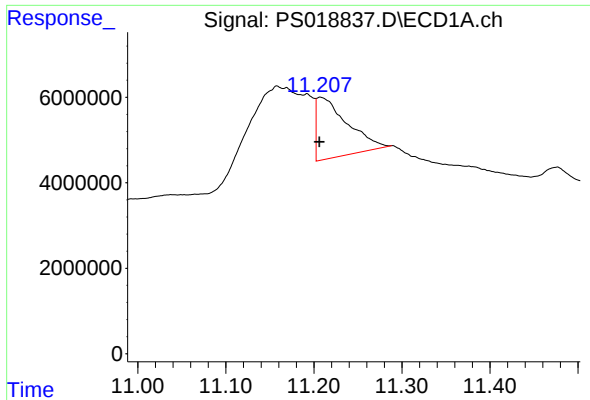

#14 DINOSEB

R.T.: 11.207 min
Delta R.T.: 0.001 min
Response: 34851084
Conc: 2.11 ng/ml

Instrument :
FID_E
ClientSampleId :

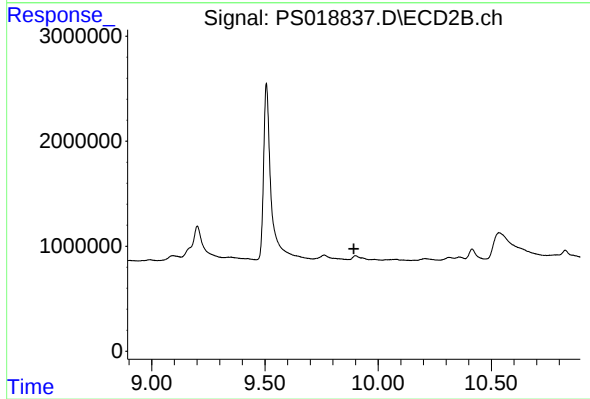

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.893 min
Response: 0
Conc: N.D.