

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033022\
 Data File : PS018841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Mar 2022 19:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 31 03:03:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033022.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 02:39:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.809	1250.0E6	339.1E6	422.848	496.596
Target Compounds							
7) T	MCPA	7.685f	0.000	2920937	0	<MDL	N.D. #
9) T	2,4-D	8.420f	0.000	6883194	0	1.750	N.D. #
11) T	2,4,5-TP ...	9.220	8.642	20621904	15416414	1.015	3.511 #
12) T	2,4,5-T	9.496	0.000	14781813	0	<MDL	N.D. #
13) T	2,4-DB	10.085	0.000	4153640	0	1.443	N.D. #
15) T	Picloram	11.011f	10.899	6759437	18283177	<MDL	4.331 #
16) T	DCPA	11.475	0.000	1892666	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS033022\
Data File : PS018841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Mar 2022 19:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 31 03:03:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033022.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 02:39:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

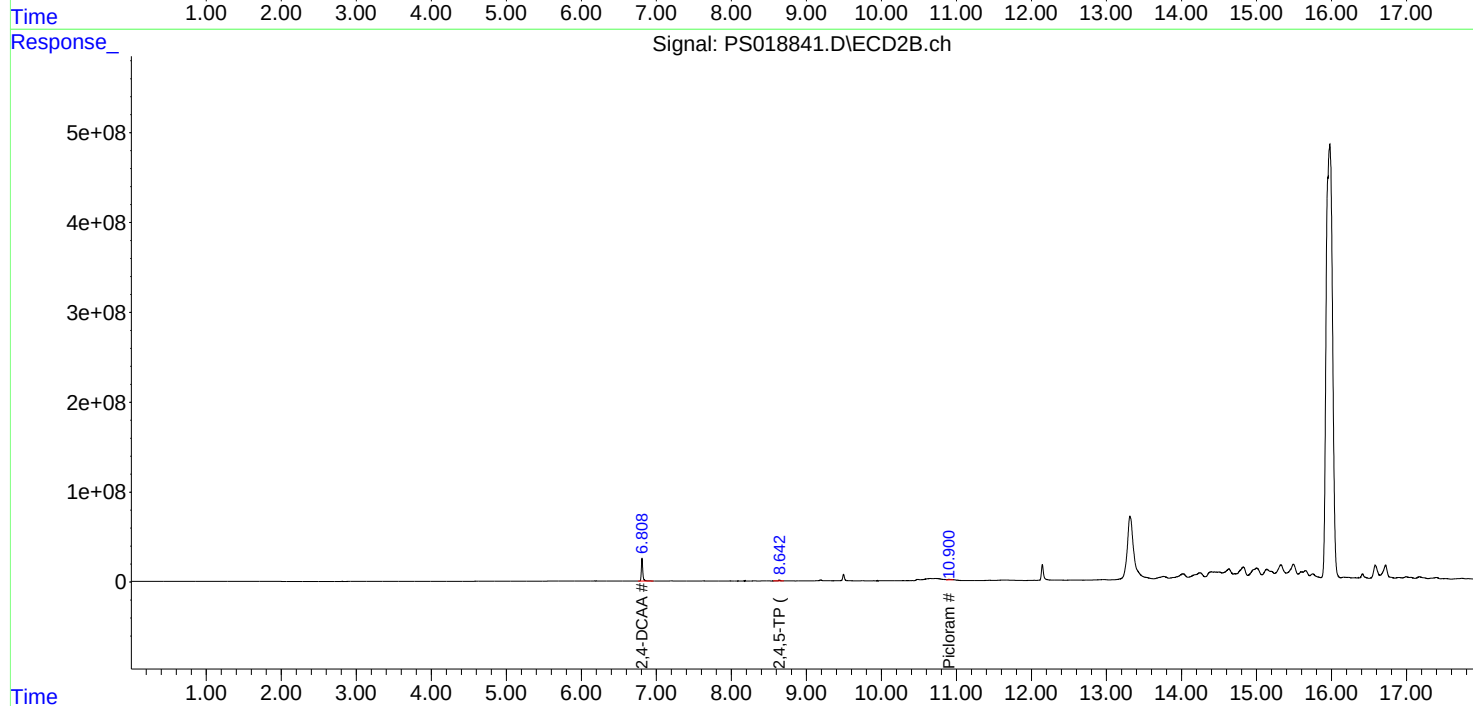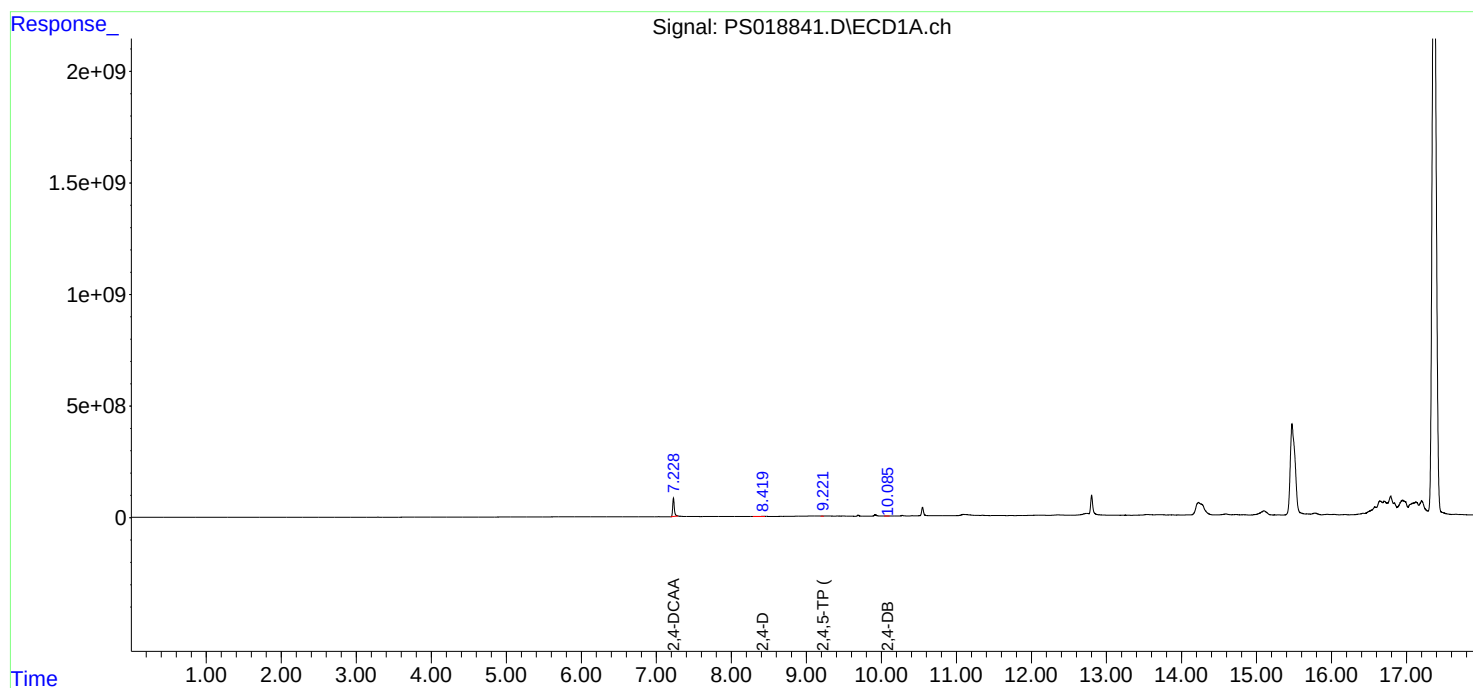


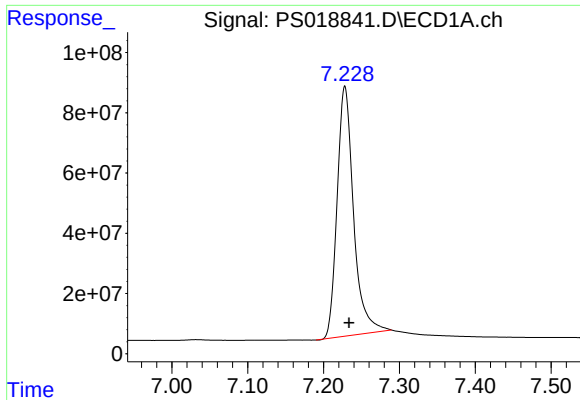

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: -0.005 min
Response: 1249975524
Conc: 422.85 ng/ml

Instrument :
FID_E
ClientSampleId :

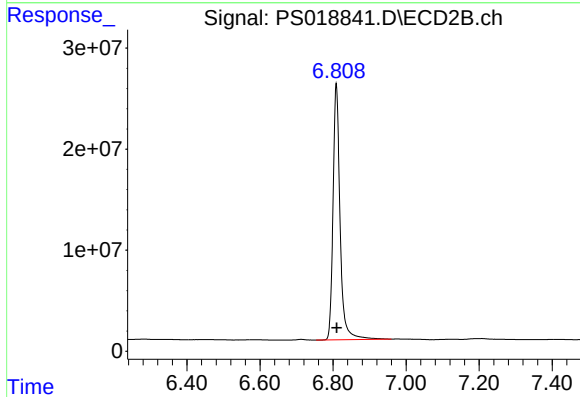


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.001 min
Response: 339086687
Conc: 496.60 ng/ml

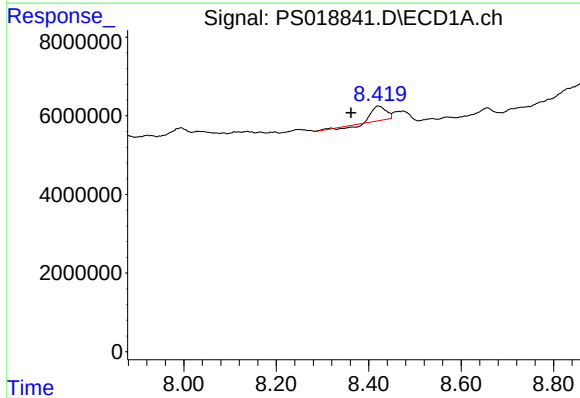


#9 2,4-D

R.T.: 8.420 min
Delta R.T.: 0.058 min
Response: 6883194
Conc: 1.75 ng/ml

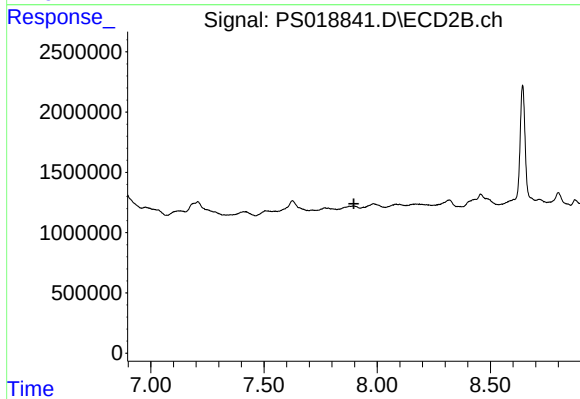

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.897 min
Response: 0
Conc: N.D.

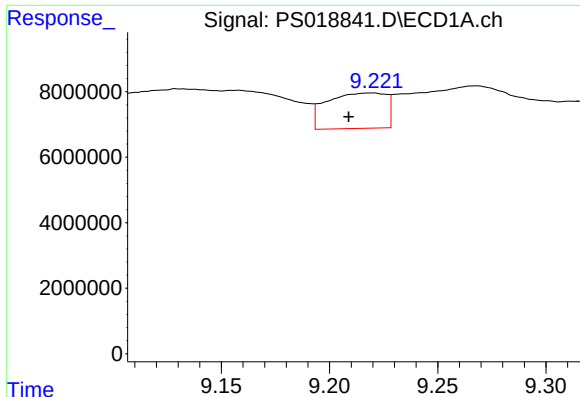

#11 2,4,5-TP (SILVEX)


R.T.: 9.220 min
Delta R.T.: 0.011 min
Response: 20621904
Conc: 1.02 ng/ml

Instrument :
FID_E
ClientSampleId :

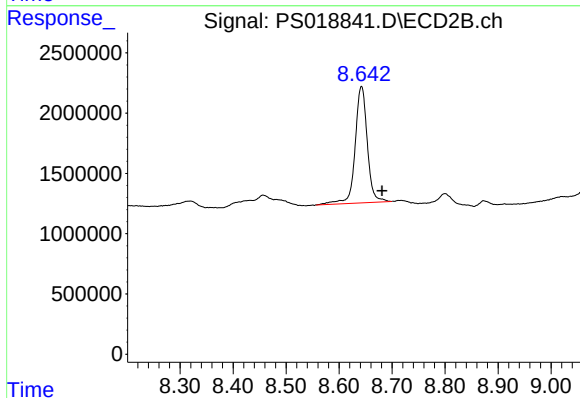


#11 2,4,5-TP (SILVEX)

R.T.: 8.642 min
Delta R.T.: -0.039 min
Response: 15416414
Conc: 3.51 ng/ml

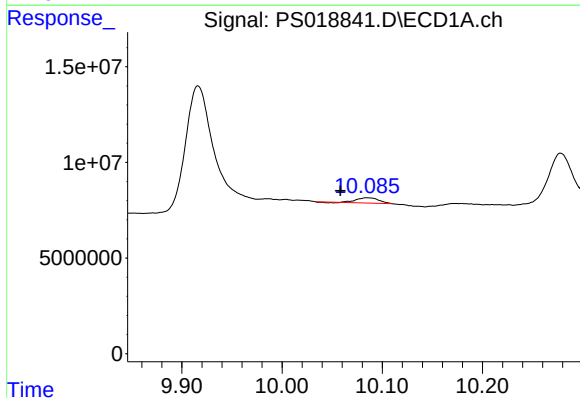


#13 2,4-DB

R.T.: 10.085 min
Delta R.T.: 0.027 min
Response: 4153640
Conc: 1.44 ng/ml

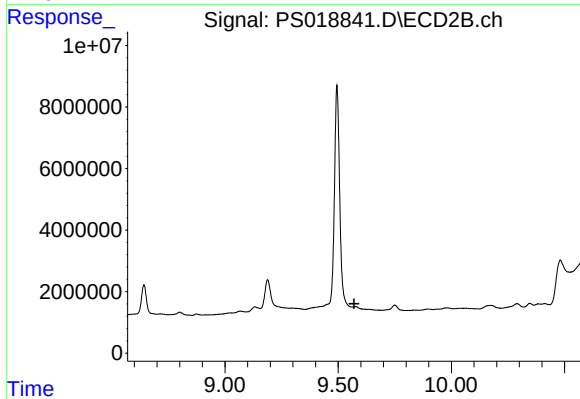

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

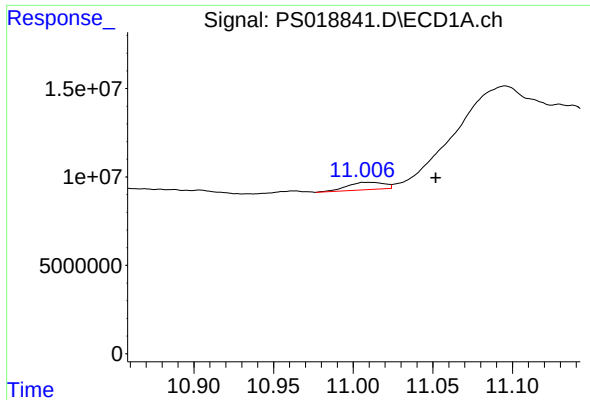

#15 Picloram

R.T.: 11.011 min
Delta R.T.: -0.041 min
Response: 6759437
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

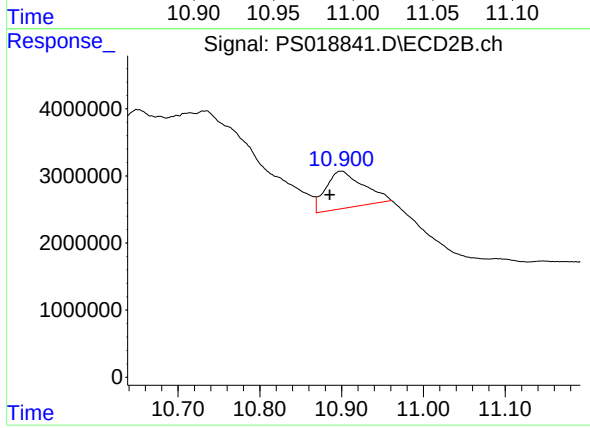

#15 Picloram

R.T.: 10.899 min
Delta R.T.: 0.014 min
Response: 18283177
Conc: 4.33 ng/ml