

Data Path : P:\HPCHEM1\FID E\Data\FE040918\
Data File : FE026571.D
Signal(s) : FID1B.CH
Acq On : 09 Apr 2018 16:02
Operator : UA/AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 06:00:57 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
Quant Title :
QLast Update : Mon Apr 09 14:09:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	7.012	3691791	19.656 ug/ml
12)	N-OCTACOSANE	17.507	3756580	20.393 ug/ml
13)	N-TRIACONTANE	18.393	148004	0.864 ug/ml
14)	N-DOTRIACONTANE	19.230	162228	0.906 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE040918\
Data File : FE026571.D
Signal(s) : FID1B.CH
Acq On : 09 Apr 2018 16:02
Operator : UA/AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 06:00:57 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
Quant Title :
QLast Update : Mon Apr 09 14:09:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

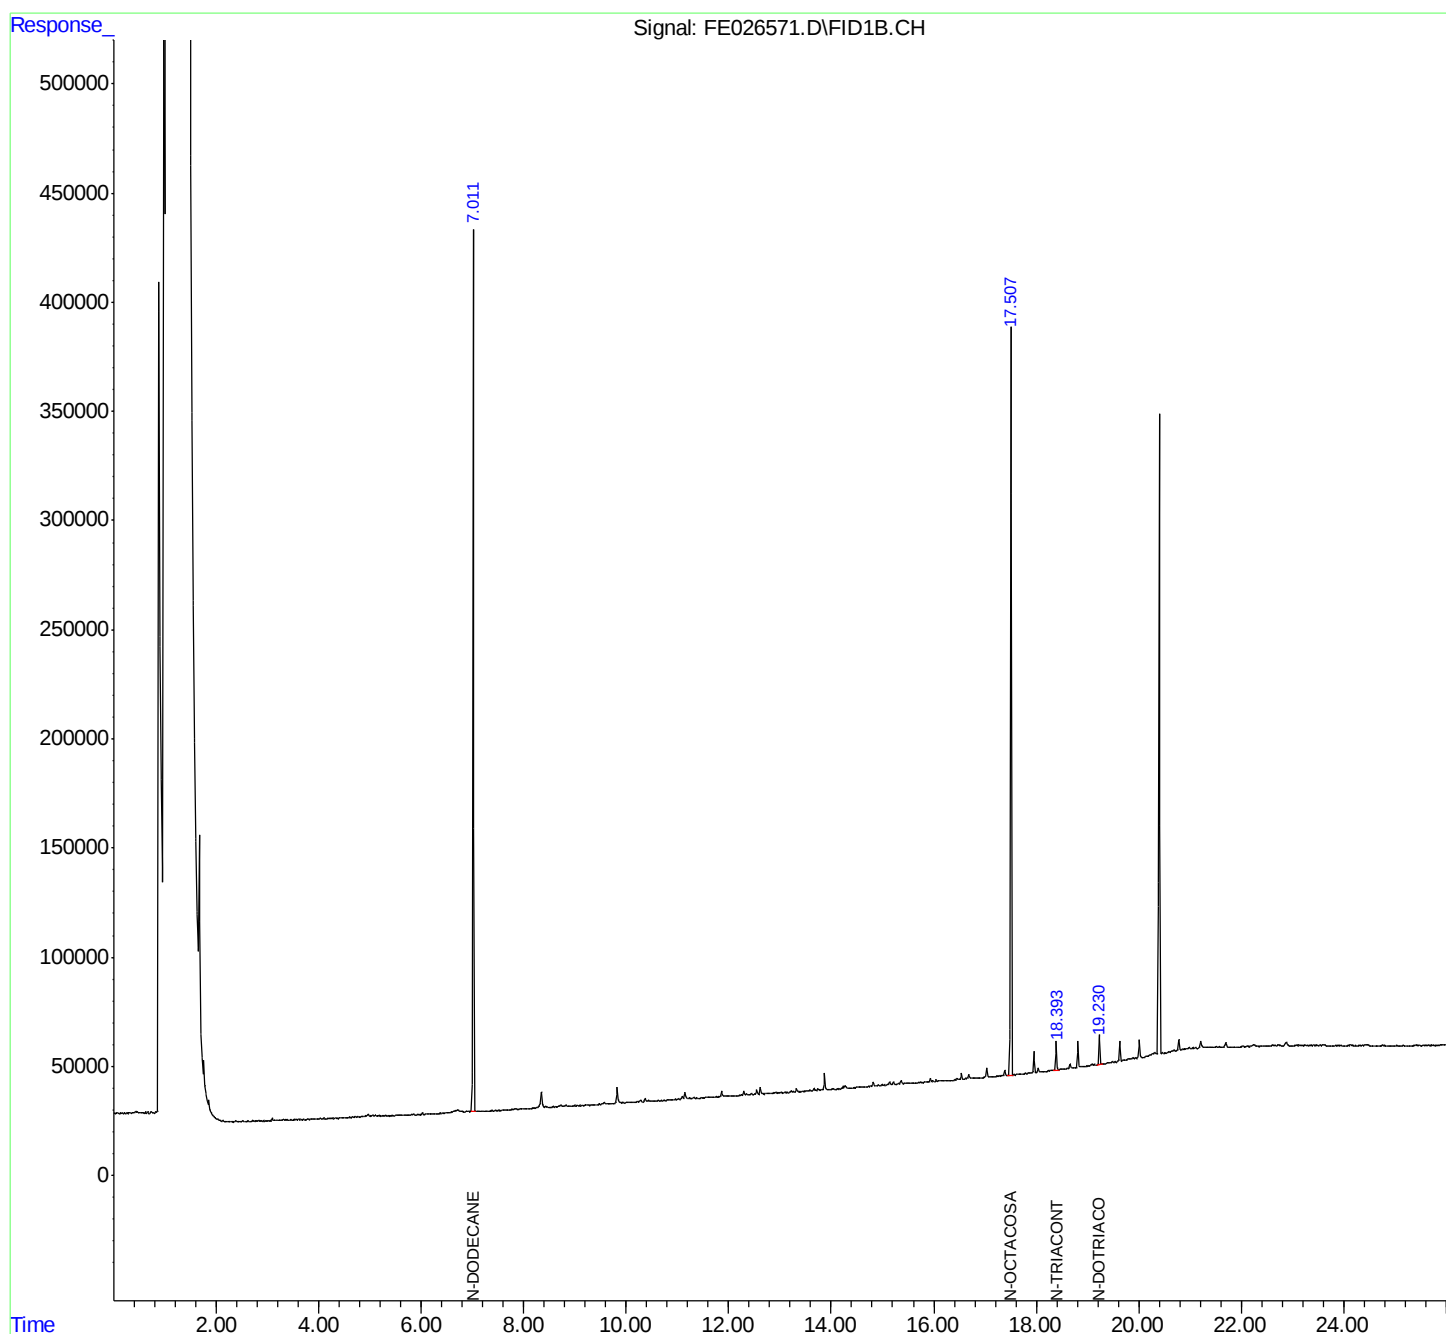


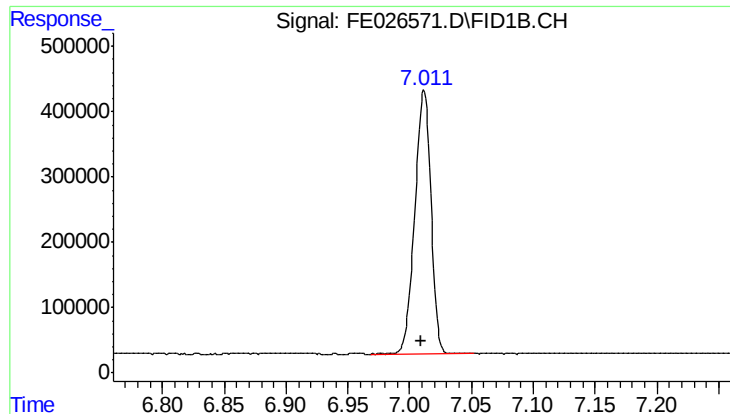

#3 N-DODECANE


R.T.: 7.012 min
Delta R.T.: 0.002 min
Response: 3691791
Conc: 19.66 ug/ml

Instrument :
FID_E
ClientSampleId :

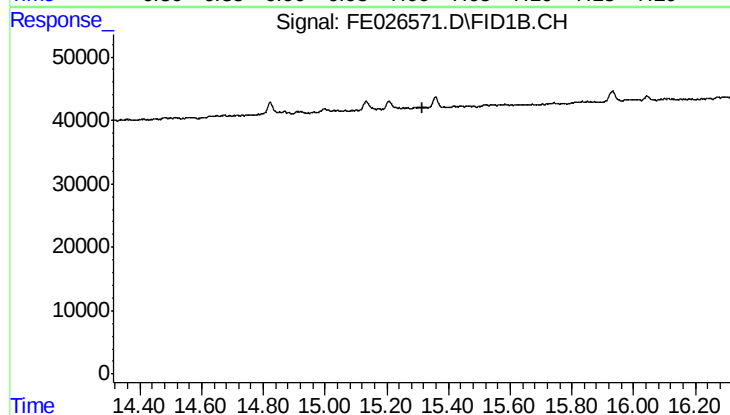


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.314 min
Response: 0
Conc: N.D.

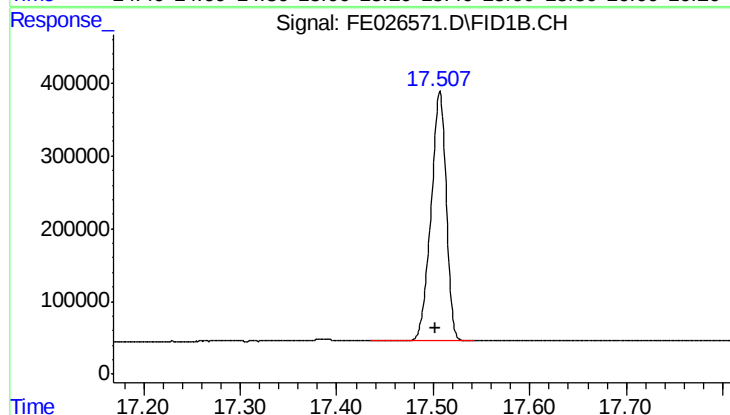


#12 N-OCTACOSANE

R.T.: 17.507 min
Delta R.T.: 0.004 min
Response: 3756580
Conc: 20.39 ug/ml

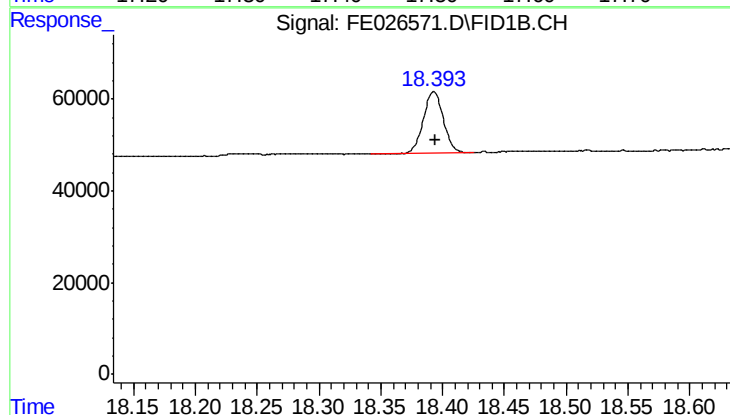

#13 N-TRIACONTANE

R.T.: 18.393 min
Delta R.T.: -0.001 min
Response: 148004
Conc: 0.86 ug/ml

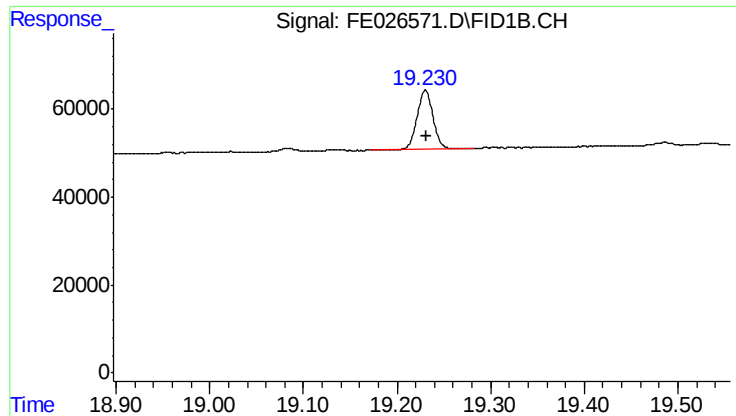

#14 N-DOTRIACONTANE

R.T.: 19.230 min
Delta R.T.: -0.001 min
Response: 162228
Conc: 0.91 ug/ml

Instrument :
FID_E
ClientSampleId :