

Data Path : P:\HPCHEM1\FID E\Data\FE040918\
 Data File : FE026578.D
 Signal(s) : FID1B.CH
 Acq On : 09 Apr 2018 20:08
 Operator : UA/AJ
 Sample : J2155-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 10 06:02:06 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
 Quant Title :
 QLast Update : Mon Apr 09 14:09:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.321	4588450	23.487 ug/ml
Target Compounds			
3) N-DODECANE	7.010	112440	0.599 ug/ml
4) N-TETRADECANE	8.820	492162	2.401 ug/ml
5) N-HEXADECANE	10.434	1076524	4.860 ug/ml
6) N-OCTADECANE	11.886	526540	2.251 ug/ml
7) N-EICOSANE	13.205	260939	1.119 ug/ml
8) N-DOCOSANE	14.412	136747	0.595 ug/ml
10) N-TETRACOSANE	15.524	345002	1.552 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE040918\
Data File : FE026578.D
Signal(s) : FID1B.CH
Acq On : 09 Apr 2018 20:08
Operator : UA/AJ
Sample : J2155-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 06:02:06 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
Quant Title :
QLast Update : Mon Apr 09 14:09:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

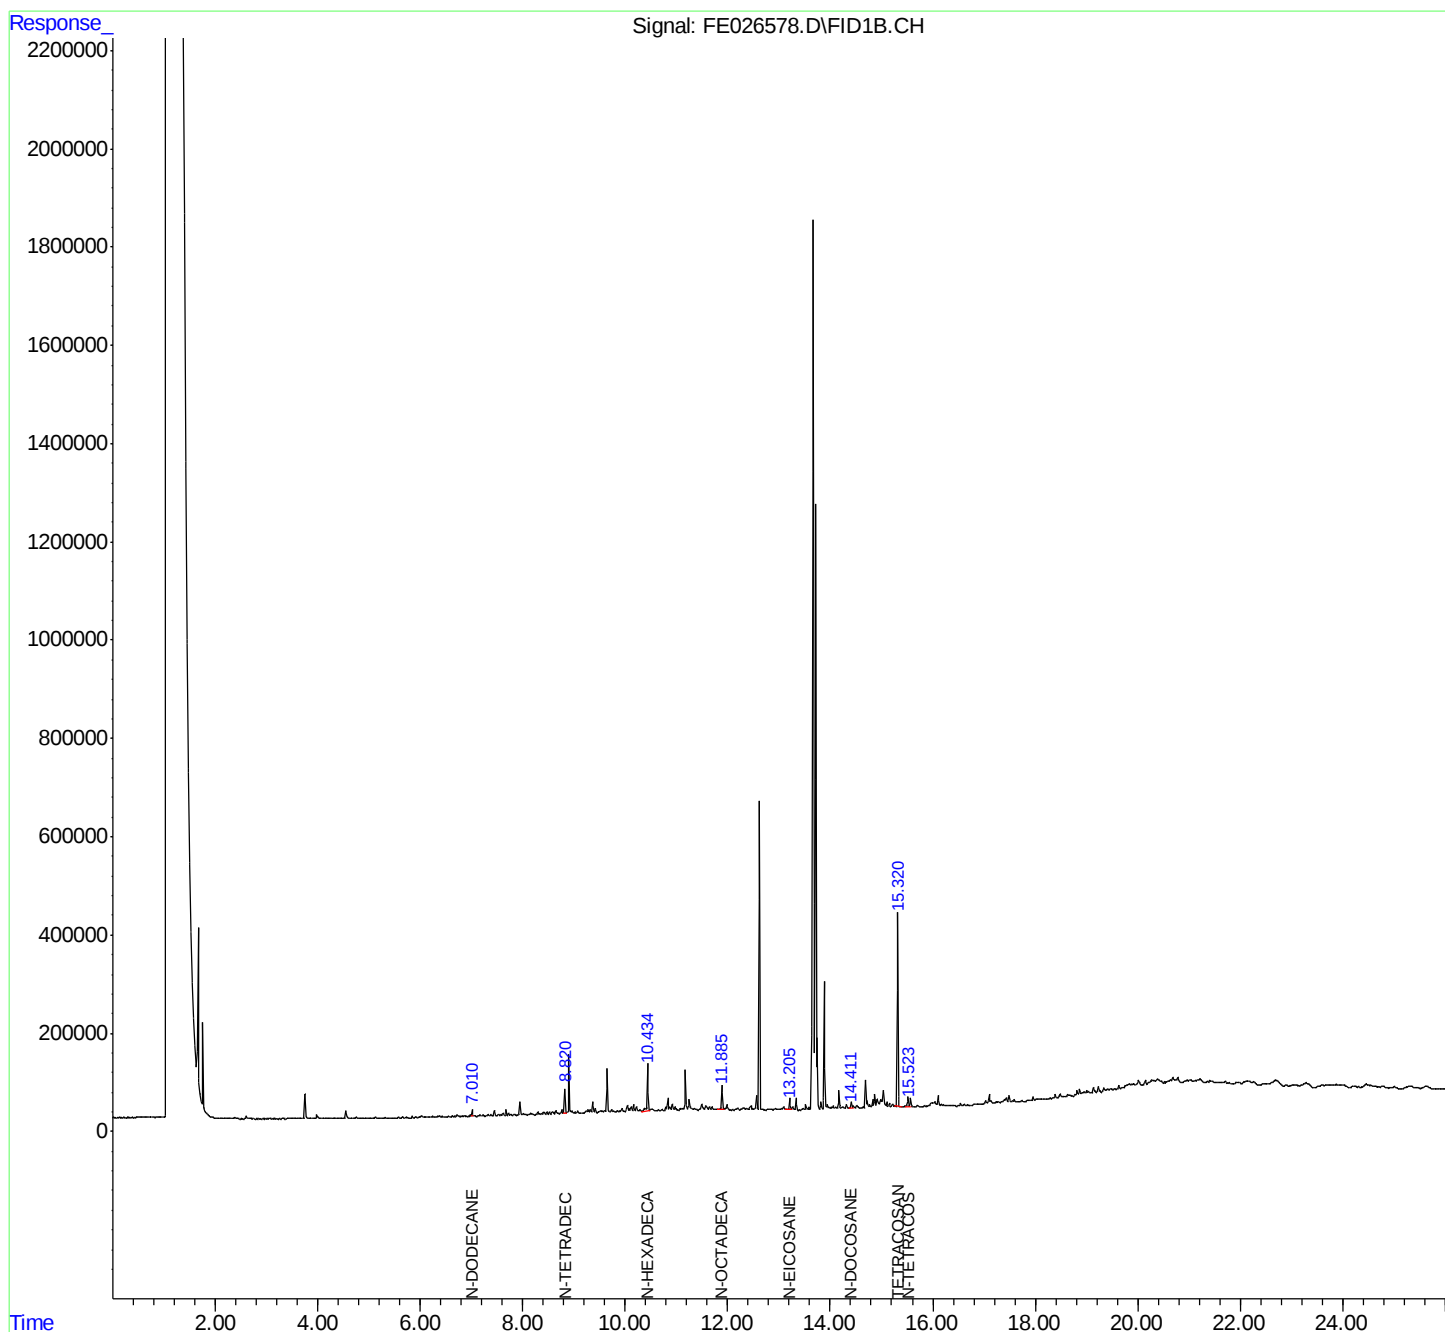


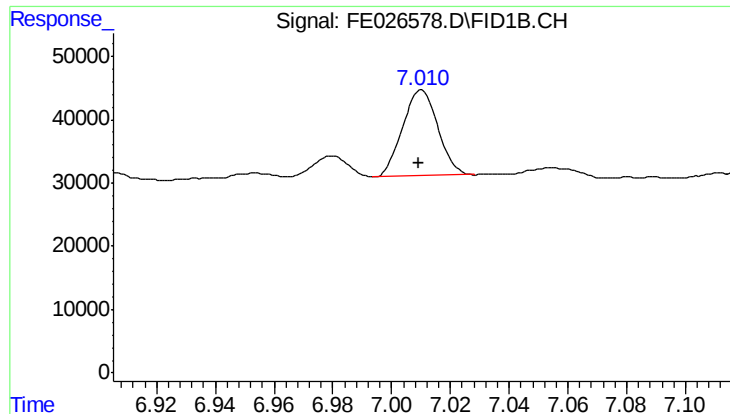

#3 N-DODECANE


R.T.: 7.010 min
Delta R.T.: 0.001 min
Response: 112440
Conc: 0.60 ug/ml

Instrument :
FID_E
ClientSampleId :

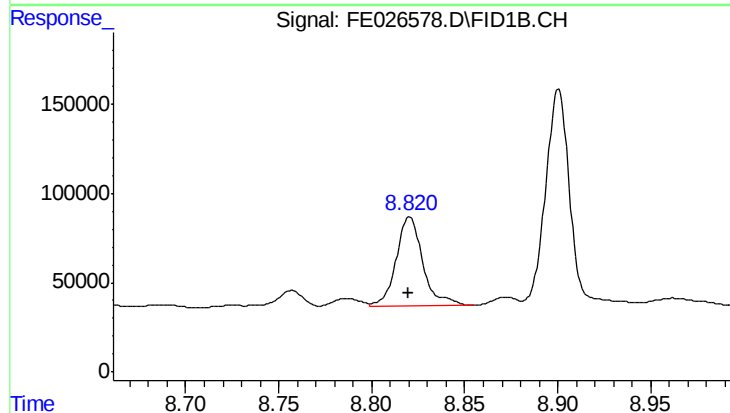


#4 N-TETRADECANE

R.T.: 8.820 min
Delta R.T.: 0.001 min
Response: 492162
Conc: 2.40 ug/ml

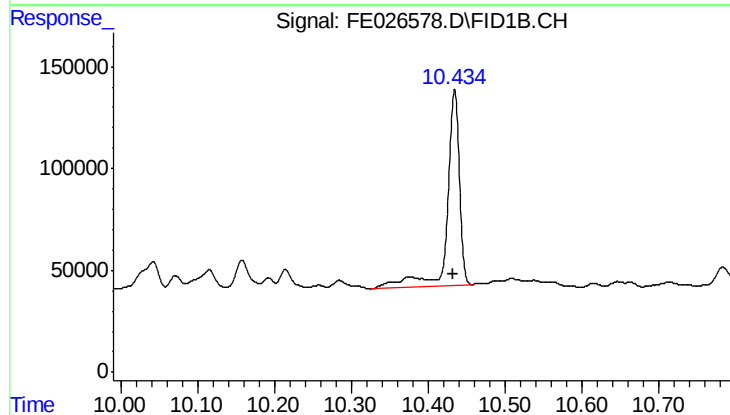


#5 N-HEXADECANE

R.T.: 10.434 min
Delta R.T.: 0.001 min
Response: 1076524
Conc: 4.86 ug/ml

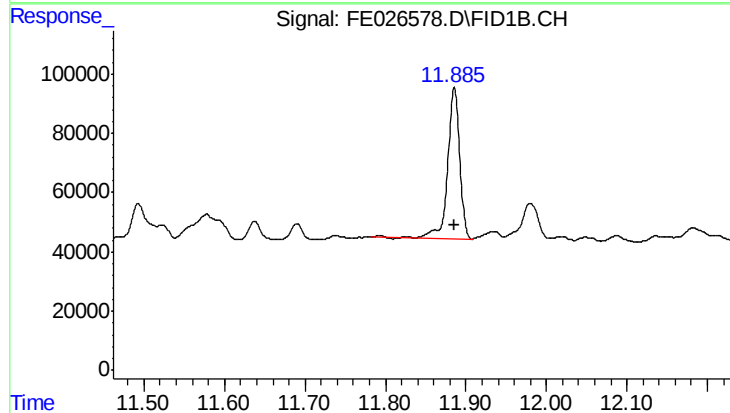

#6 N-OCTADECANE


R.T.: 11.886 min
Delta R.T.: 0.000 min
Response: 526540
Conc: 2.25 ug/ml

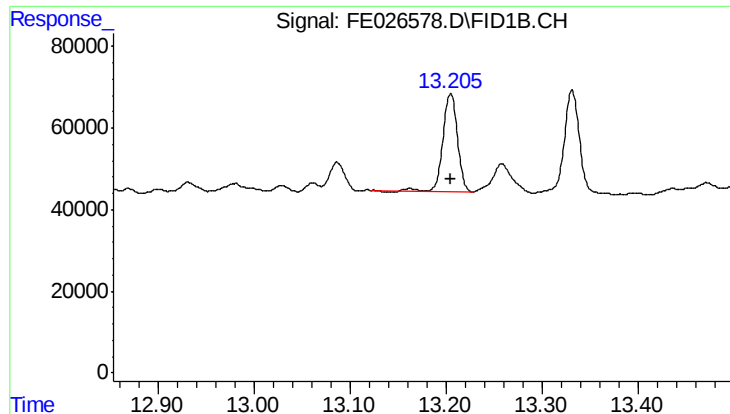

#7 N-EICOSANE


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 260939
Conc: 1.12 ug/ml

Instrument :
FID_E
ClientSampleId :

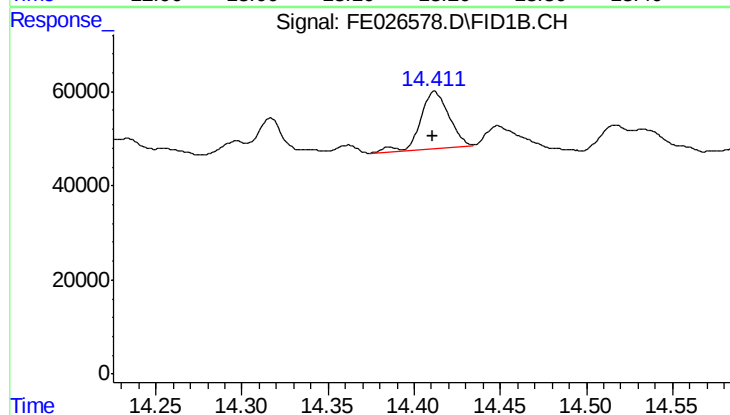


#8 N-DOCOSANE

R.T.: 14.412 min
Delta R.T.: 0.002 min
Response: 136747
Conc: 0.59 ug/ml

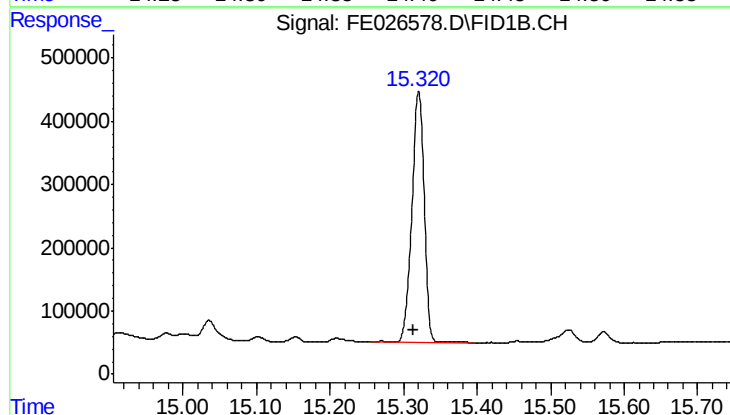

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.321 min
Delta R.T.: 0.006 min
Response: 4588450
Conc: 23.49 ug/ml

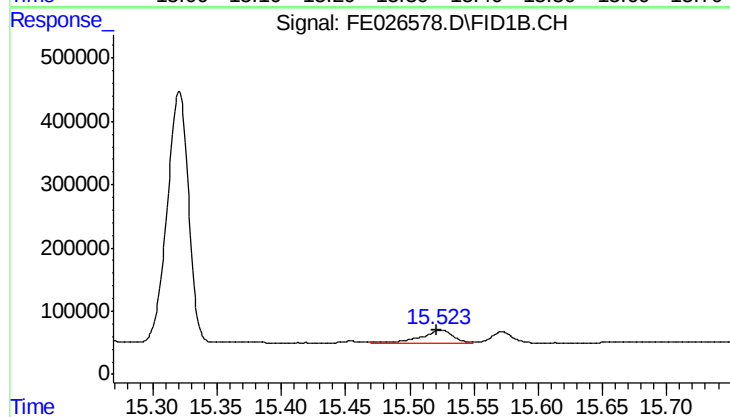

#10 N-TETRACOSANE

R.T.: 15.524 min
Delta R.T.: 0.003 min
Response: 345002
Conc: 1.55 ug/ml