

Data Path : P:\HPCHEM1\FID E\Data\FE040918\
 Data File : FE026585.D
 Signal(s) : FID1B.CH
 Acq On : 10 Apr 2018 00:12
 Operator : UA/AJ
 Sample : J2157-05 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 10 06:03:31 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
 Quant Title :
 QLast Update : Mon Apr 09 14:09:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.318	345927	1.771 ug/ml
Target Compounds				
2)	N-DECANE	5.018f	363033	2.114 ug/ml
10)	N-TETRACOSANE	15.530	245106	1.103 ug/ml
12)	N-OCTACOSANE	17.506	293404	1.593 ug/ml
13)	N-TRIACONTANE	18.406	297360	1.735 ug/ml
14)	N-DOTRIACONTANE	19.244	318492	1.779 ug/ml
15)	N-TETRATRIACONTANE	20.033	246733	1.337 ug/ml
16)	N-HEXATRIACONTANE	20.804	853454	4.654 ug/ml
17)	N-OCTATRIACONTANE	21.725	1194671	6.978 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID E\Data\FE040918\
Data File : FE026585.D
Signal(s) : FID1B.CH
Acq On : 10 Apr 2018 00:12
Operator : UA/AJ
Sample : J2157-05 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 10 06:03:31 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
Quant Title :
QLast Update : Mon Apr 09 14:09:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

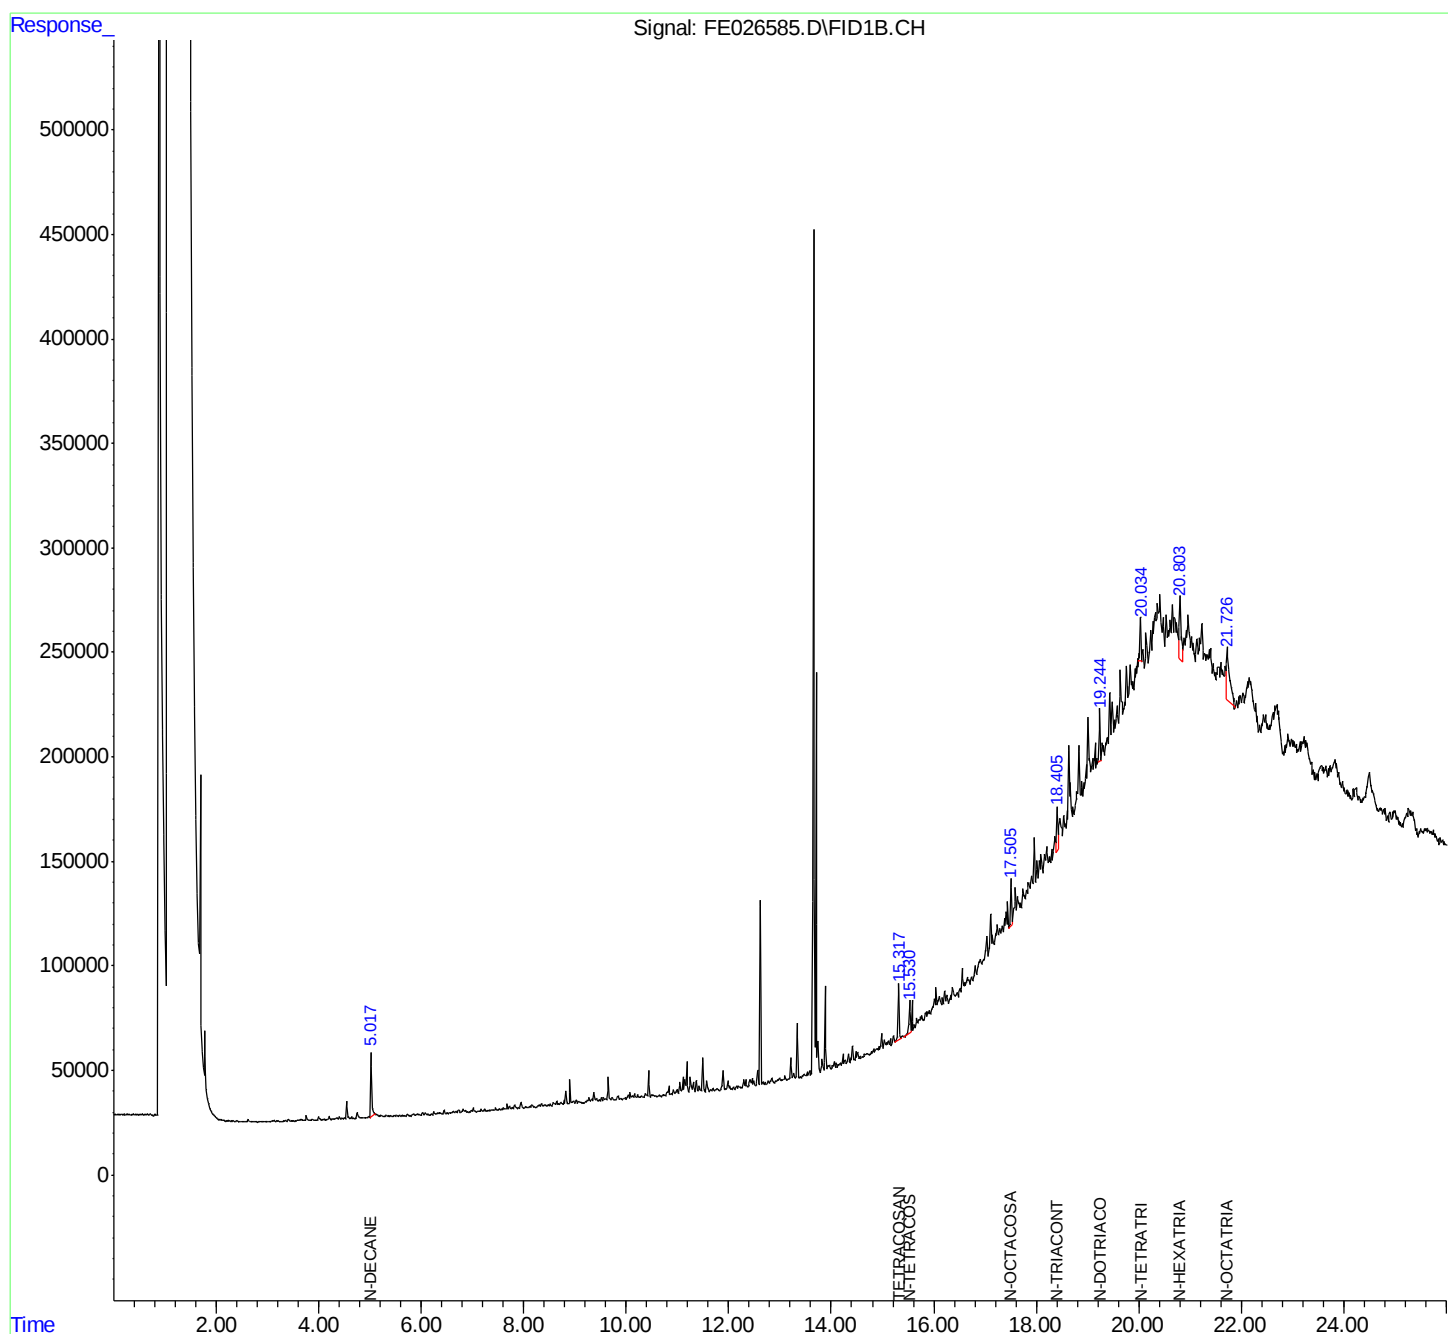


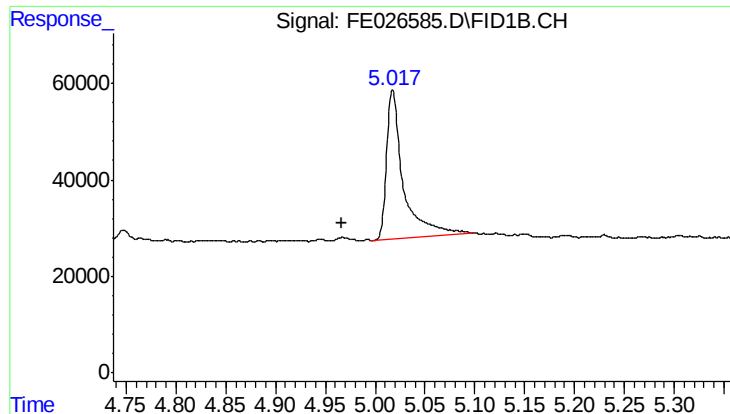

#2 N-DECANE


R.T.: 5.018 min
Delta R.T.: 0.051 min
Response: 363033
Conc: 2.11 ug/ml

Instrument :
FID_E
ClientSampleId :

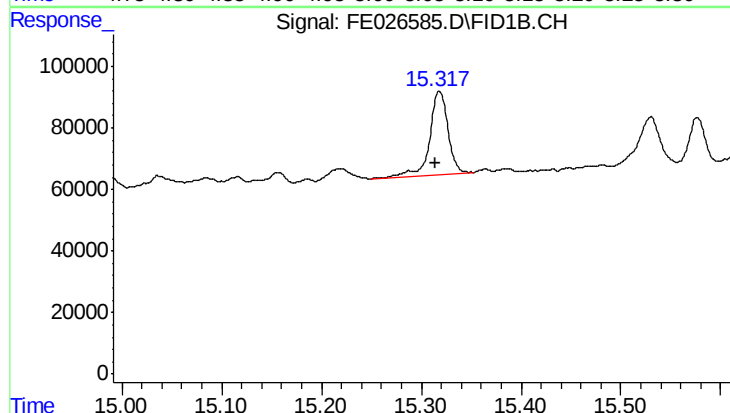


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.318 min
Delta R.T.: 0.004 min
Response: 345927
Conc: 1.77 ug/ml

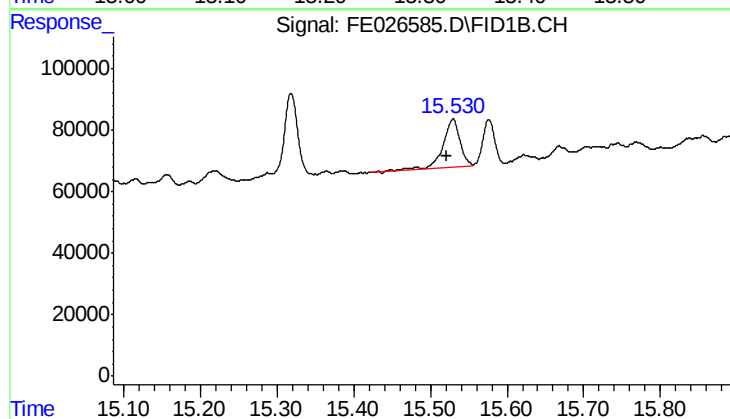


#10 N-TETRACOSANE

R.T.: 15.530 min
Delta R.T.: 0.008 min
Response: 245106
Conc: 1.10 ug/ml

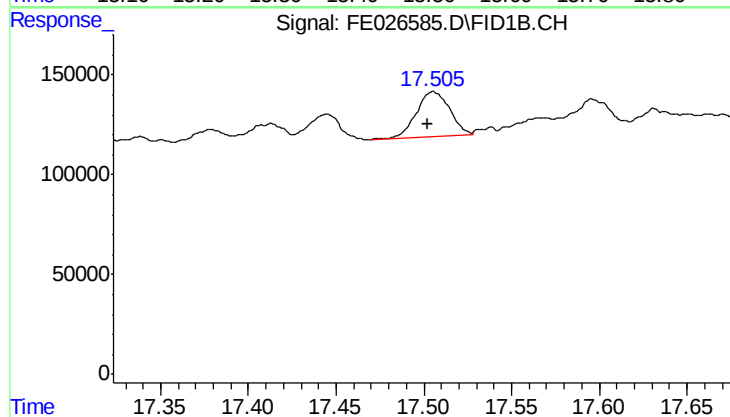

#12 N-OCTACOSANE


R.T.: 17.506 min
Delta R.T.: 0.003 min
Response: 293404
Conc: 1.59 ug/ml

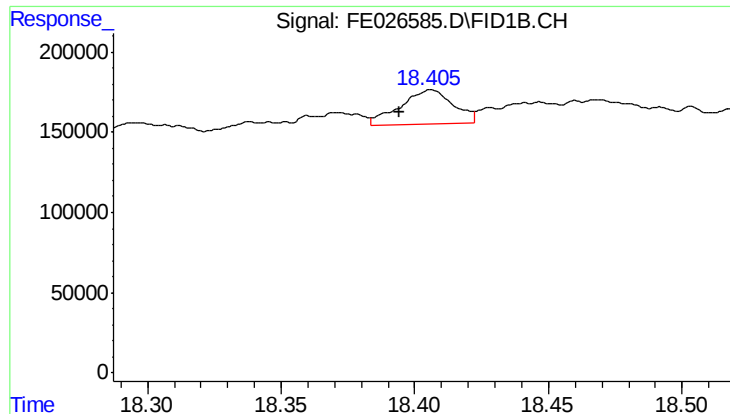

#13 N-TRIACONTANE


R.T.: 18.406 min
Delta R.T.: 0.012 min
Response: 297360
Conc: 1.73 ug/ml

Instrument :
FID_E
ClientSampleId :

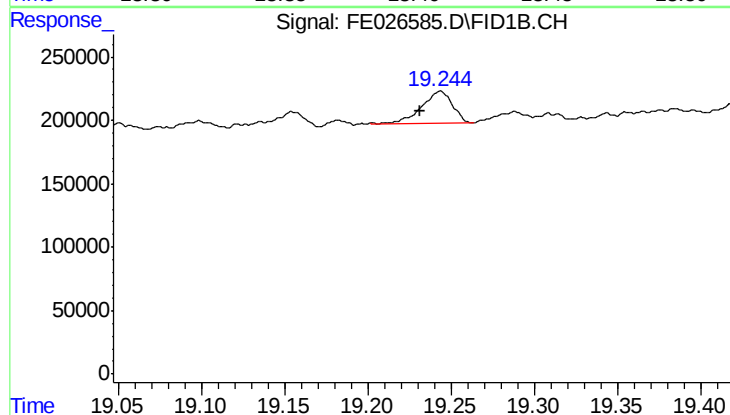


#14 N-DOTRIACONTANE

R.T.: 19.244 min
Delta R.T.: 0.012 min
Response: 318492
Conc: 1.78 ug/ml

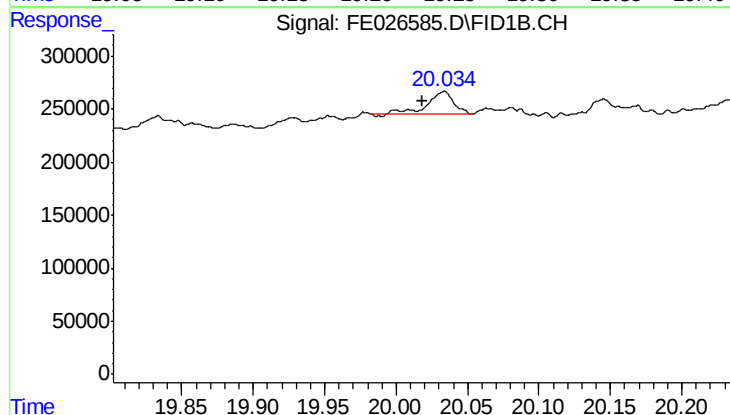


#15 N-TETRATRIACONTANE

R.T.: 20.033 min
Delta R.T.: 0.015 min
Response: 246733
Conc: 1.34 ug/ml

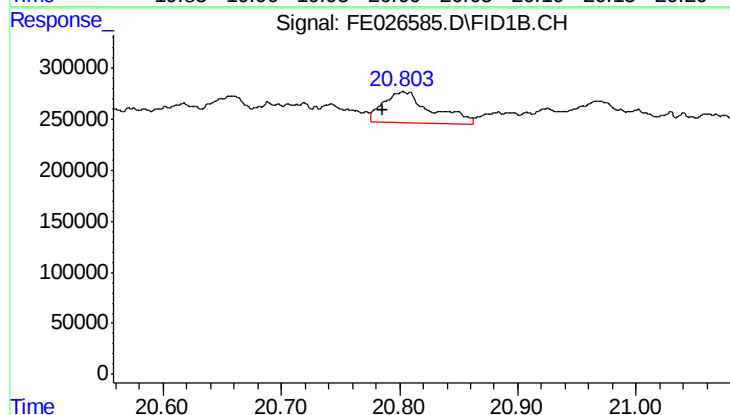

#16 N-HEXATRIACONTANE

R.T.: 20.804 min
Delta R.T.: 0.017 min
Response: 853454
Conc: 4.65 ug/ml

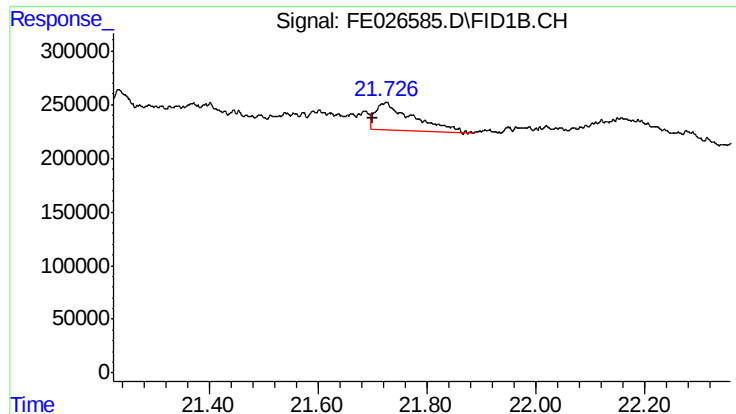

#17 N-OCTATRIACONTANE

R.T.: 21.725 min
Delta R.T.: 0.024 min
Response: 1194671
Conc: 6.98 ug/ml

Instrument :
FID_E
ClientSampleId :