

Data Path : P:\HPCHEM1\FID_E\Data\FE050418\
 Data File : FE026863.D
 Signal(s) : FID1B.CH
 Acq On : 03 May 2018 18:19
 Operator : UA/AJ
 Sample : J2681-01 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 04 07:35:26 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
 Quant Title :
 QLast Update : Mon Apr 09 14:09:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.301	336642	1.723 ug/ml
Target Compounds			
4) N-TETRADECANE	8.805	223677	1.091 ug/ml
5) N-HEXADECANE	10.418	453950	2.049 ug/ml
6) N-OCTADECANE	11.871	325767	1.393 ug/ml
7) N-EICOSANE	13.191	285068	1.223 ug/ml
8) N-DOCOSANE	14.399	284867	1.239 ug/ml
10) N-TETRACOSANE	15.509	696174	3.132 ug/ml
12) N-OCTACOSANE	17.488	272091	1.477 ug/ml
13) N-TRIACONTANE	18.383	235454	1.374 ug/ml
14) N-DOTRIACONTANE	19.221	286404	1.599 ug/ml
15) N-TETRATRIACONTANE	20.009	262502	1.422 ug/ml
16) N-HEXATRIACONTANE	20.773	460673	2.512 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050418\
Data File : FE026863.D
Signal(s) : FID1B.CH
Acq On : 03 May 2018 18:19
Operator : UA/AJ
Sample : J2681-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 04 07:35:26 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
Quant Title :
QLast Update : Mon Apr 09 14:09:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

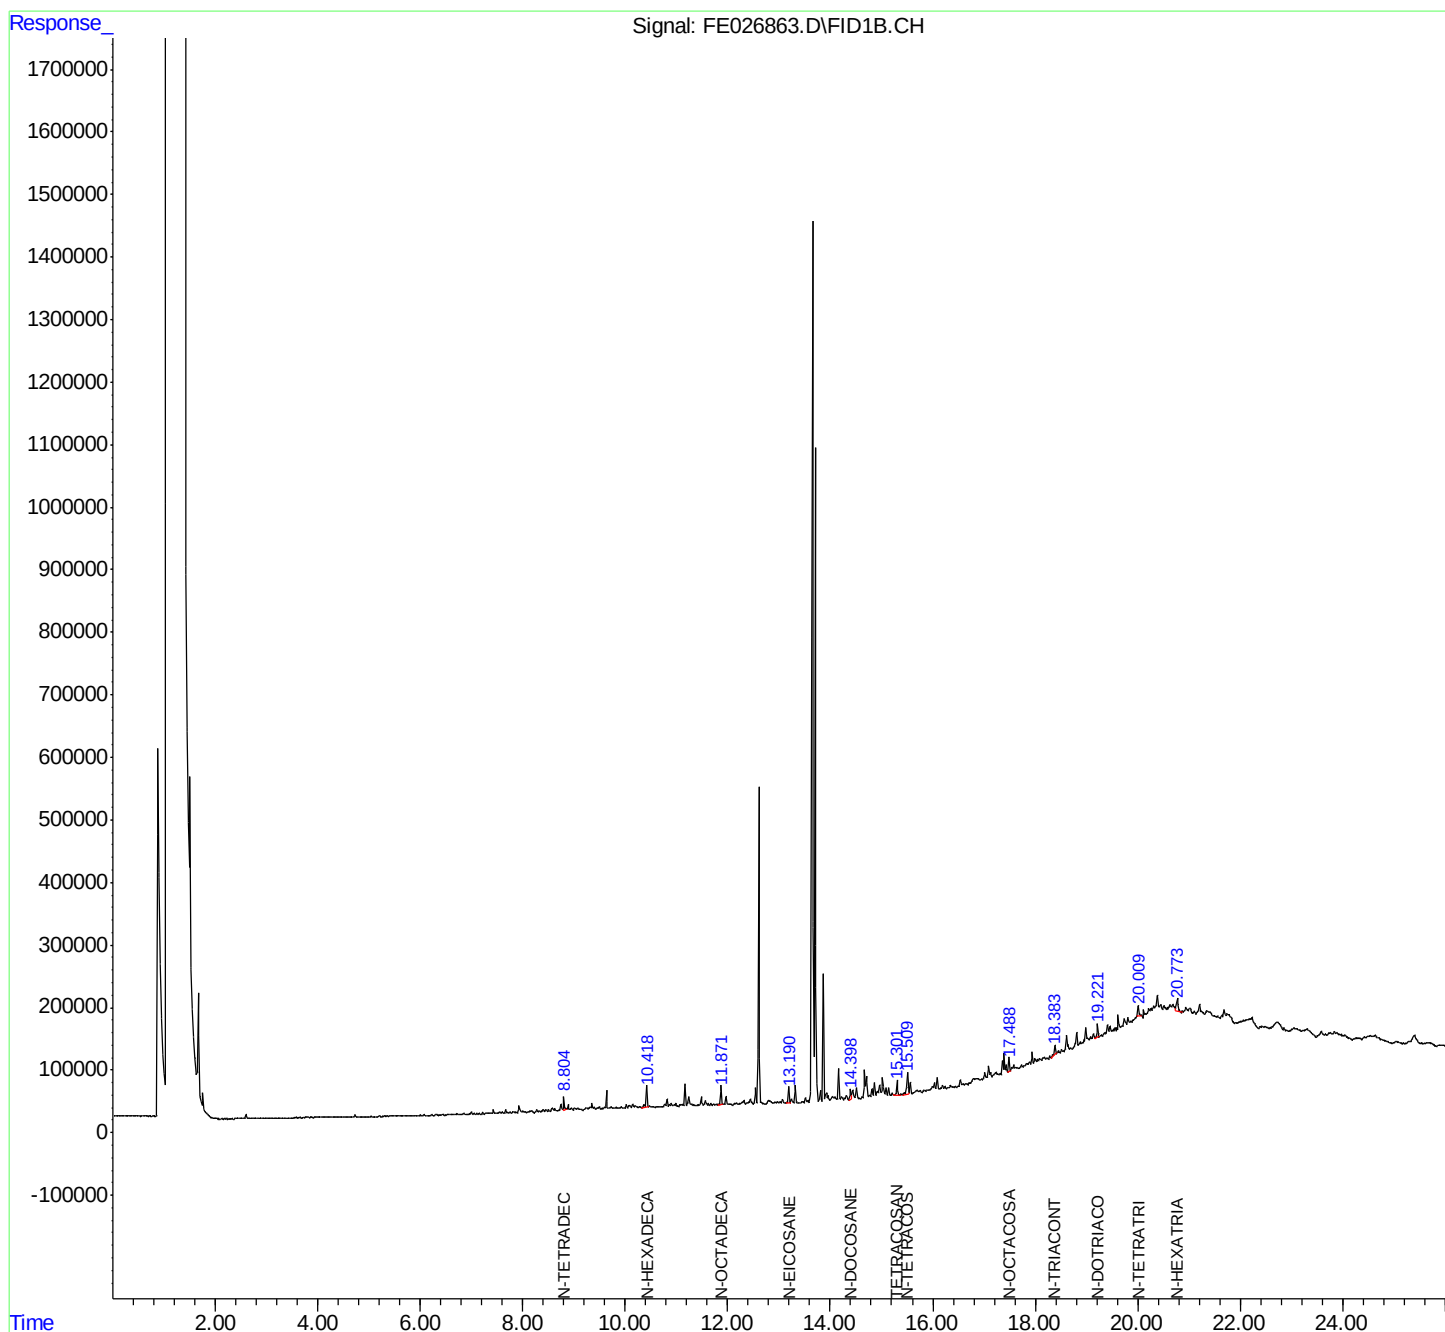


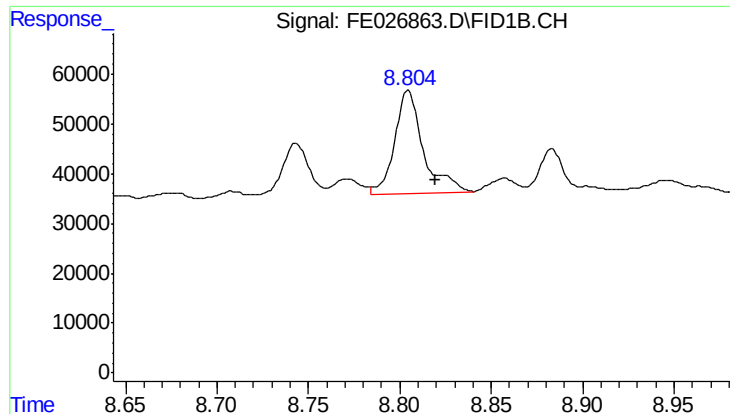

#4 N-TETRADECANE


R.T.: 8.805 min
Delta R.T.: -0.015 min
Response: 223677
Conc: 1.09 ug/ml

Instrument :
FID_E
ClientSampleId :

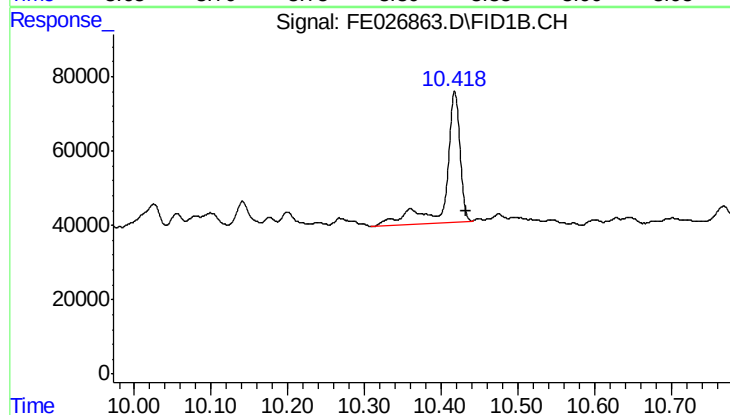


#5 N-HEXADECANE

R.T.: 10.418 min
Delta R.T.: -0.014 min
Response: 453950
Conc: 2.05 ug/ml

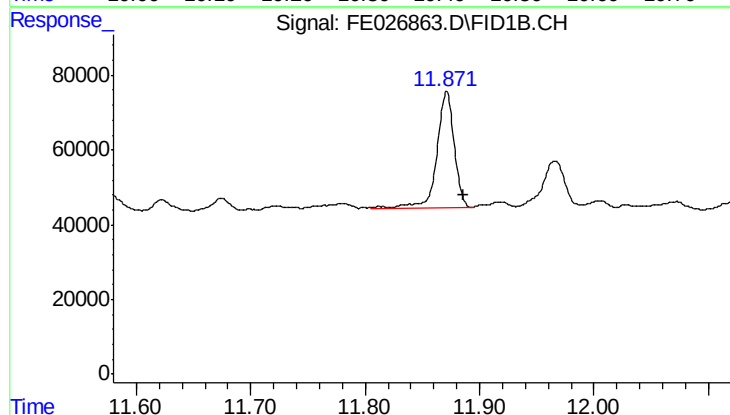


#6 N-OCTADECANE

R.T.: 11.871 min
Delta R.T.: -0.015 min
Response: 325767
Conc: 1.39 ug/ml

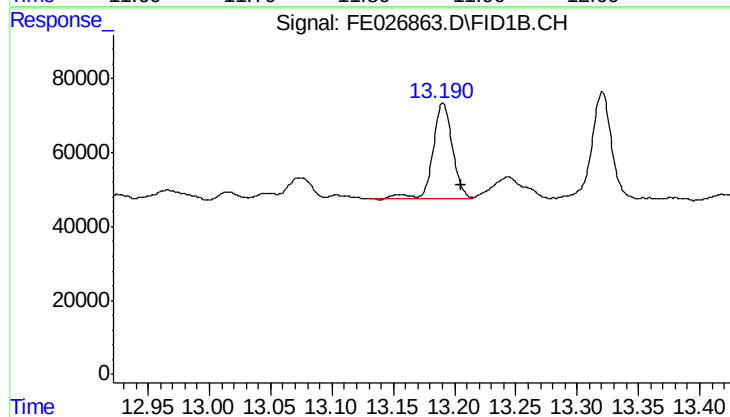

#7 N-EICOSANE


R.T.: 13.191 min
Delta R.T.: -0.014 min
Response: 285068
Conc: 1.22 ug/ml

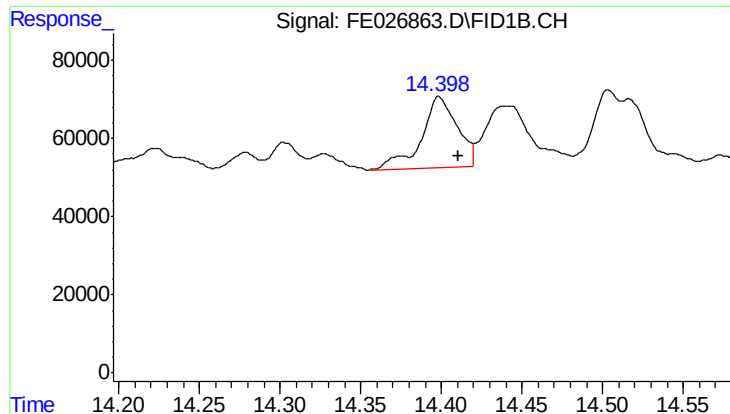

#8 N-DOCOSANE


R.T.: 14.399 min
Delta R.T.: -0.012 min
Response: 284867
Conc: 1.24 ug/ml

Instrument :
FID_E
ClientSampleId :

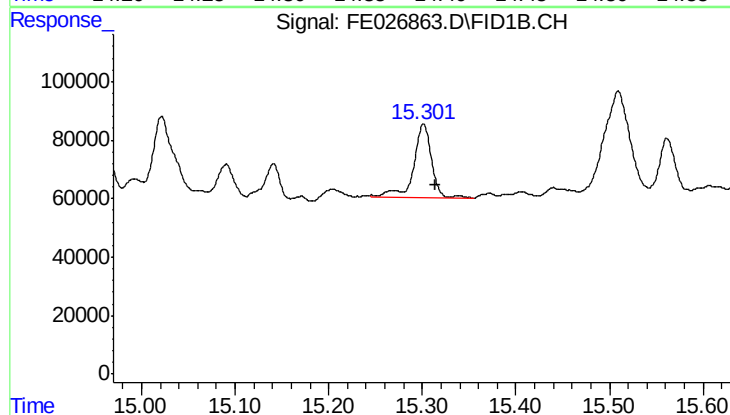


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.301 min
Delta R.T.: -0.013 min
Response: 336642
Conc: 1.72 ug/ml

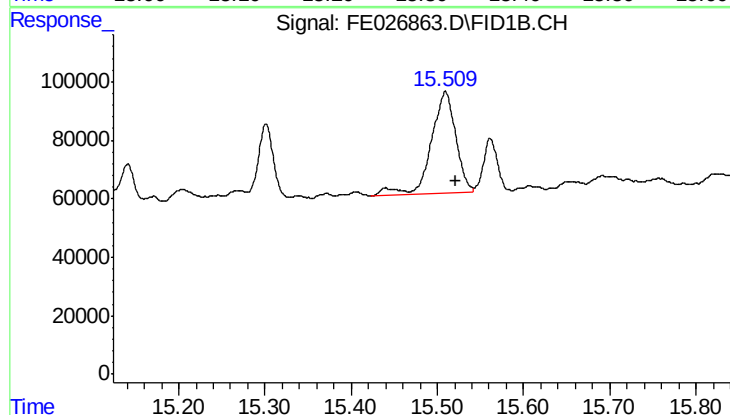


#10 N-TETRACOSANE

R.T.: 15.509 min
Delta R.T.: -0.012 min
Response: 696174
Conc: 3.13 ug/ml

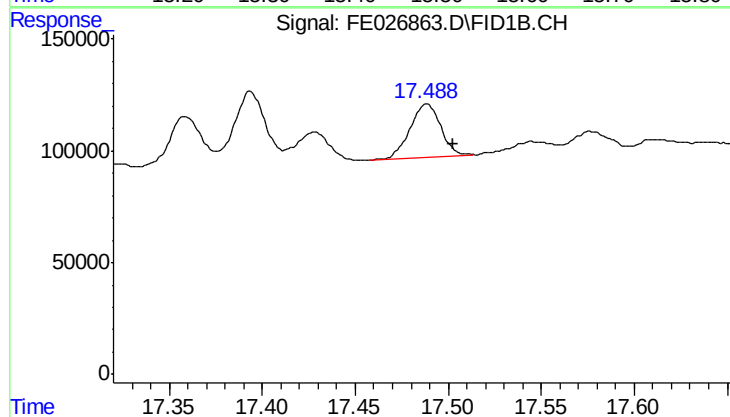

#12 N-OCTACOSANE


R.T.: 17.488 min
Delta R.T.: -0.014 min
Response: 272091
Conc: 1.48 ug/ml

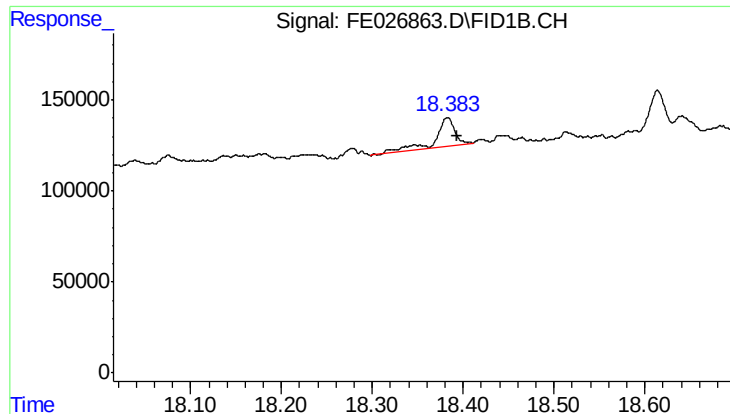

#13 N-TRIACONTANE


R.T.: 18.383 min
Delta R.T.: -0.011 min
Response: 235454
Conc: 1.37 ug/ml

Instrument :
FID_E
ClientSampleId :

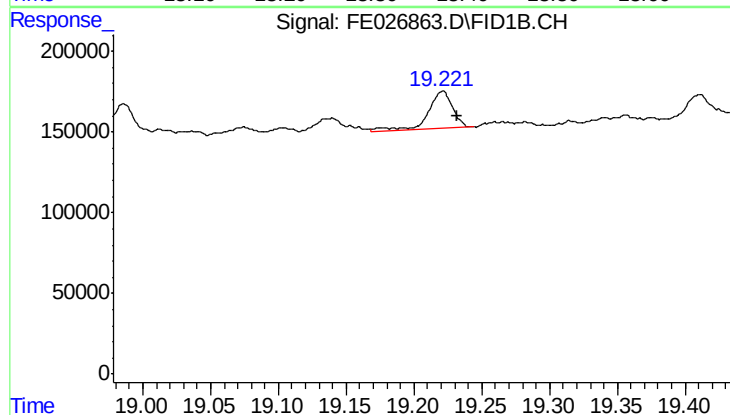


#14 N-DOTRIACONTANE

R.T.: 19.221 min
Delta R.T.: -0.011 min
Response: 286404
Conc: 1.60 ug/ml

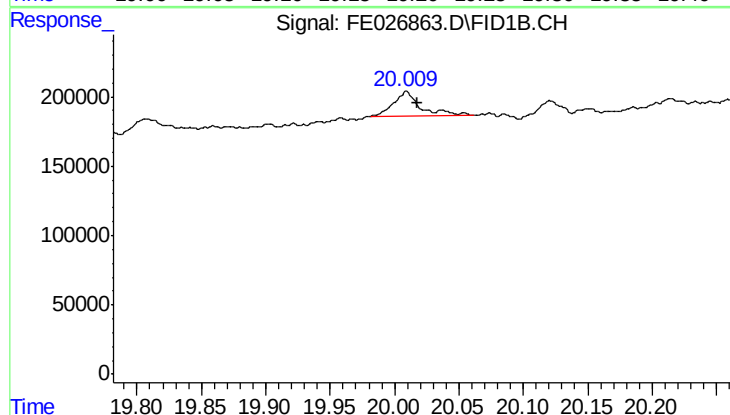

#15 N-TETRATRIACONTANE

R.T.: 20.009 min
Delta R.T.: -0.009 min
Response: 262502
Conc: 1.42 ug/ml

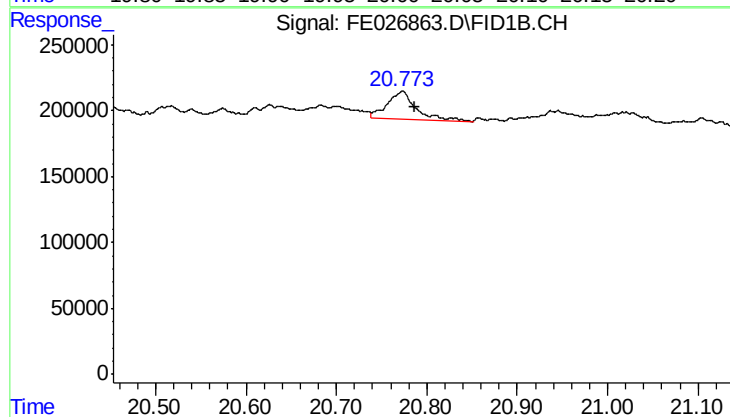

#16 N-HEXATRIACONTANE

R.T.: 20.773 min
Delta R.T.: -0.013 min
Response: 460673
Conc: 2.51 ug/ml