

Data Path : P:\HPCHEM1\FID_E\Data\FE050418\
 Data File : FE026865.D
 Signal(s) : FID1B.CH
 Acq On : 03 May 2018 19:35
 Operator : UA/AJ
 Sample : J2682-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 EPE-F-6(0-5)

Integration File: autoint1.e
 Quant Time: May 04 07:35:53 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
 Quant Title :
 QLast Update : Mon Apr 09 14:09:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.302	2738737	14.019 ug/ml
Target Compounds			
4) N-TETRADECANE	8.884f	711681	3.471 ug/ml
5) N-HEXADECANE	10.418	312487	1.411 ug/ml
6) N-OCTADECANE	11.870	153348	0.656 ug/ml
10) N-TETRACOSANE	15.515	292311	1.315 ug/ml
12) N-OCTACOSANE	17.486	359874	1.954 ug/ml
13) N-TRIACONTANE	18.380	230525	1.345 ug/ml
14) N-DOTRIACONTANE	19.215	224725	1.255 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050418\
Data File : FE026865.D
Signal(s) : FID1B.CH
Acq On : 03 May 2018 19:35
Operator : UA/AJ
Sample : J2682-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
EPE-F-6(0-5)

Integration File: autoint1.e
Quant Time: May 04 07:35:53 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
Quant Title :
QLast Update : Mon Apr 09 14:09:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

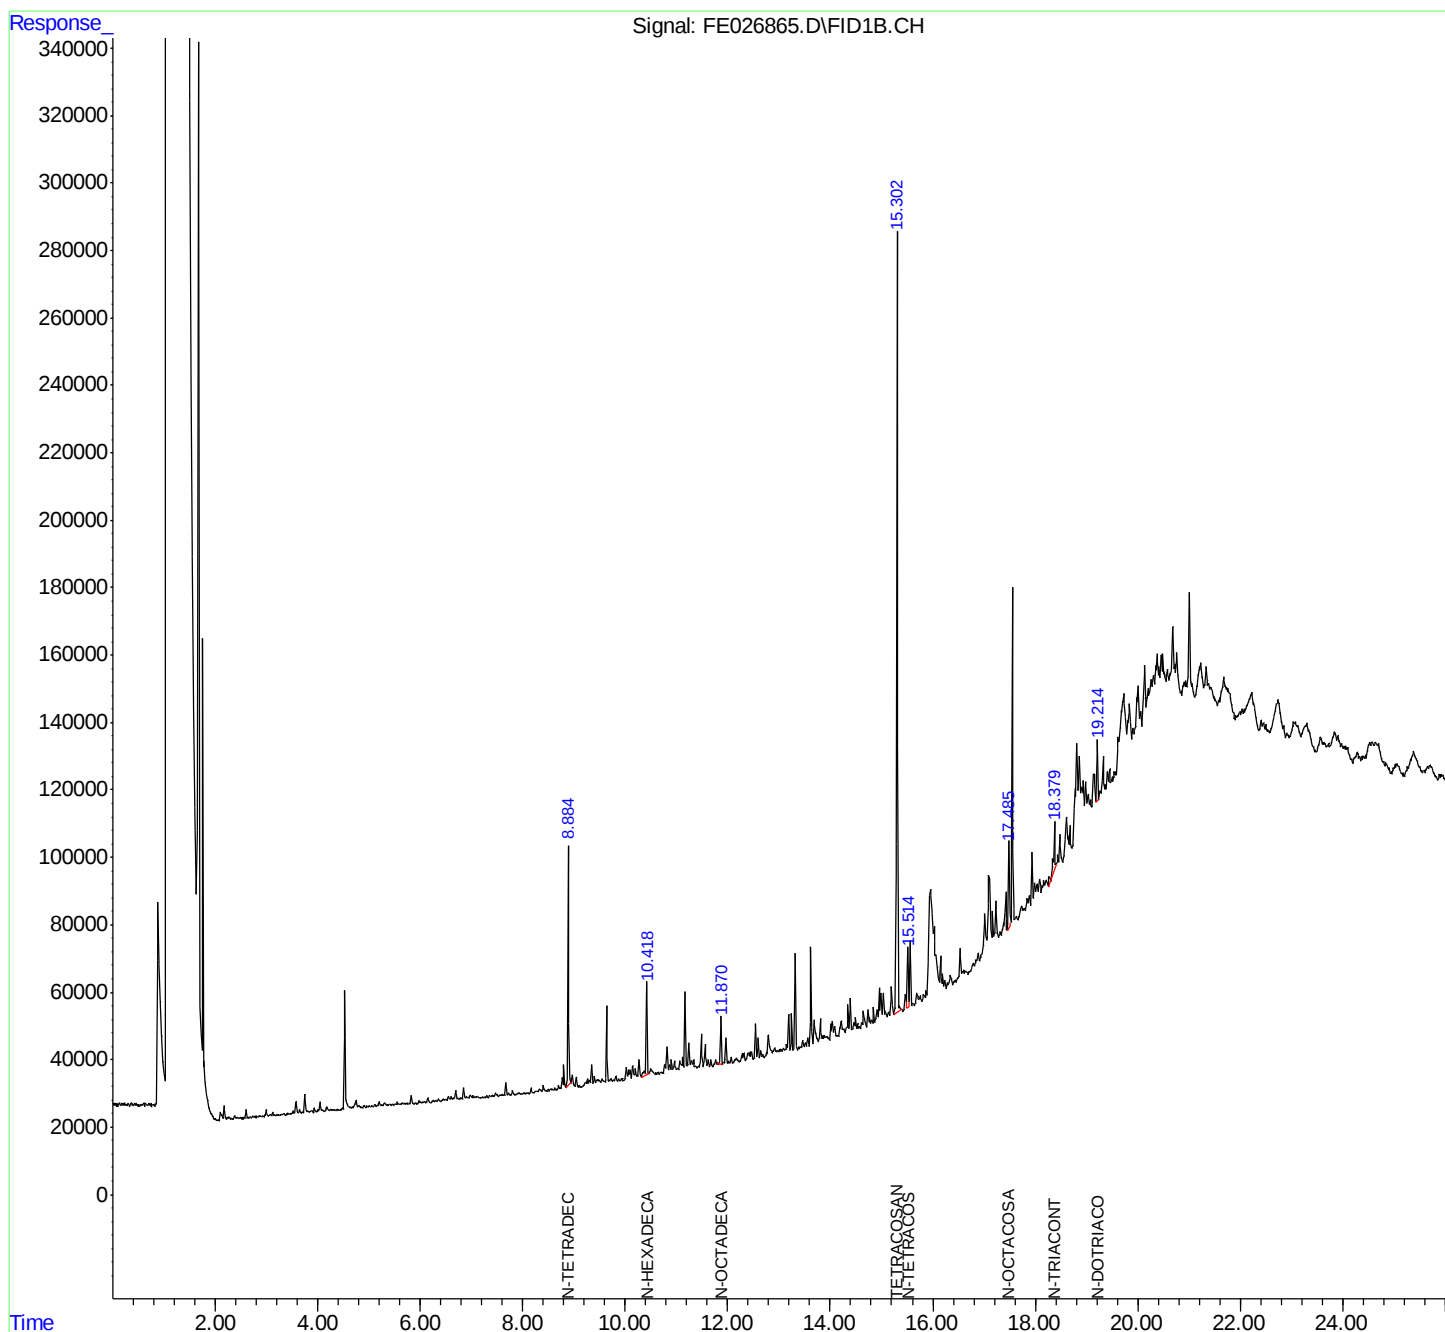


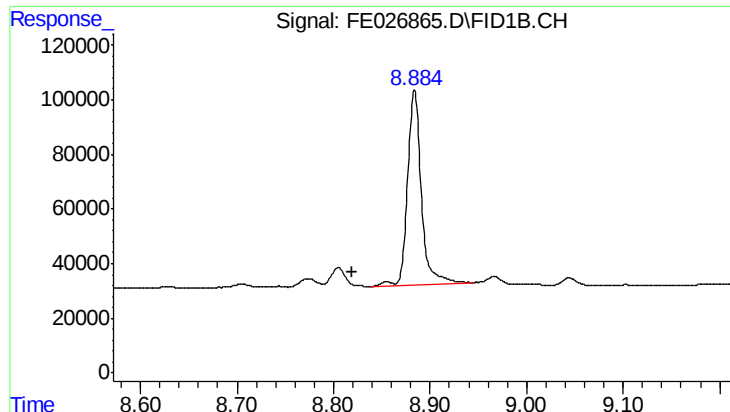

#4 N-TETRADECANE


R.T.: 8.884 min
Delta R.T.: 0.064 min
Response: 711681
Conc: 3.47 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-6(0-5)

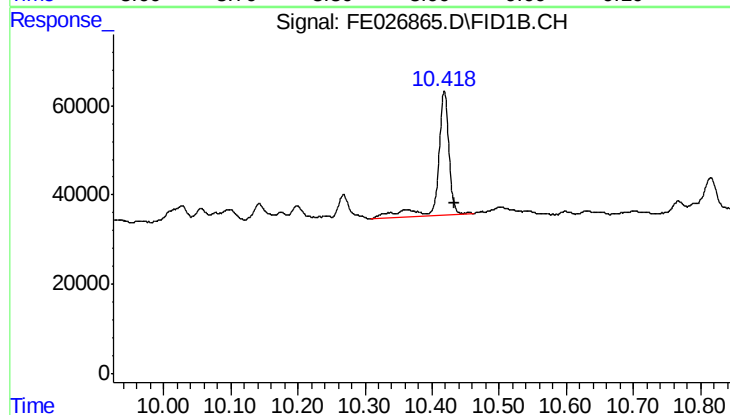


#5 N-HEXADECANE

R.T.: 10.418 min
Delta R.T.: -0.015 min
Response: 312487
Conc: 1.41 ug/ml

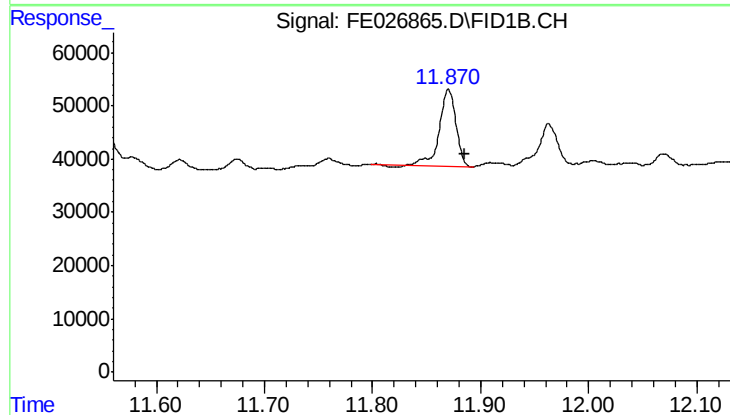


#6 N-OCTADECANE

R.T.: 11.870 min
Delta R.T.: -0.015 min
Response: 153348
Conc: 0.66 ug/ml

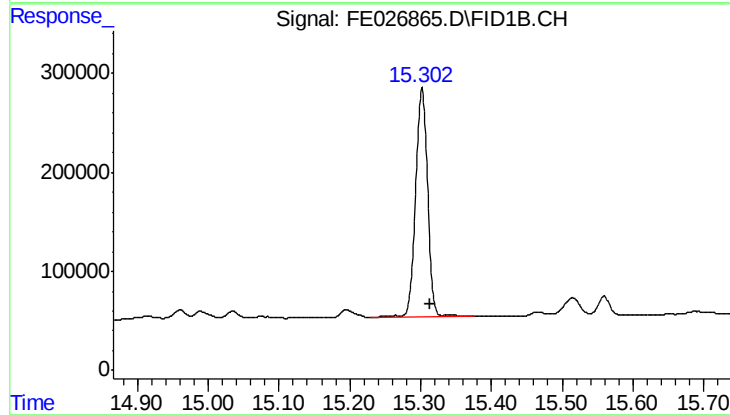

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.302 min
Delta R.T.: -0.012 min
Response: 2738737
Conc: 14.02 ug/ml

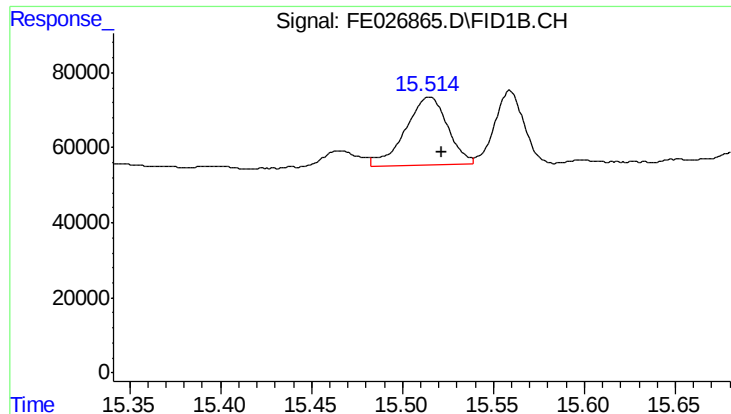

#10 N-TETRACOSANE


R.T.: 15.515 min
Delta R.T.: -0.007 min
Response: 292311
Conc: 1.32 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-6(0-5)

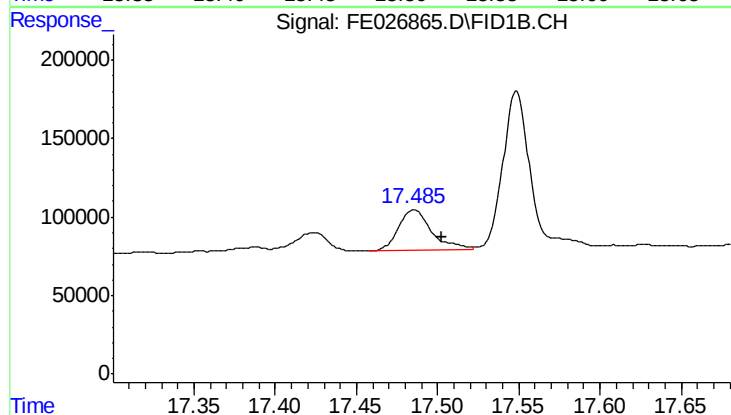


#12 N-OCTACOSANE

R.T.: 17.486 min
Delta R.T.: -0.017 min
Response: 359874
Conc: 1.95 ug/ml

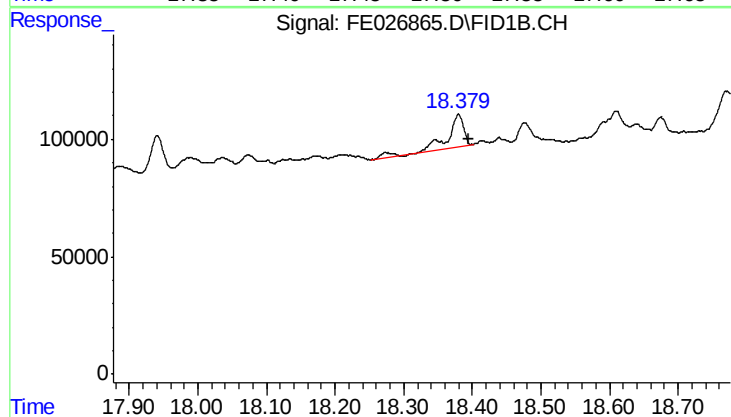

#13 N-TRIACONTANE

R.T.: 18.380 min
Delta R.T.: -0.014 min
Response: 230525
Conc: 1.35 ug/ml

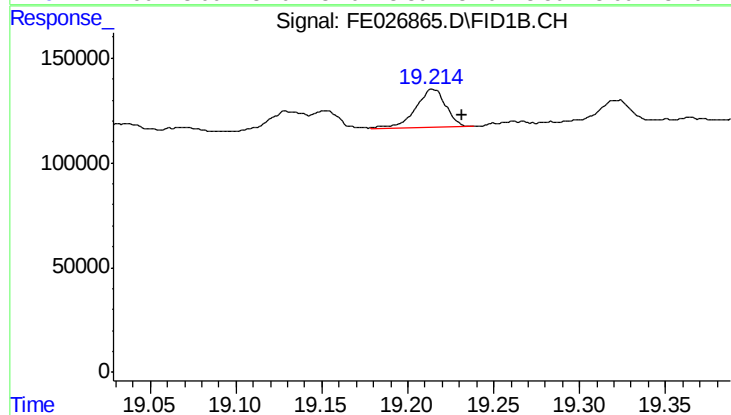

#14 N-DOTRIACONTANE

R.T.: 19.215 min
Delta R.T.: -0.017 min
Response: 224725
Conc: 1.26 ug/ml