

Data Path : P:\HPCHEM1\FID_E\Data\FE050418\
 Data File : FE026883.D
 Signal(s) : FID1B.CH
 Acq On : 04 May 2018 6:43
 Operator : UA/AJ
 Sample : J2705-01MS
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 EPE-F-6A(0-5)MS

Integration File: Sample.e
 Quant Time: May 04 07:39:35 2018
 Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
 Quant Title :
 QLast Update : Mon Apr 09 14:09:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.299	3122169	15.981 ug/ml
Target Compounds			
2) N-DECANE	4.951	2776305	16.166 ug/ml
3) N-DODECANE	6.994	3062250	16.304 ug/ml
4) N-TETRADECANE	8.805	3189105	15.555 ug/ml
5) N-HEXADECANE	10.418	3383087	15.273 ug/ml
6) N-OCTADECANE	11.871	3306389	14.136 ug/ml
7) N-EICOSANE	13.190	3139860	13.469 ug/ml
8) N-DOCOSANE	14.395	3144127	13.680 ug/ml
10) N-TETRACOSANE	15.506	3200509	14.399 ug/ml
11) N-HEXACOSANE	16.532	3204581	15.415 ug/ml
12) N-OCTACOSANE	17.486	3335713	18.108 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_E\Data\FE050418\
Data File : FE026883.D
Signal(s) : FID1B.CH
Acq On : 04 May 2018 6:43
Operator : UA/AJ
Sample : J2705-01MS
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
EPE-F-6A(0-5)MS

Integration File: Sample.e
Quant Time: May 04 07:39:35 2018
Quant Method : P:\HPCHEM1\FID_E\methods\FE040918.M
Quant Title :
QLast Update : Mon Apr 09 14:09:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

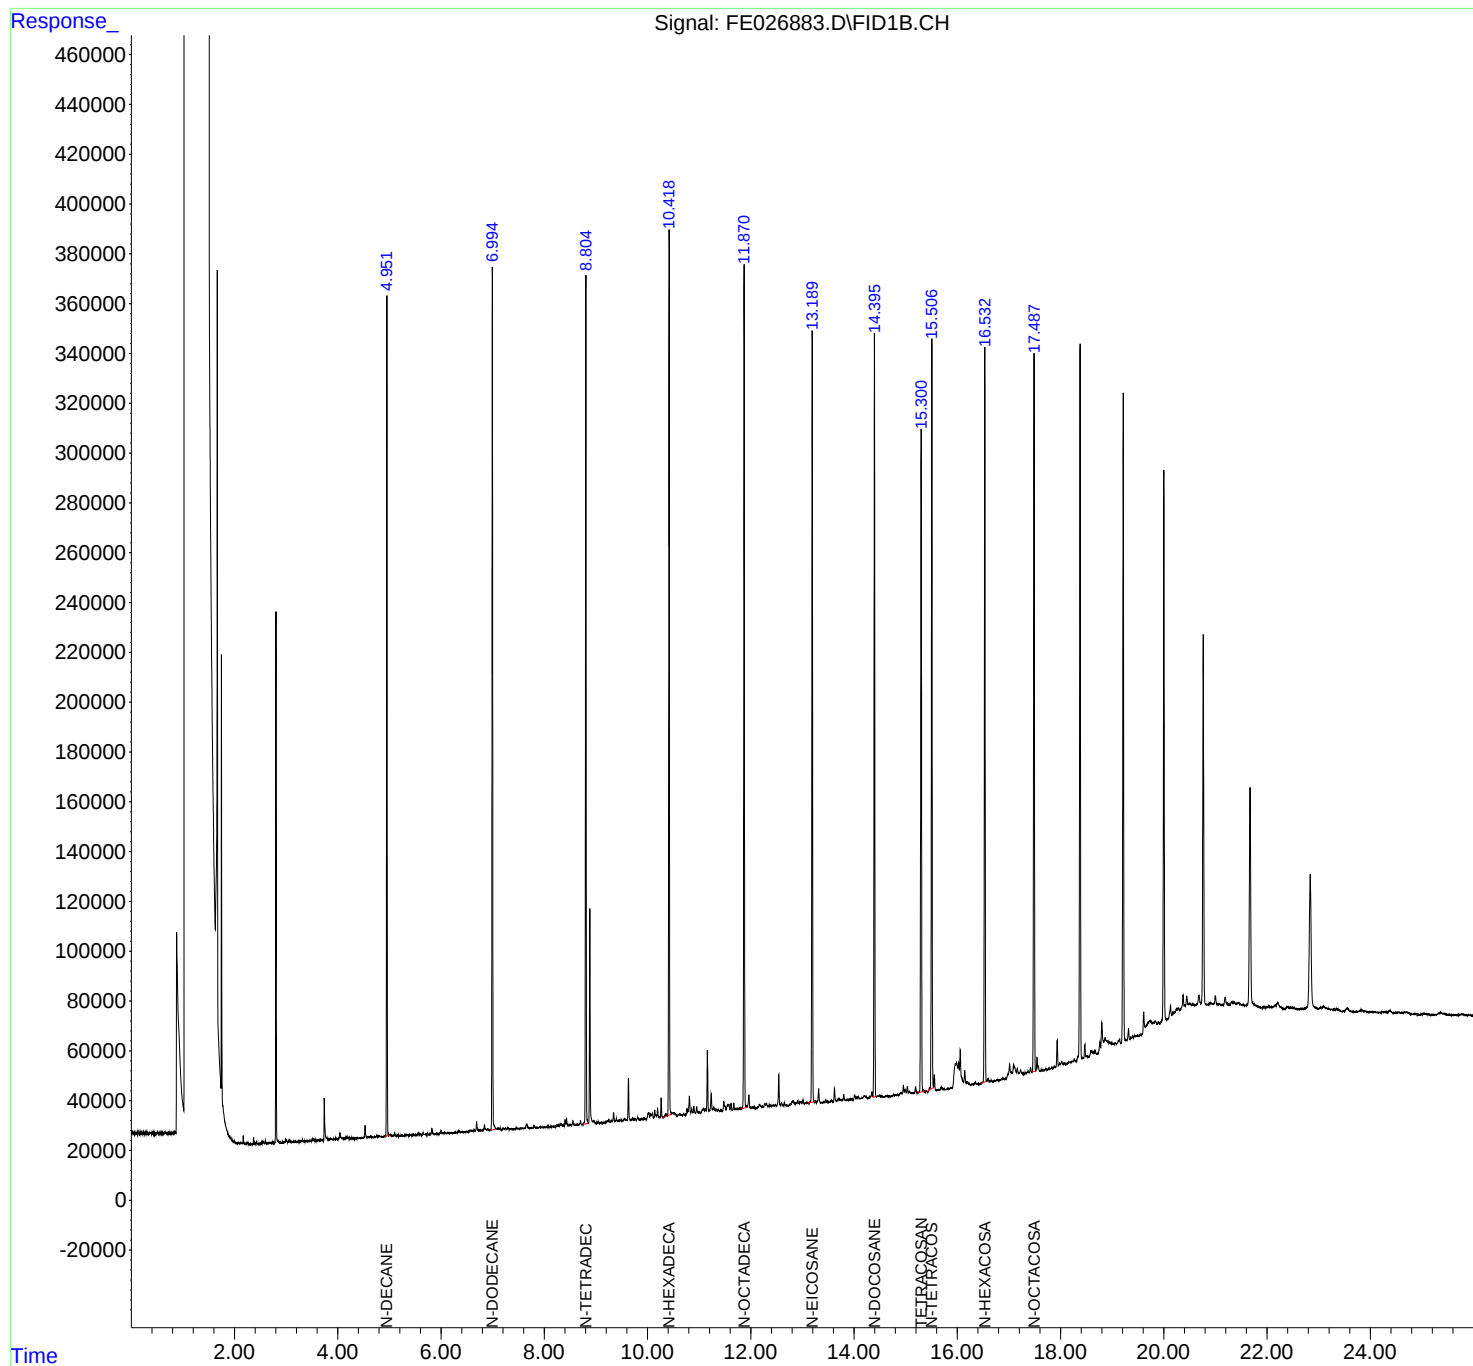


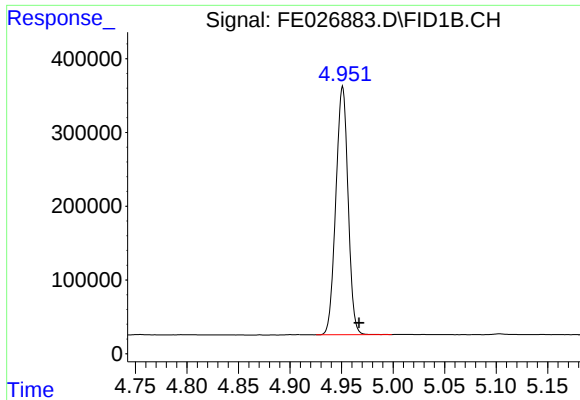

#2 N-DECANE


R.T.: 4.951 min
Delta R.T.: -0.016 min
Response: 2776305
Conc: 16.17 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-6A(0-5)MS

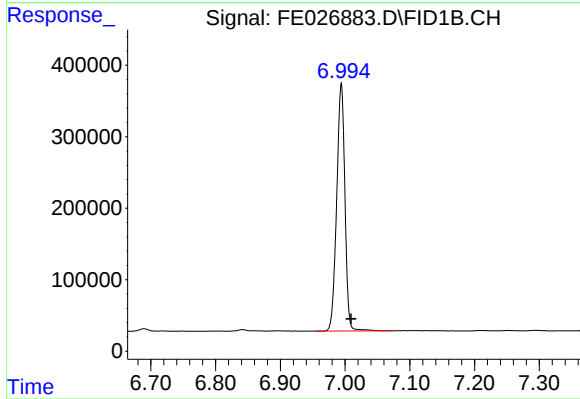


#3 N-DODECANE

R.T.: 6.994 min
Delta R.T.: -0.015 min
Response: 3062250
Conc: 16.30 ug/ml

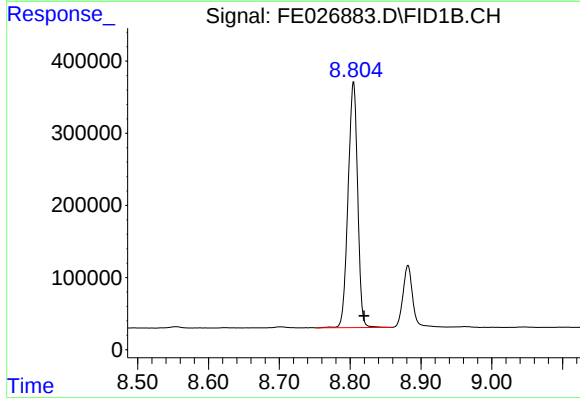


#4 N-TETRADECANE

R.T.: 8.805 min
Delta R.T.: -0.015 min
Response: 3189105
Conc: 15.55 ug/ml

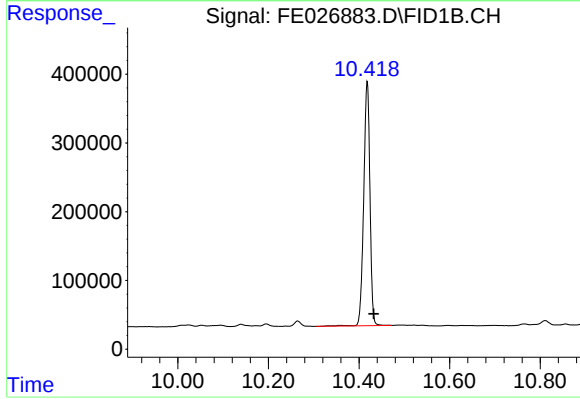

#5 N-HEXADECANE


R.T.: 10.418 min
Delta R.T.: -0.015 min
Response: 3383087
Conc: 15.27 ug/ml

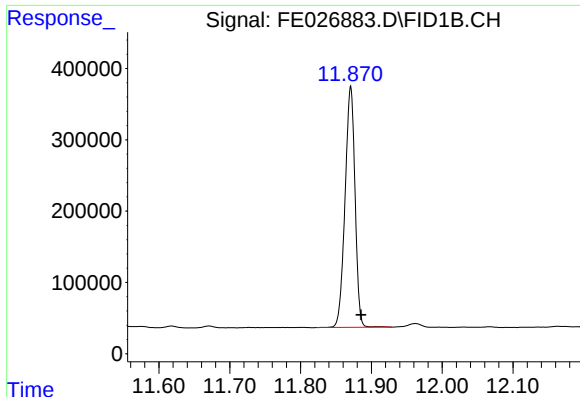

#6 N-OCTADECANE


R.T.: 11.871 min
Delta R.T.: -0.015 min
Response: 3306389
Conc: 14.14 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-6A(0-5)MS

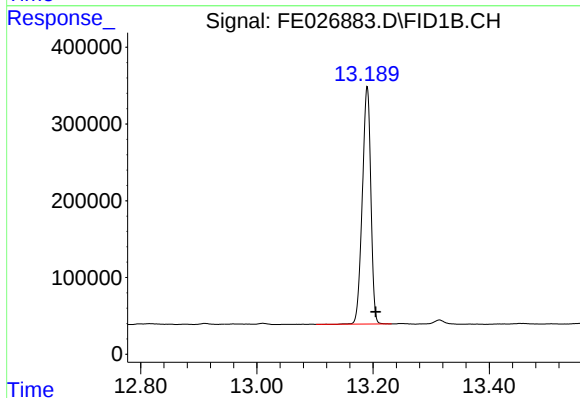


#7 N-EICOSANE

R.T.: 13.190 min
Delta R.T.: -0.015 min
Response: 3139860
Conc: 13.47 ug/ml

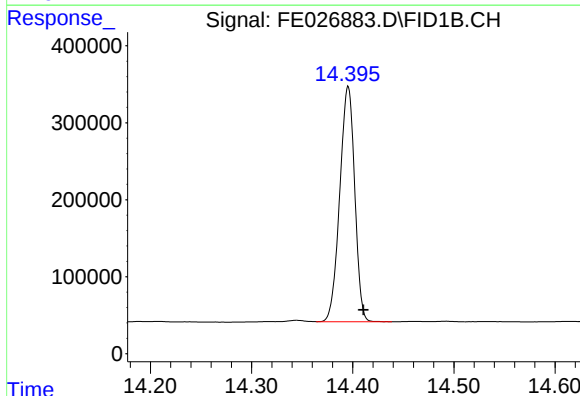


#8 N-DOCOSANE

R.T.: 14.395 min
Delta R.T.: -0.015 min
Response: 3144127
Conc: 13.68 ug/ml

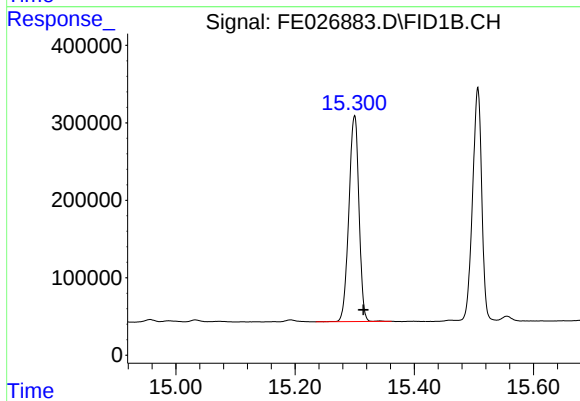

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.299 min
Delta R.T.: -0.015 min
Response: 3122169
Conc: 15.98 ug/ml

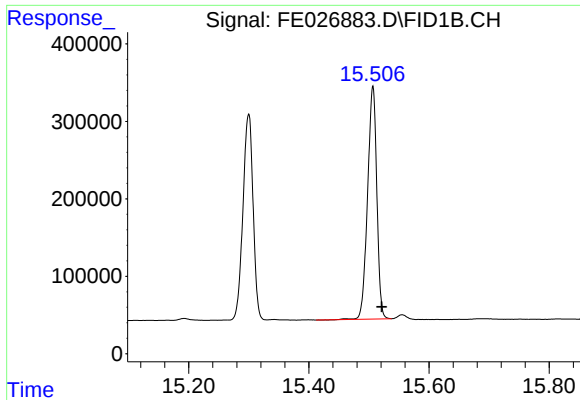

#10 N-TETRACOSANE


R.T.: 15.506 min
Delta R.T.: -0.015 min
Response: 3200509
Conc: 14.40 ug/ml

Instrument :
FID_E
ClientSampleId :
EPE-F-6A(0-5)MS

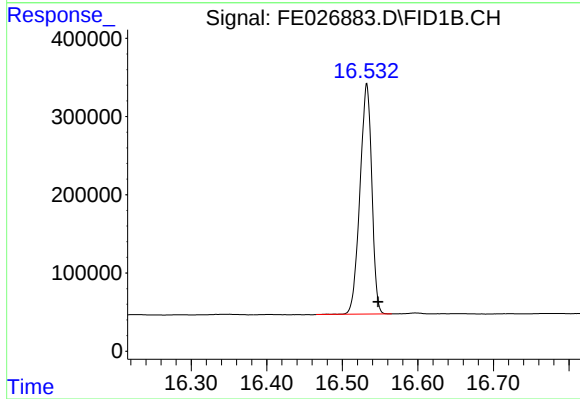

#11 N-HEXACOSANE

R.T.: 16.532 min
Delta R.T.: -0.015 min
Response: 3204581
Conc: 15.42 ug/ml

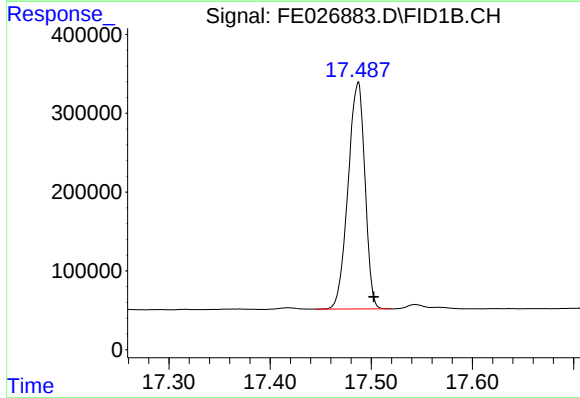

#12 N-OCTACOSANE

R.T.: 17.486 min
Delta R.T.: -0.016 min
Response: 3335713
Conc: 18.11 ug/ml