

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070518\
 Data File : FE028065.D
 Signal(s) : FID1B.CH
 Acq On : 05 Jul 2018 20:58
 Operator : AJ\MA
 Sample : J3814-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 06 09:47:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
 Quant Title :
 QLast Update : Tue Jun 26 18:10:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	15.030	3631968	10.884 ug/ml
Target Compounds			
6) N-TETRADECANE	8.618	1724685	8.663 ug/ml
9) N-EICOSANE	12.924	246225	0.890 ug/ml
10) N-TETRACOSANE	15.255	2586698	9.113 ug/ml
11) N-OCTACOSANE	17.210	460974	1.729 ug/ml
12) N-DOTRIACONTANE	18.937	877196	3.785 ug/ml
14) N-HEXATRIACONTANE	20.416	176462	0.956 ug/ml
15) N-TETRACONTANE	22.341	289450	1.715 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070518\
Data File : FE028065.D
Signal(s) : FID1B.CH
Acq On : 05 Jul 2018 20:58
Operator : AJ\MA
Sample : J3814-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 06 09:47:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
Quant Title :
QLast Update : Tue Jun 26 18:10:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

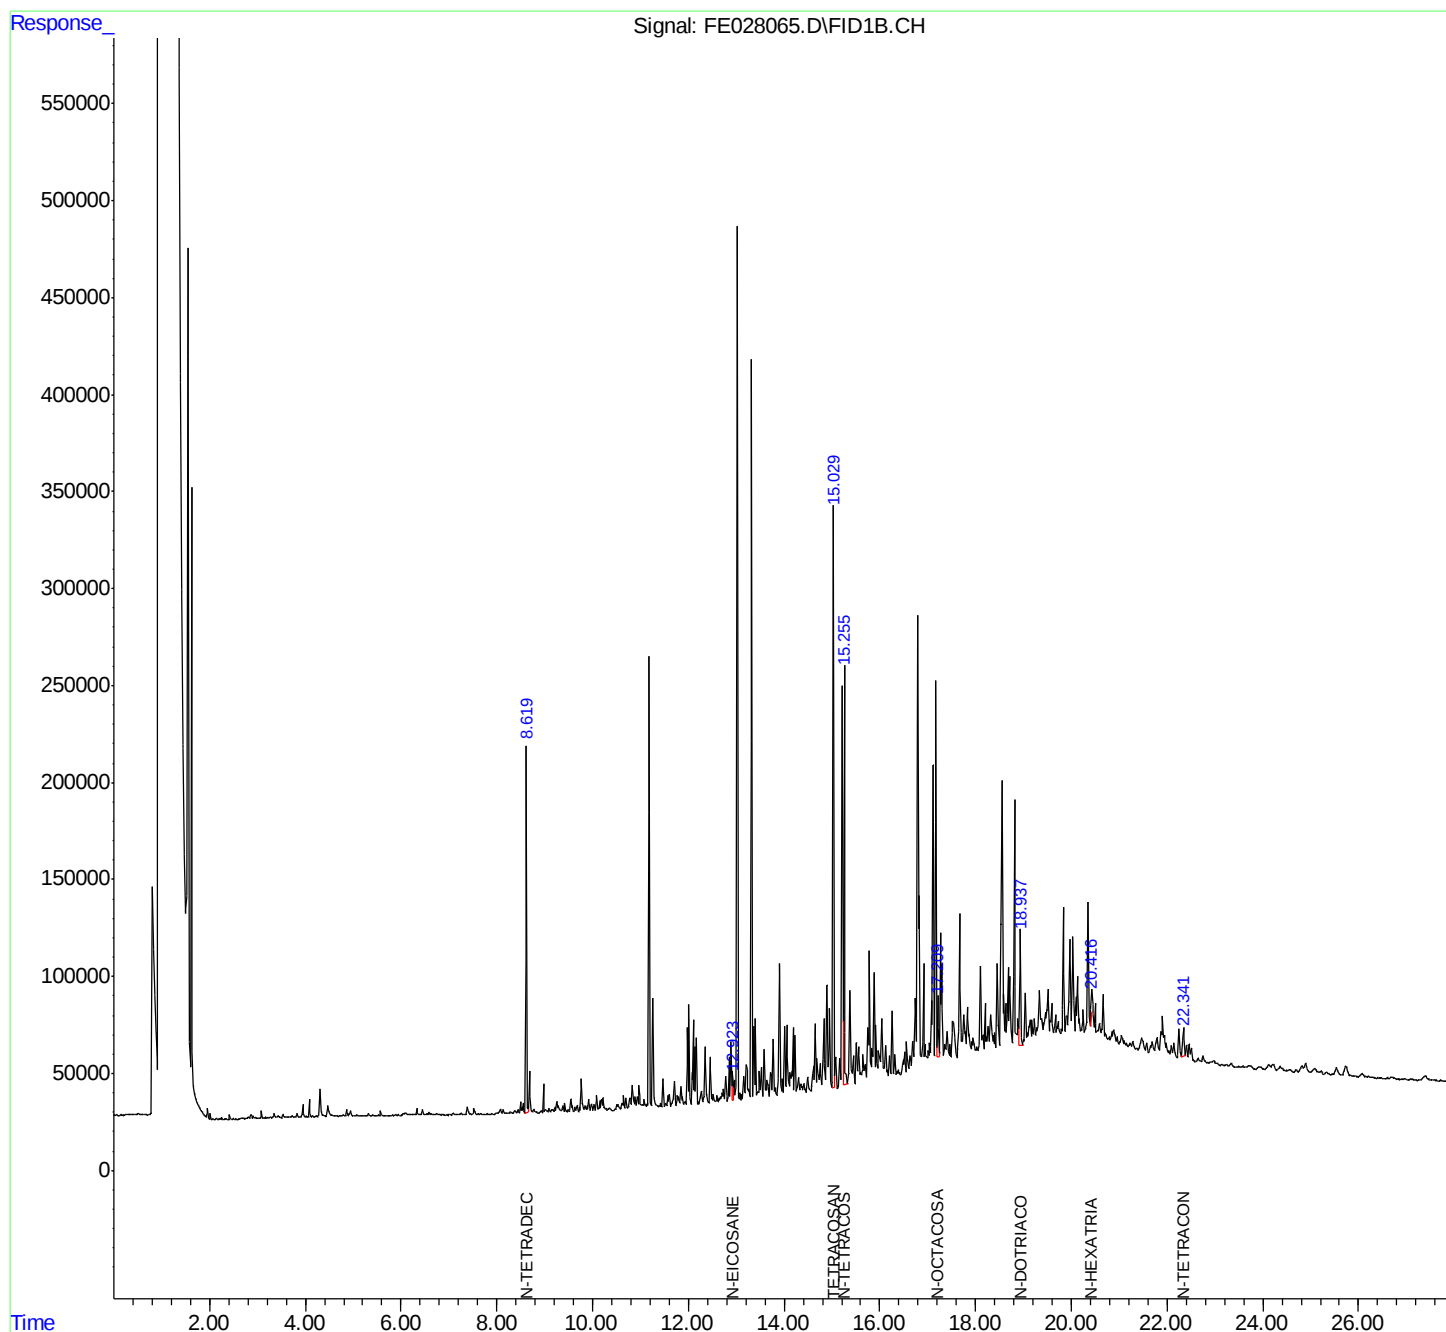

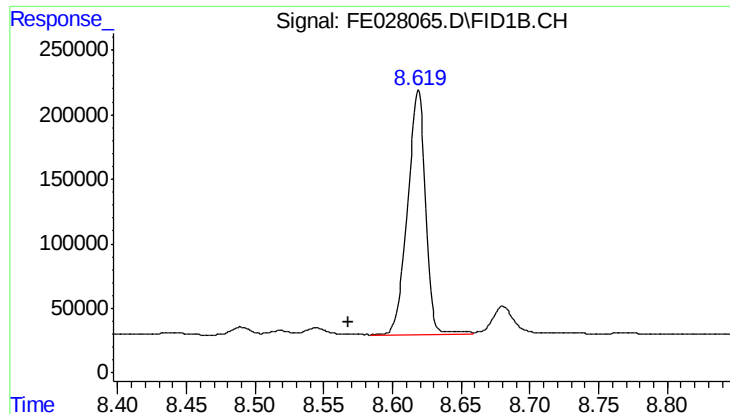


#6 N-TETRADECANE

R.T.: 8.618 min
Delta R.T.: 0.050 min
Response: 1724685
Conc: 8.66 ug/ml

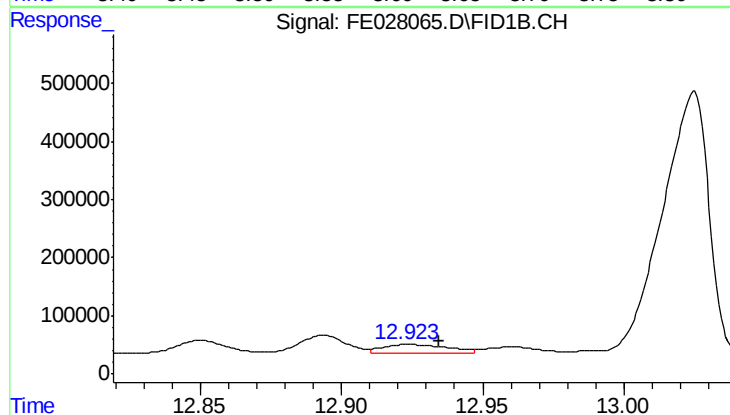


#9 N-EICOSANE

R.T.: 12.924 min
Delta R.T.: -0.010 min
Response: 246225
Conc: 0.89 ug/ml

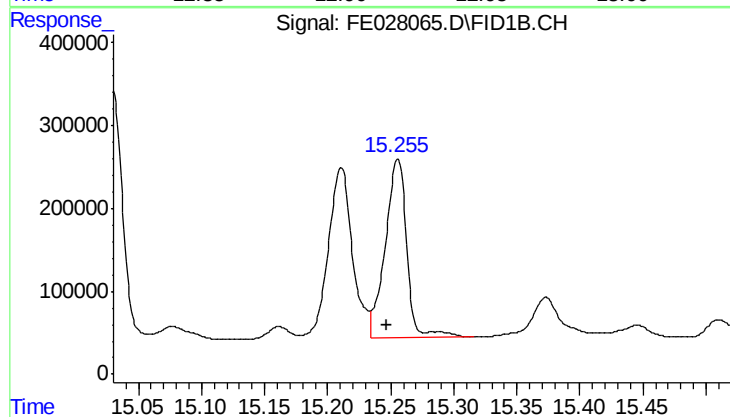


#10 N-TETRACOSANE

R.T.: 15.255 min
Delta R.T.: 0.008 min
Response: 2586698
Conc: 9.11 ug/ml

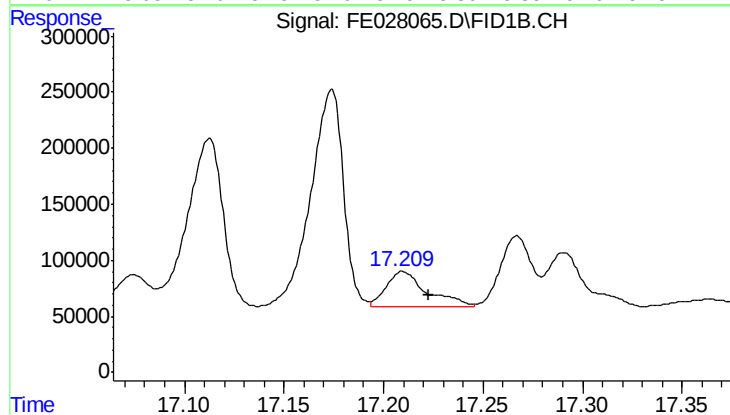


#11 N-OCTACOSANE

R.T.: 17.210 min
Delta R.T.: -0.013 min
Response: 460974
Conc: 1.73 ug/ml

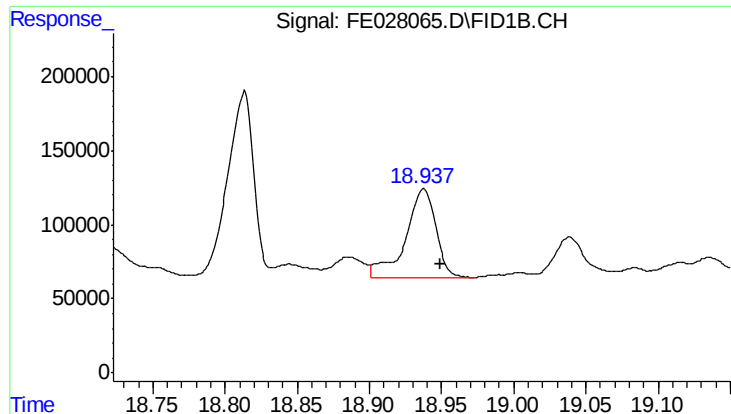


#12 N-DOTRIACONTANE

R.T.: 18.937 min
Delta R.T.: -0.012 min
Response: 877196
Conc: 3.78 ug/ml

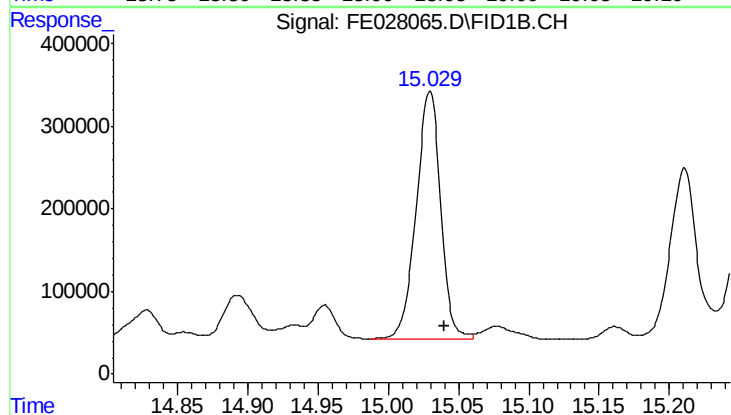


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.030 min
Delta R.T.: -0.010 min
Response: 3631968
Conc: 10.88 ug/ml

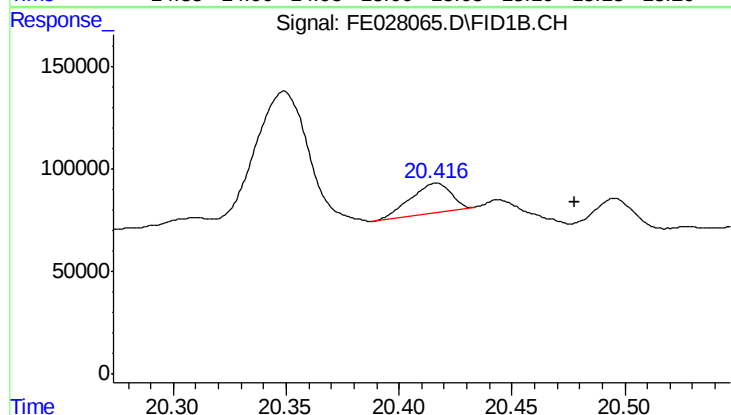

#14 N-HEXATRIACONTANE

R.T.: 20.416 min
Delta R.T.: -0.061 min
Response: 176462
Conc: 0.96 ug/ml

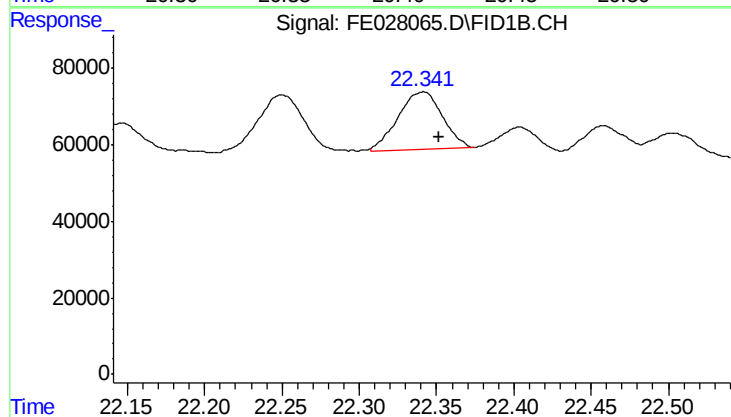

#15 N-TETRACONTANE

R.T.: 22.341 min
Delta R.T.: -0.011 min
Response: 289450
Conc: 1.71 ug/ml