

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070518\
 Data File : FE028077.D
 Signal(s) : FID1B.CH
 Acq On : 06 Jul 2018 5:04
 Operator : AJ\MA
 Sample : J3852-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 06 09:49:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
 Quant Title :
 QLast Update : Tue Jun 26 18:10:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	15.031	4180959	12.529 ug/ml
Target Compounds			
6) N-TETRADECANE	8.624	3170680	15.926 ug/ml
7) N-HEXADECANE	10.152	201380	0.874 ug/ml
8) N-OCTADECANE	11.603	194996	0.756 ug/ml
10) N-TETRACOSANE	15.246	272781	0.961 ug/ml
11) N-OCTACOSANE	17.211	585464	2.196 ug/ml
12) N-DOTRIACONTANE	18.937	795791	3.434 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070518\
Data File : FE028077.D
Signal(s) : FID1B.CH
Acq On : 06 Jul 2018 5:04
Operator : AJ\MA
Sample : J3852-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 06 09:49:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
Quant Title :
QLast Update : Tue Jun 26 18:10:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

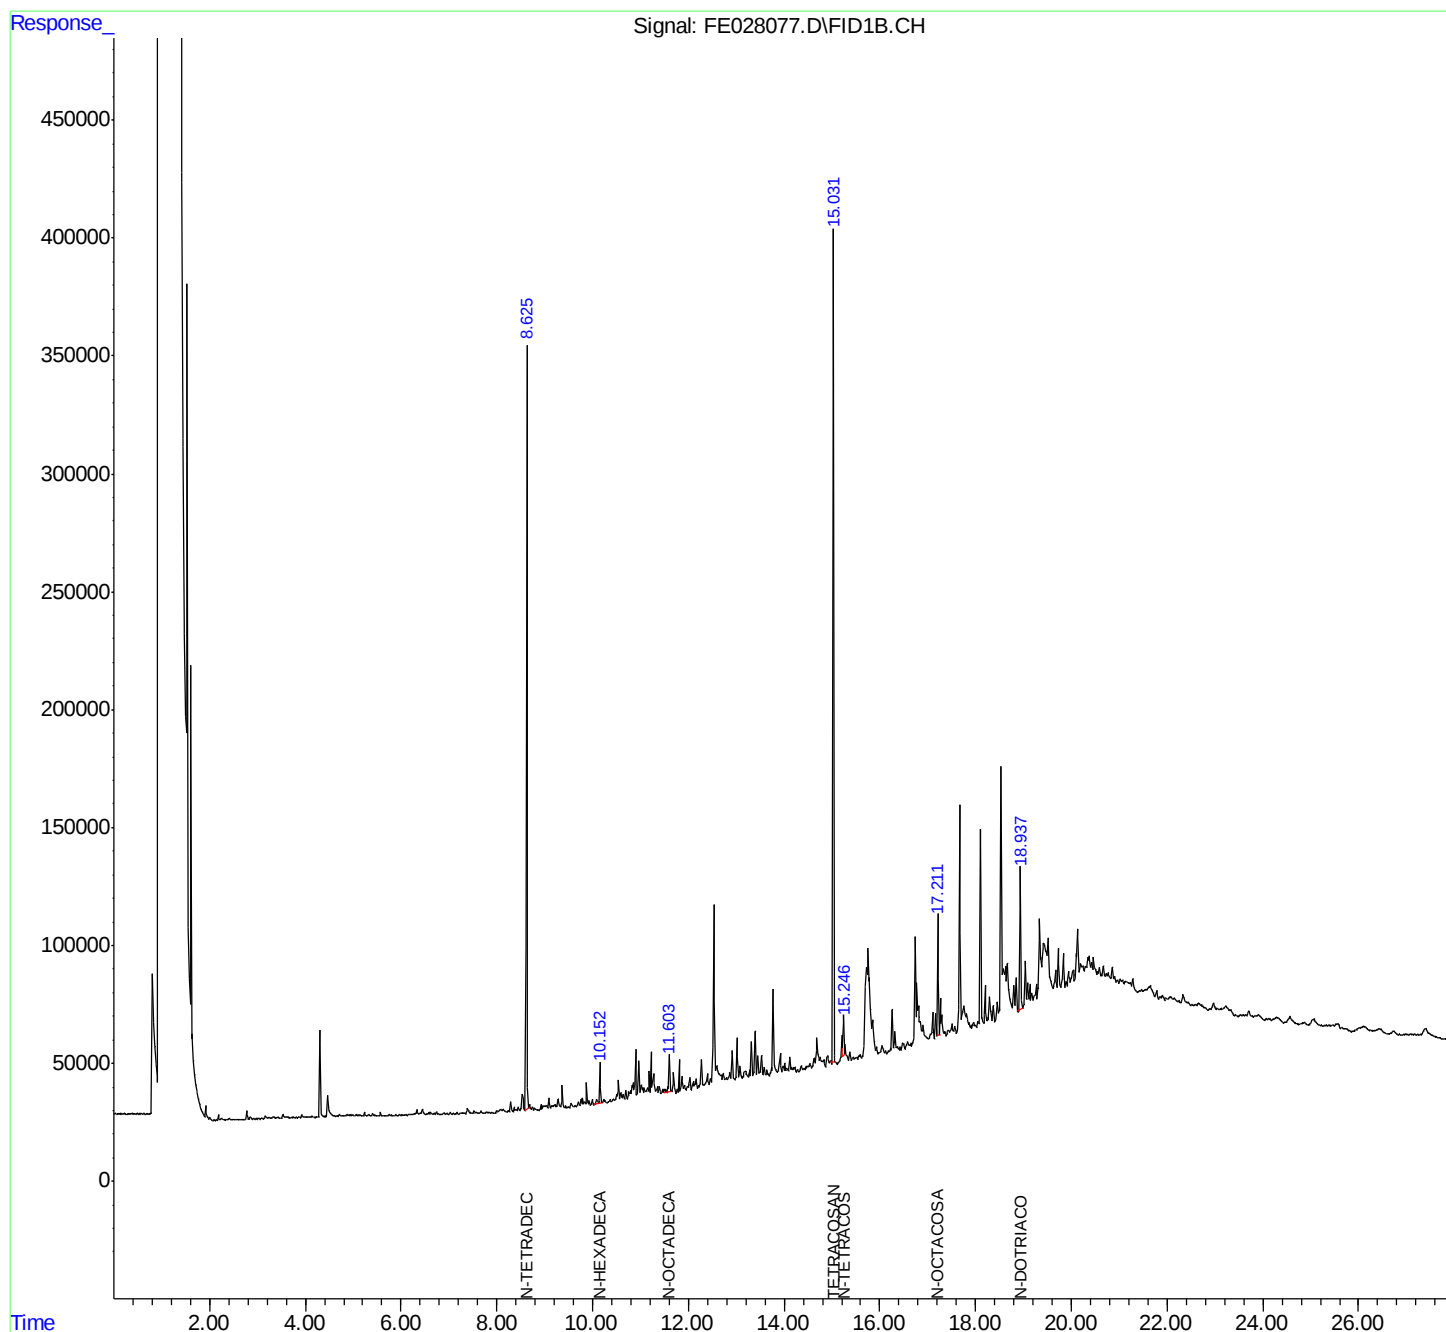

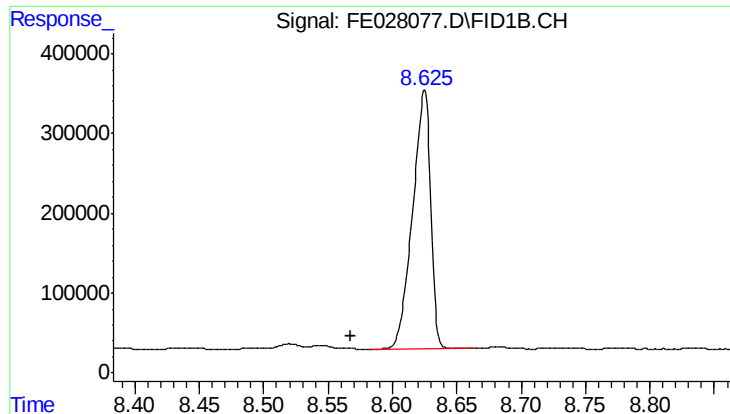


#6 N-TETRADECANE

R.T.: 8.624 min
Delta R.T.: 0.056 min
Response: 3170680
Conc: 15.93 ug/ml

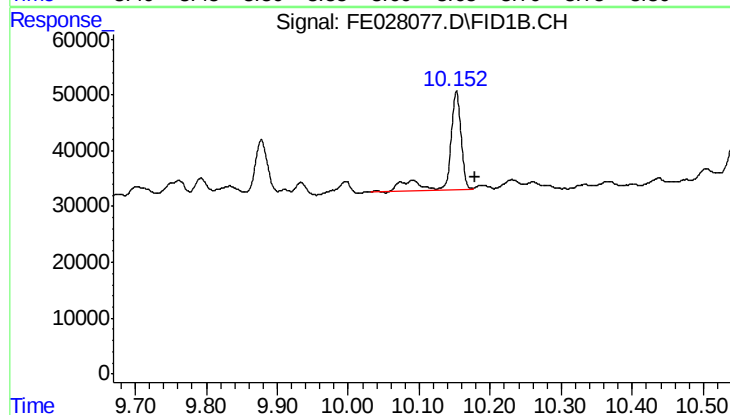


#7 N-HEXADECANE

R.T.: 10.152 min
Delta R.T.: -0.027 min
Response: 201380
Conc: 0.87 ug/ml

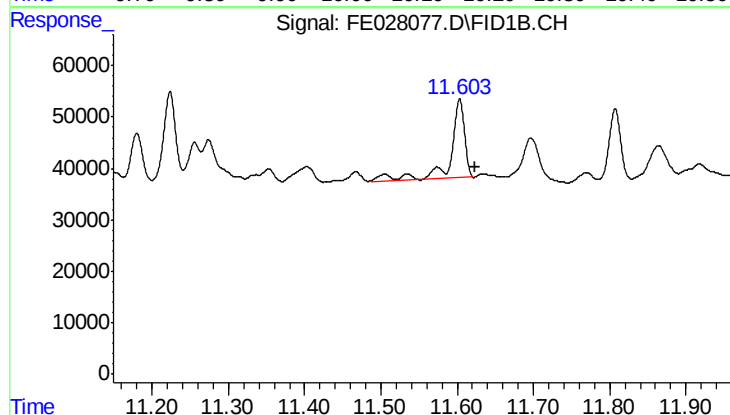


#8 N-OCTADECANE

R.T.: 11.603 min
Delta R.T.: -0.020 min
Response: 194996
Conc: 0.76 ug/ml

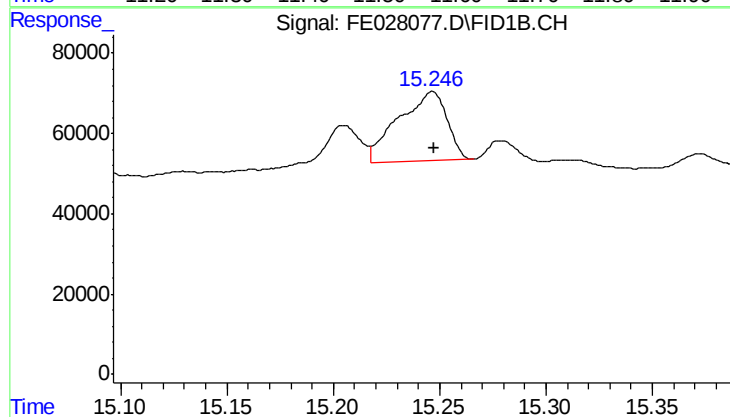


#10 N-TETRACOSANE

R.T.: 15.246 min
Delta R.T.: 0.000 min
Response: 272781
Conc: 0.96 ug/ml

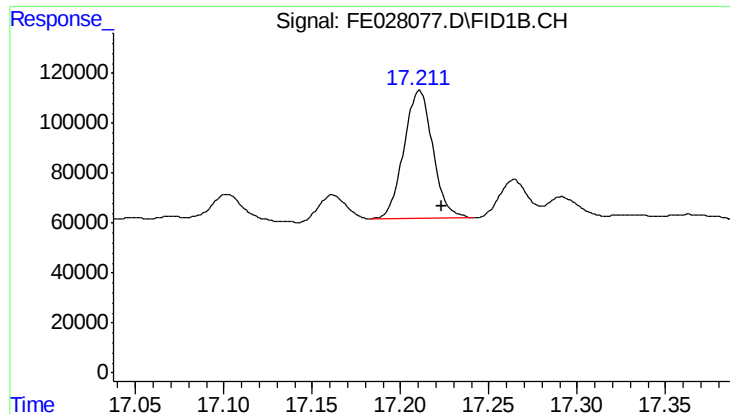


#11 N-OCTACOSANE

R.T.: 17.211 min
Delta R.T.: -0.013 min
Response: 585464
Conc: 2.20 ug/ml

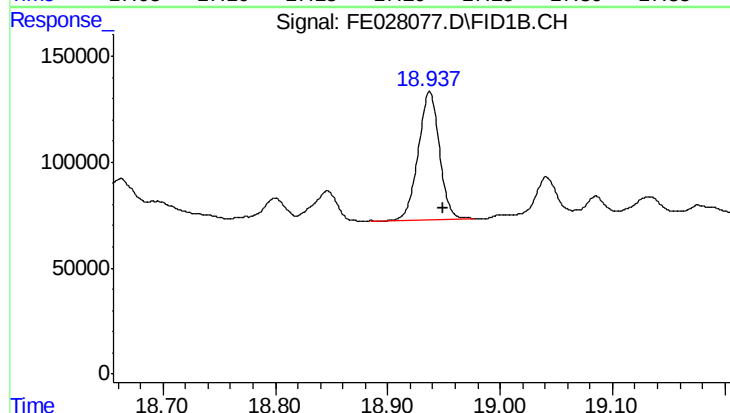

#12 N-DOTRIACONTANE

R.T.: 18.937 min
Delta R.T.: -0.012 min
Response: 795791
Conc: 3.43 ug/ml

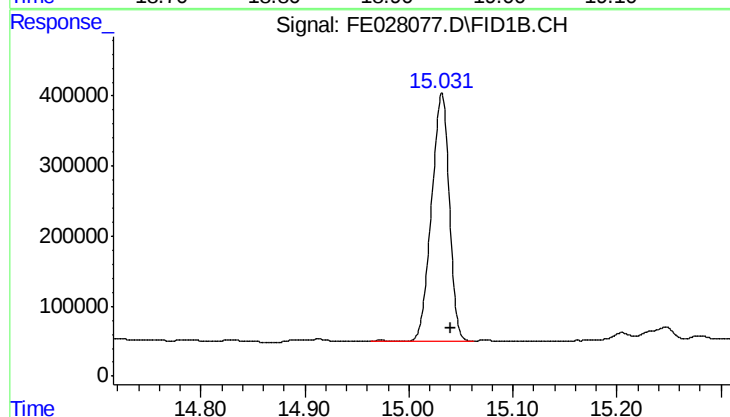

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.031 min
Delta R.T.: -0.008 min
Response: 4180959
Conc: 12.53 ug/ml