

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092519\
 Data File : FE030552.D
 Signal(s) : FID1B.CH
 Acq On : 25 Sep 2019 13:58
 Operator : DD\AJ
 Sample : K3591-01
 Misc : LOD 1 PPM
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 26 00:42:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
 Quant Title :
 QLast Update : Wed Sep 25 02:50:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.680	841626	2.715 ug/ml
Target Compounds			
2) N-DECANE	4.416	485685	1.272 ug/ml
3) N-DODECANE	6.428	490160	1.281 ug/ml
4) N-TETRADECANE	8.223	481200	1.280 ug/ml
5) N-HEXADECANE	9.825	474130	1.270 ug/ml
6) N-OCTADECANE	11.268	472975	1.291 ug/ml
7) N-EICOSANE	12.580	463998	1.272 ug/ml
8) N-DOCOSANE	13.779	460475	1.283 ug/ml
10) N-TETRACOSANE	14.883	465474	1.309 ug/ml
11) N-HEXACOSANE	15.905	458973	1.310 ug/ml
12) N-OCTACOSANE	16.856	517518	1.504 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092519\
 Data File : FE030552.D
 Signal(s) : FID1B.CH
 Acq On : 25 Sep 2019 13:58
 Operator : DD\AJ
 Sample : K3591-01
 Misc : LOD 1 PPM
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 26 00:42:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE092419.M
 Quant Title :
 QLast Update : Wed Sep 25 02:50:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

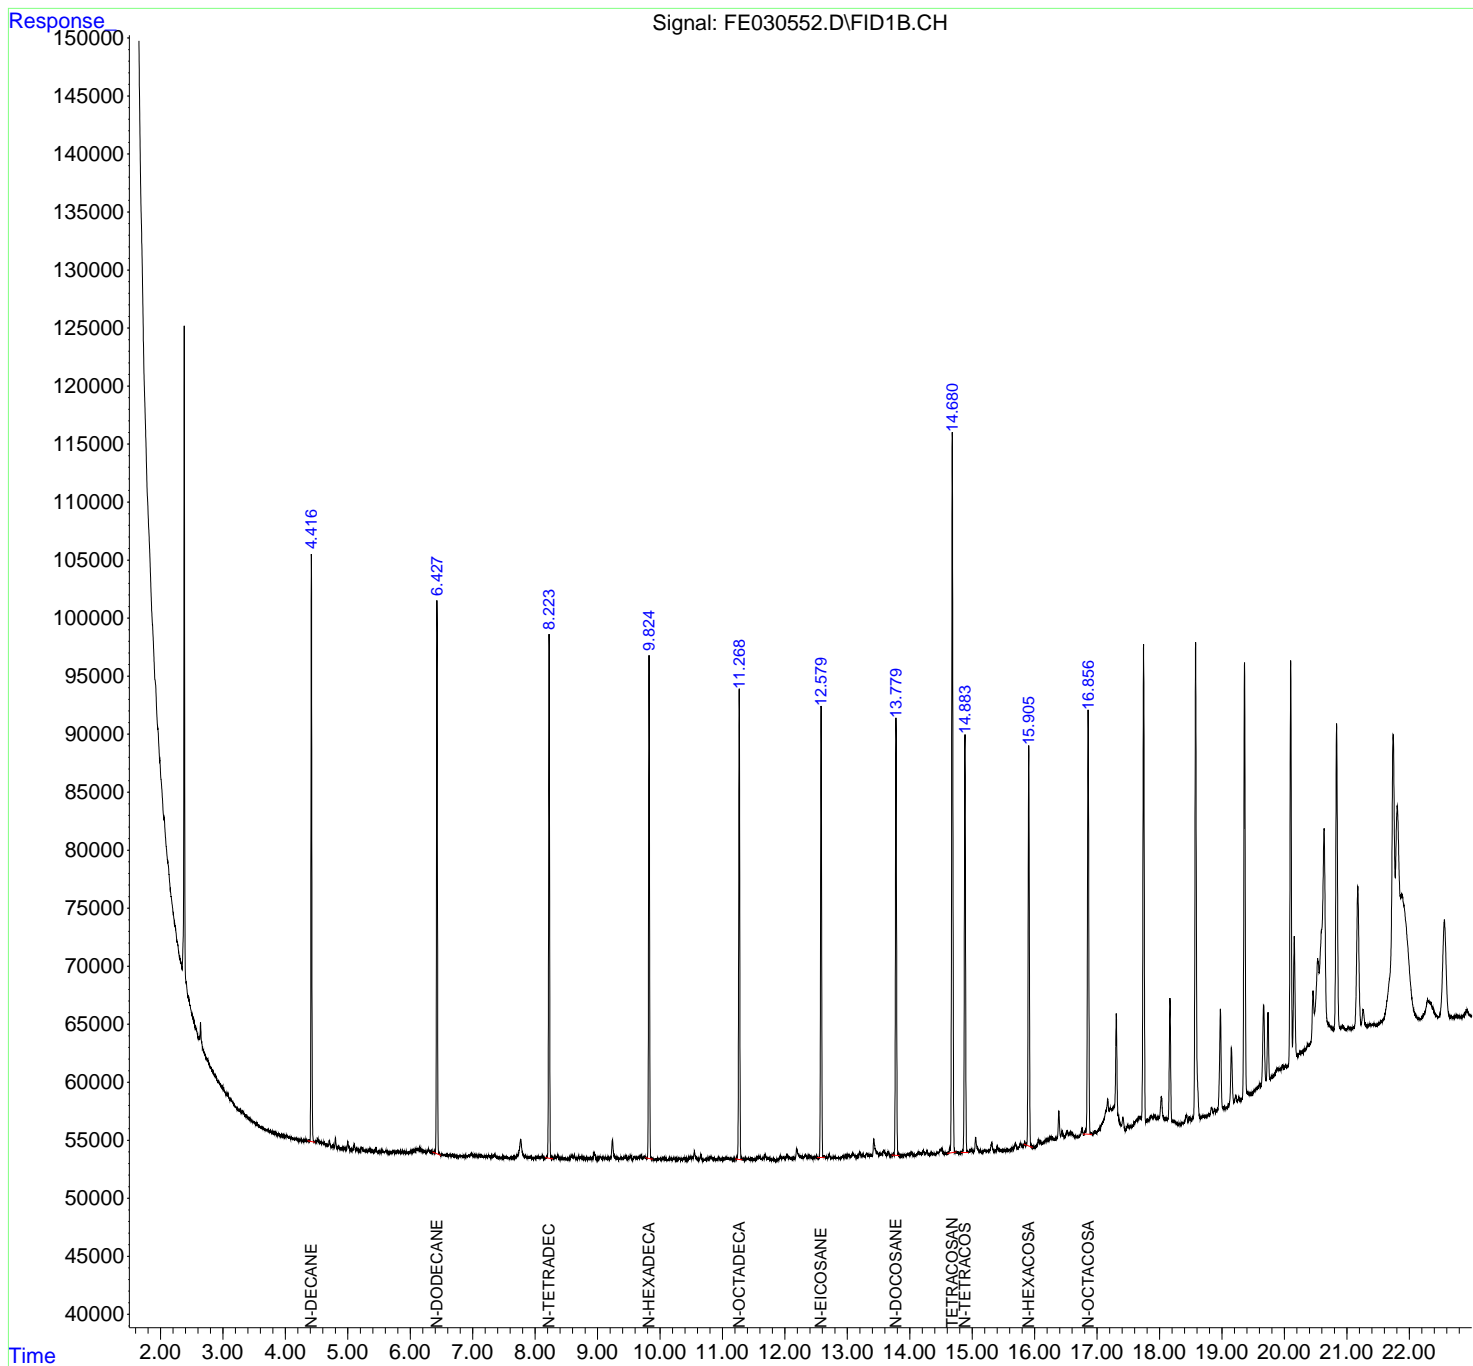

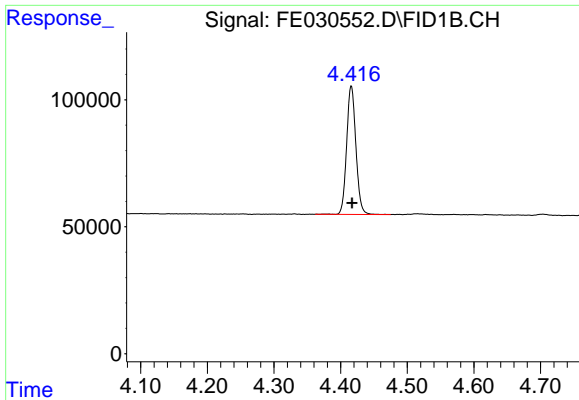


#2 N-DECANE

R.T.: 4.416 min
Delta R.T.: -0.001 min
Response: 485685
Conc: 1.27 ug/ml

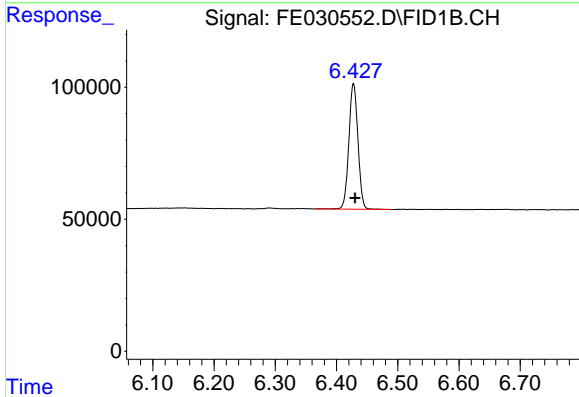


#3 N-DODECANE

R.T.: 6.428 min
Delta R.T.: -0.002 min
Response: 490160
Conc: 1.28 ug/ml

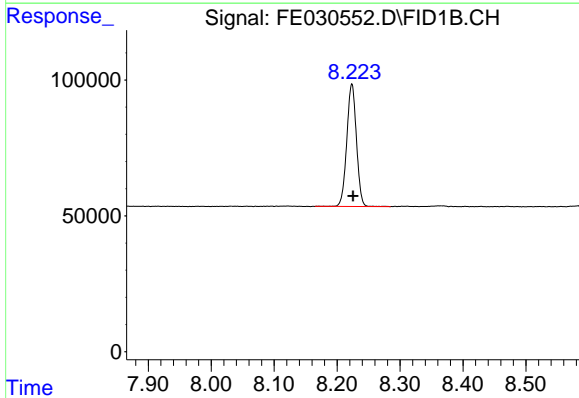


#4 N-TETRADECANE

R.T.: 8.223 min
Delta R.T.: -0.002 min
Response: 481200
Conc: 1.28 ug/ml

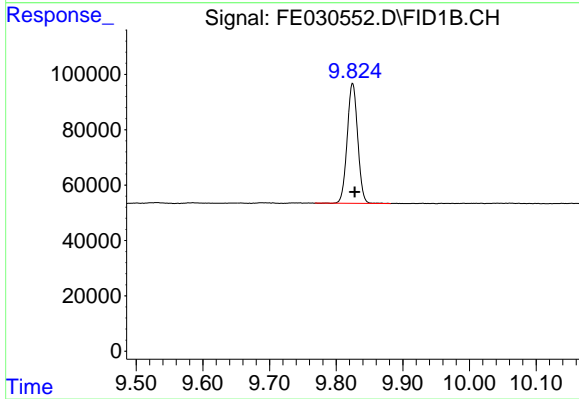


#5 N-HEXADECANE

R.T.: 9.825 min
Delta R.T.: -0.003 min
Response: 474130
Conc: 1.27 ug/ml

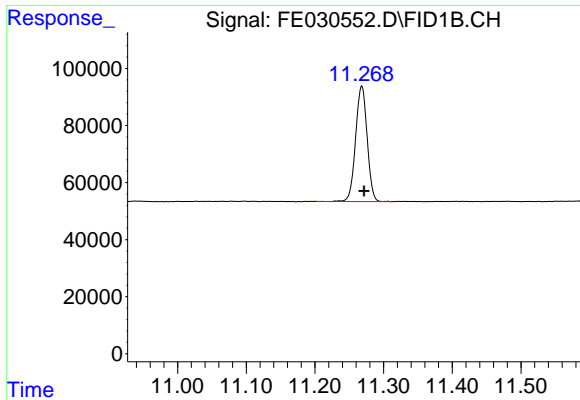


#6 N-OCTADECANE

R.T.: 11.268 min
Delta R.T.: -0.003 min
Response: 472975
Conc: 1.29 ug/ml

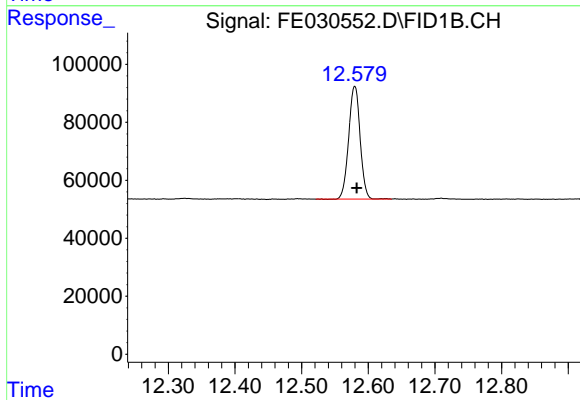


#7 N-EICOSANE

R.T.: 12.580 min
Delta R.T.: -0.003 min
Response: 463998
Conc: 1.27 ug/ml

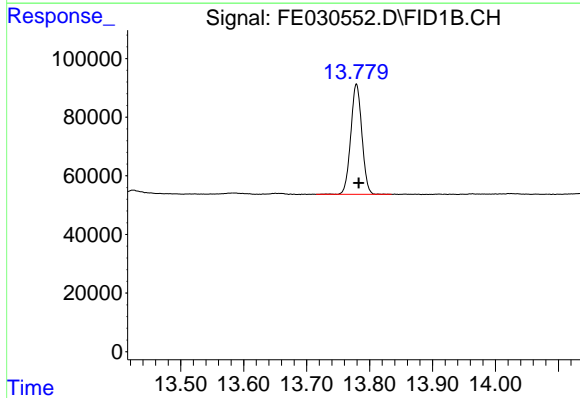


#8 N-DOCOSANE

R.T.: 13.779 min
Delta R.T.: -0.004 min
Response: 460475
Conc: 1.28 ug/ml

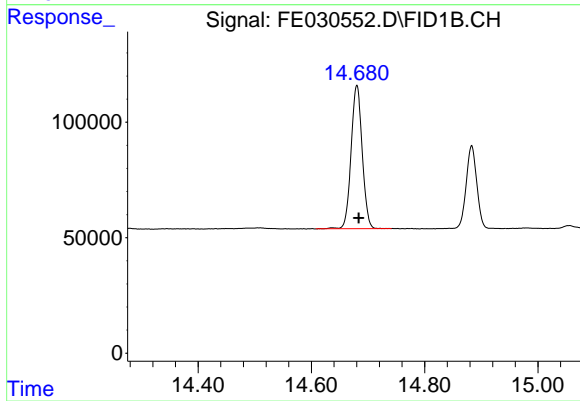


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.680 min
Delta R.T.: -0.003 min
Response: 841626
Conc: 2.71 ug/ml

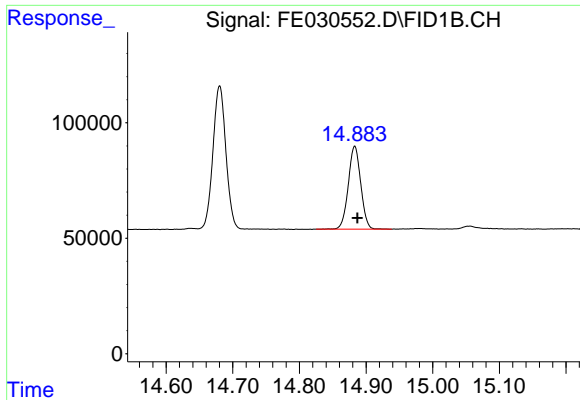


#10 N-TETRACOSANE

R.T.: 14.883 min
Delta R.T.: -0.004 min
Response: 465474
Conc: 1.31 ug/ml

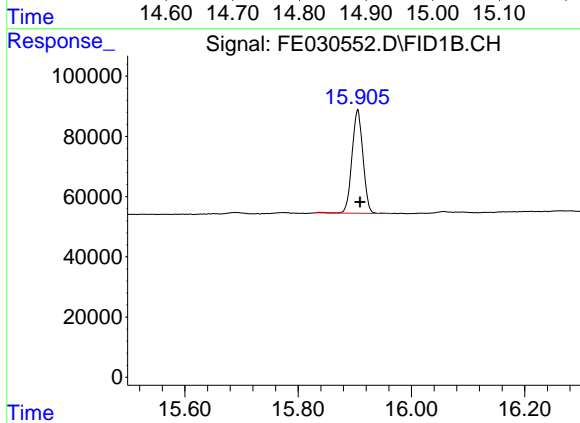

#11 N-HEXACOSANE

R.T.: 15.905 min
Delta R.T.: -0.004 min
Response: 458973
Conc: 1.31 ug/ml

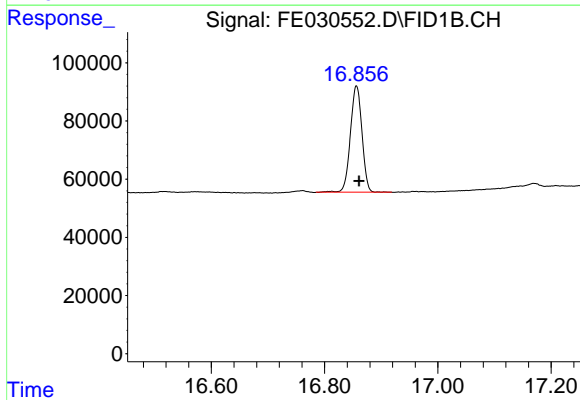

#12 N-OCTACOSANE

R.T.: 16.856 min
Delta R.T.: -0.005 min
Response: 517518
Conc: 1.50 ug/ml