

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010319\
 Data File : FG003370.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jan 2019 20:01
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Jan 04 00:01:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
 Quant Title :
 QLast Update : Thu Dec 13 00:59:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.701	5584920	45.029 ug/ml
Target Compounds			
2) N-DECANE	4.405	7122735	53.088 ug/ml
3) N-DODECANE	6.432	7151180	52.563 ug/ml
4) N-TETRADECANE	8.232	7134685	51.699 ug/ml
5) N-HEXADECANE	9.837	7062261	50.408 ug/ml
6) N-OCTADECANE	11.282	6929127	48.907 ug/ml
7) N-EICOSANE	12.595	6674193	47.243 ug/ml
8) N-DOCOSANE	13.798	6411673	45.586 ug/ml
10) N-TETRACOSANE	14.906	6176829	44.129 ug/ml
11) N-HEXACOSANE	15.930	6028219	43.250 ug/ml
12) N-OCTACOSANE	16.884	5968566	42.712 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010319\
Data File : FG003370.D
Signal(s) : FID1A.ch
Acq On : 03 Jan 2019 20:01
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: Sample.e
Quant Time: Jan 04 00:01:57 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
Quant Title :
QLast Update : Thu Dec 13 00:59:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

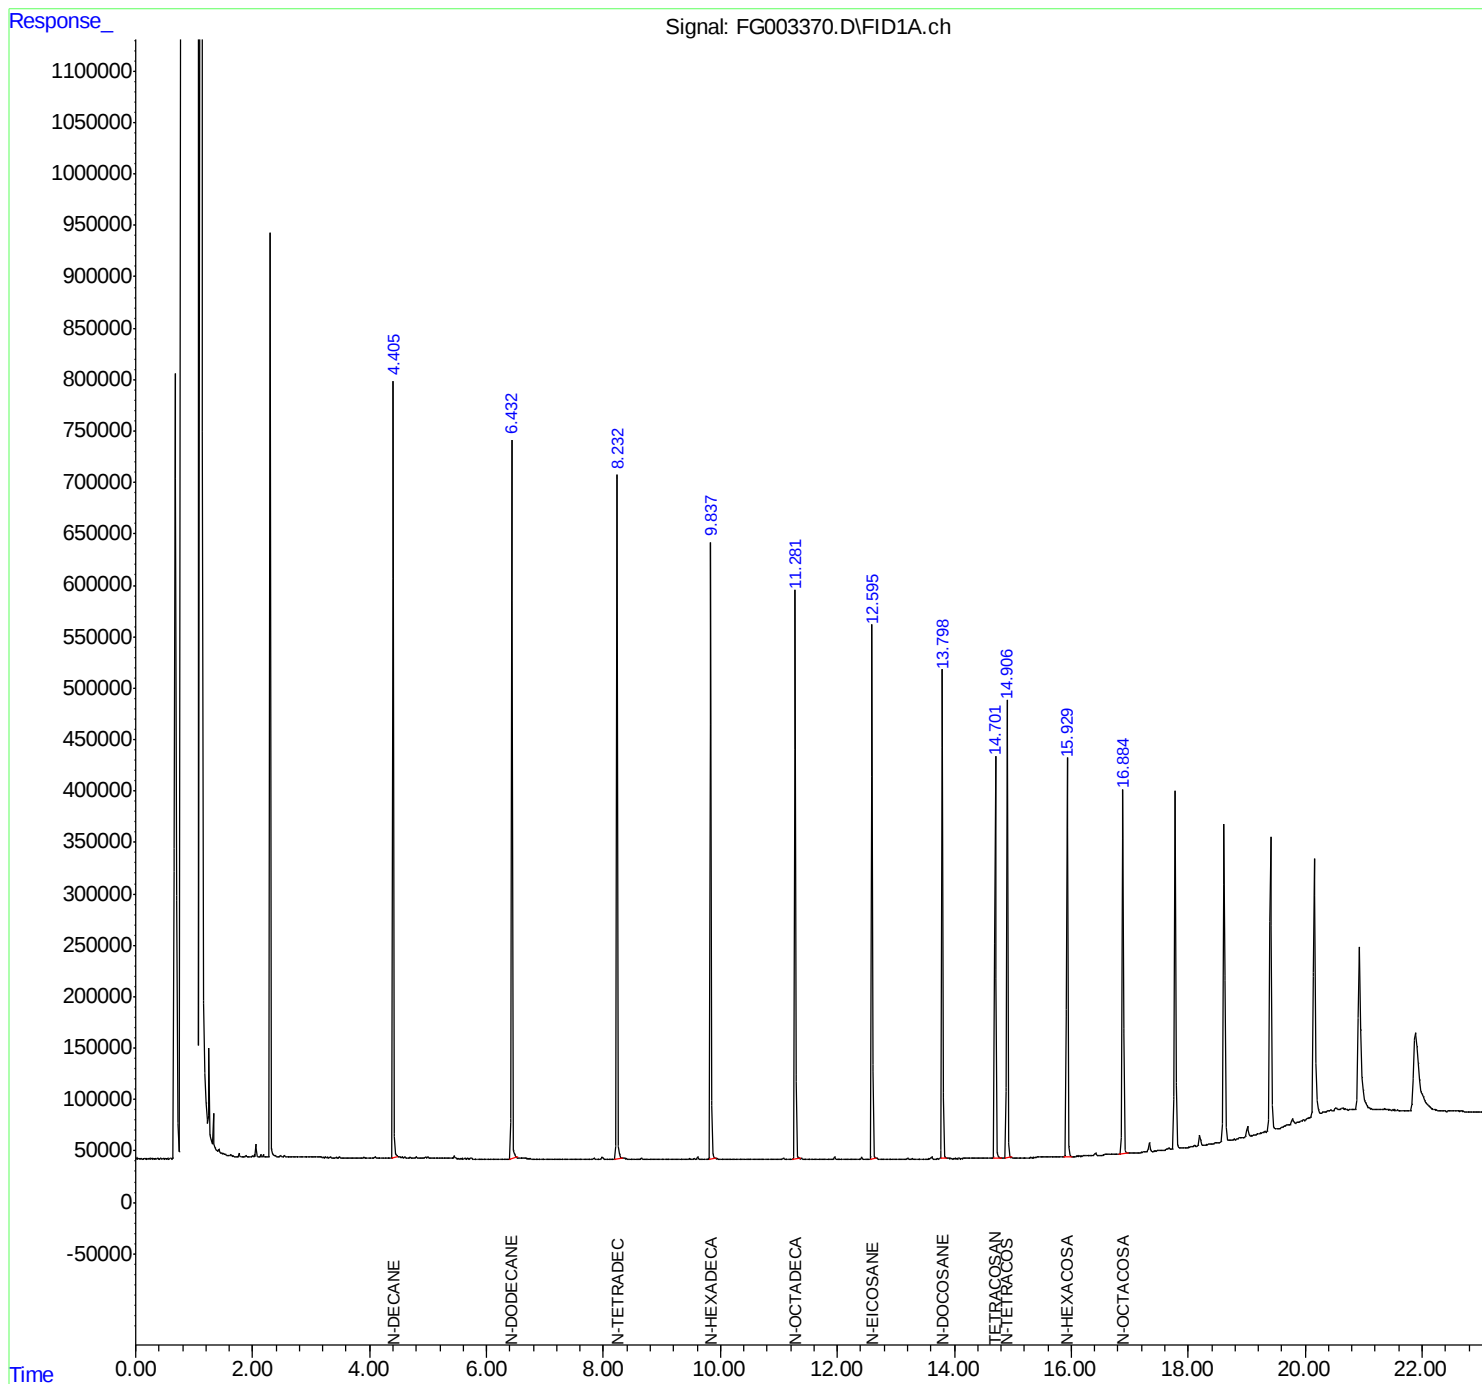


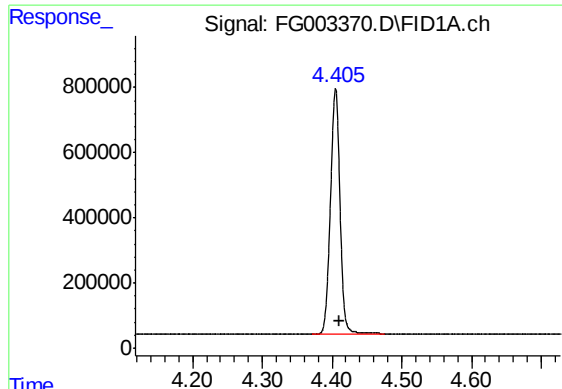

#2 N-DECANE


R.T.: 4.405 min
Delta R.T.: -0.006 min
Response: 7122735
Conc: 53.09 ug/ml

Instrument :
FID_G
ClientSampleId :

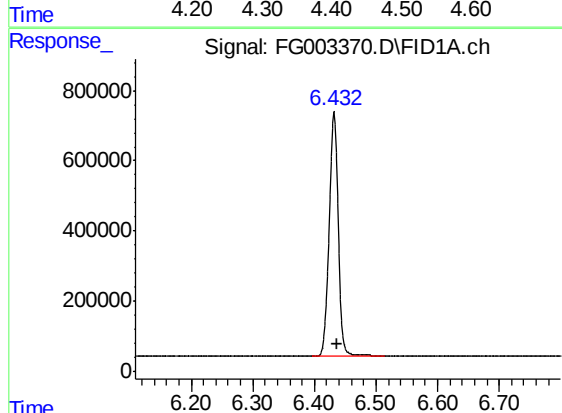


#3 N-DODECANE

R.T.: 6.432 min
Delta R.T.: -0.004 min
Response: 7151180
Conc: 52.56 ug/ml

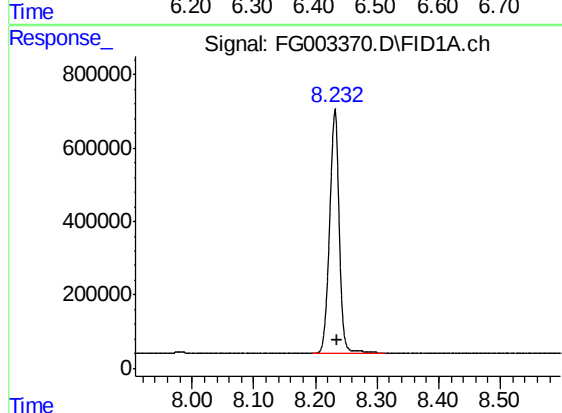


#4 N-TETRADECANE

R.T.: 8.232 min
Delta R.T.: -0.003 min
Response: 7134685
Conc: 51.70 ug/ml

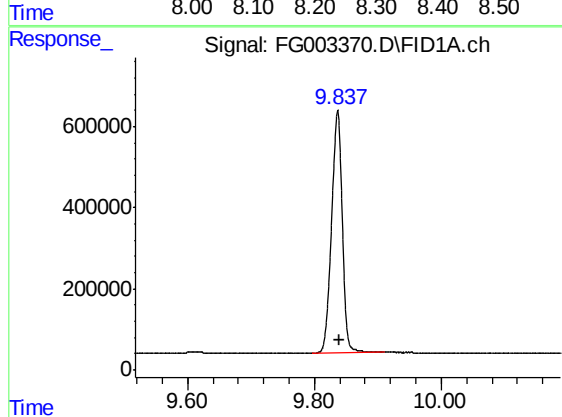

#5 N-HEXADECANE


R.T.: 9.837 min
Delta R.T.: -0.003 min
Response: 7062261
Conc: 50.41 ug/ml

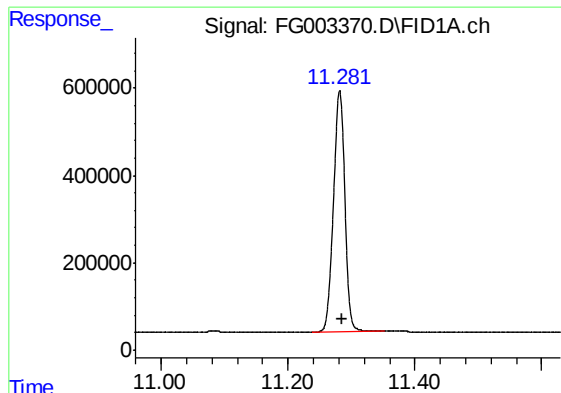

#6 N-OCTADECANE


R.T.: 11.282 min
Delta R.T.: -0.003 min
Response: 6929127
Conc: 48.91 ug/ml

Instrument :
FID_G
ClientSampleId :

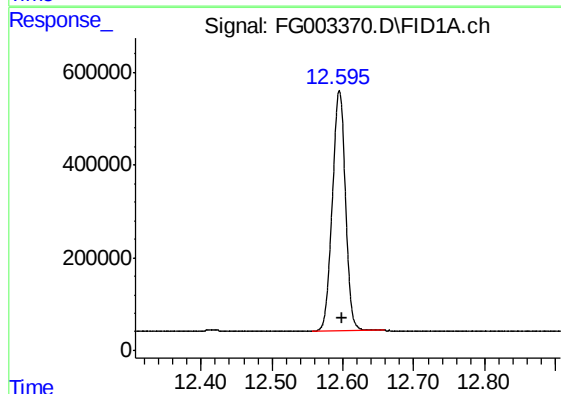


#7 N-EICOSANE

R.T.: 12.595 min
Delta R.T.: -0.003 min
Response: 6674193
Conc: 47.24 ug/ml

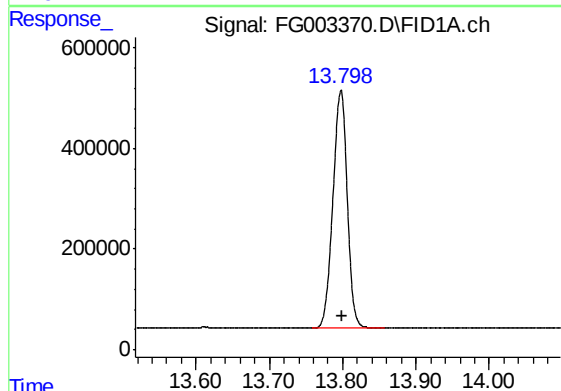


#8 N-DOCOSANE

R.T.: 13.798 min
Delta R.T.: -0.002 min
Response: 6411673
Conc: 45.59 ug/ml

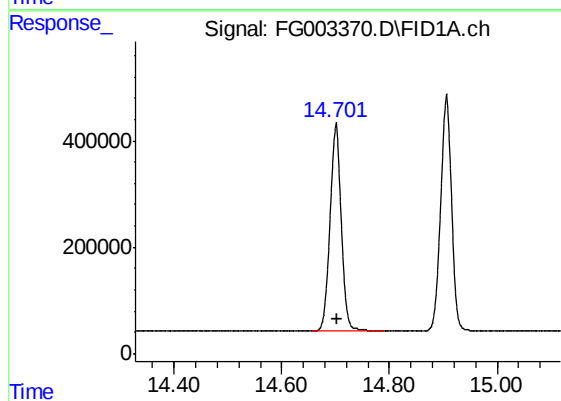

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.701 min
Delta R.T.: 0.000 min
Response: 5584920
Conc: 45.03 ug/ml

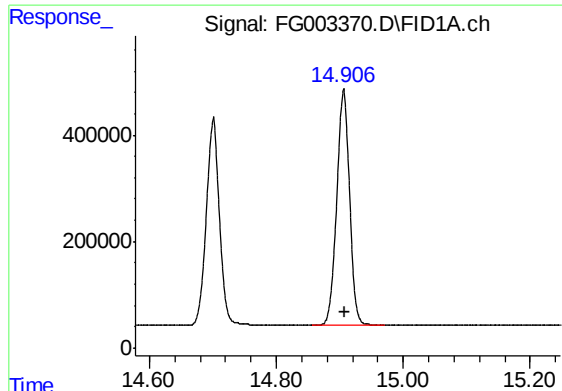

#10 N-TETRACOSANE


R.T.: 14.906 min
Delta R.T.: 0.000 min
Response: 6176829
Conc: 44.13 ug/ml

Instrument :
FID_G
ClientSampleId :

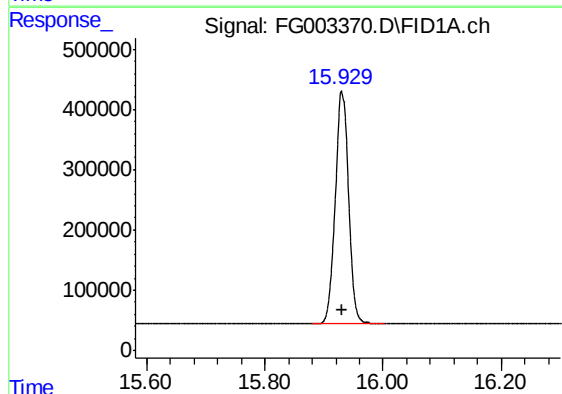

#11 N-HEXACOSANE

R.T.: 15.930 min
Delta R.T.: -0.002 min
Response: 6028219
Conc: 43.25 ug/ml

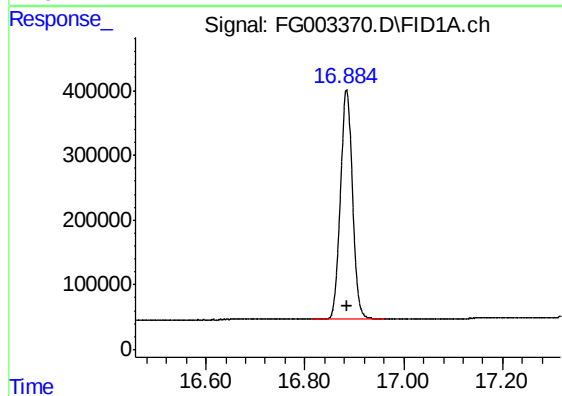

#12 N-OCTACOSANE

R.T.: 16.884 min
Delta R.T.: -0.002 min
Response: 5968566
Conc: 42.71 ug/ml