

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010623\
Data File : FG011251.D
Signal(s) : FID1A.ch
Acq On : 06 Jan 2023 13:34
Operator : YP\AJ
Sample : PB150079BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB150079BL

Integration File: autoint1.e
Quant Time: Jan 06 17:36:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
Quant Title :
QLast Update : Mon Jan 02 04:44:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.066	2381415	15.540 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010623\
Data File : FG011251.D
Signal(s) : FID1A.ch
Acq On : 06 Jan 2023 13:34
Operator : YP\AJ
Sample : PB150079BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB150079BL

Integration File: autoint1.e
Quant Time: Jan 06 17:36:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
Quant Title :
QLast Update : Mon Jan 02 04:44:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

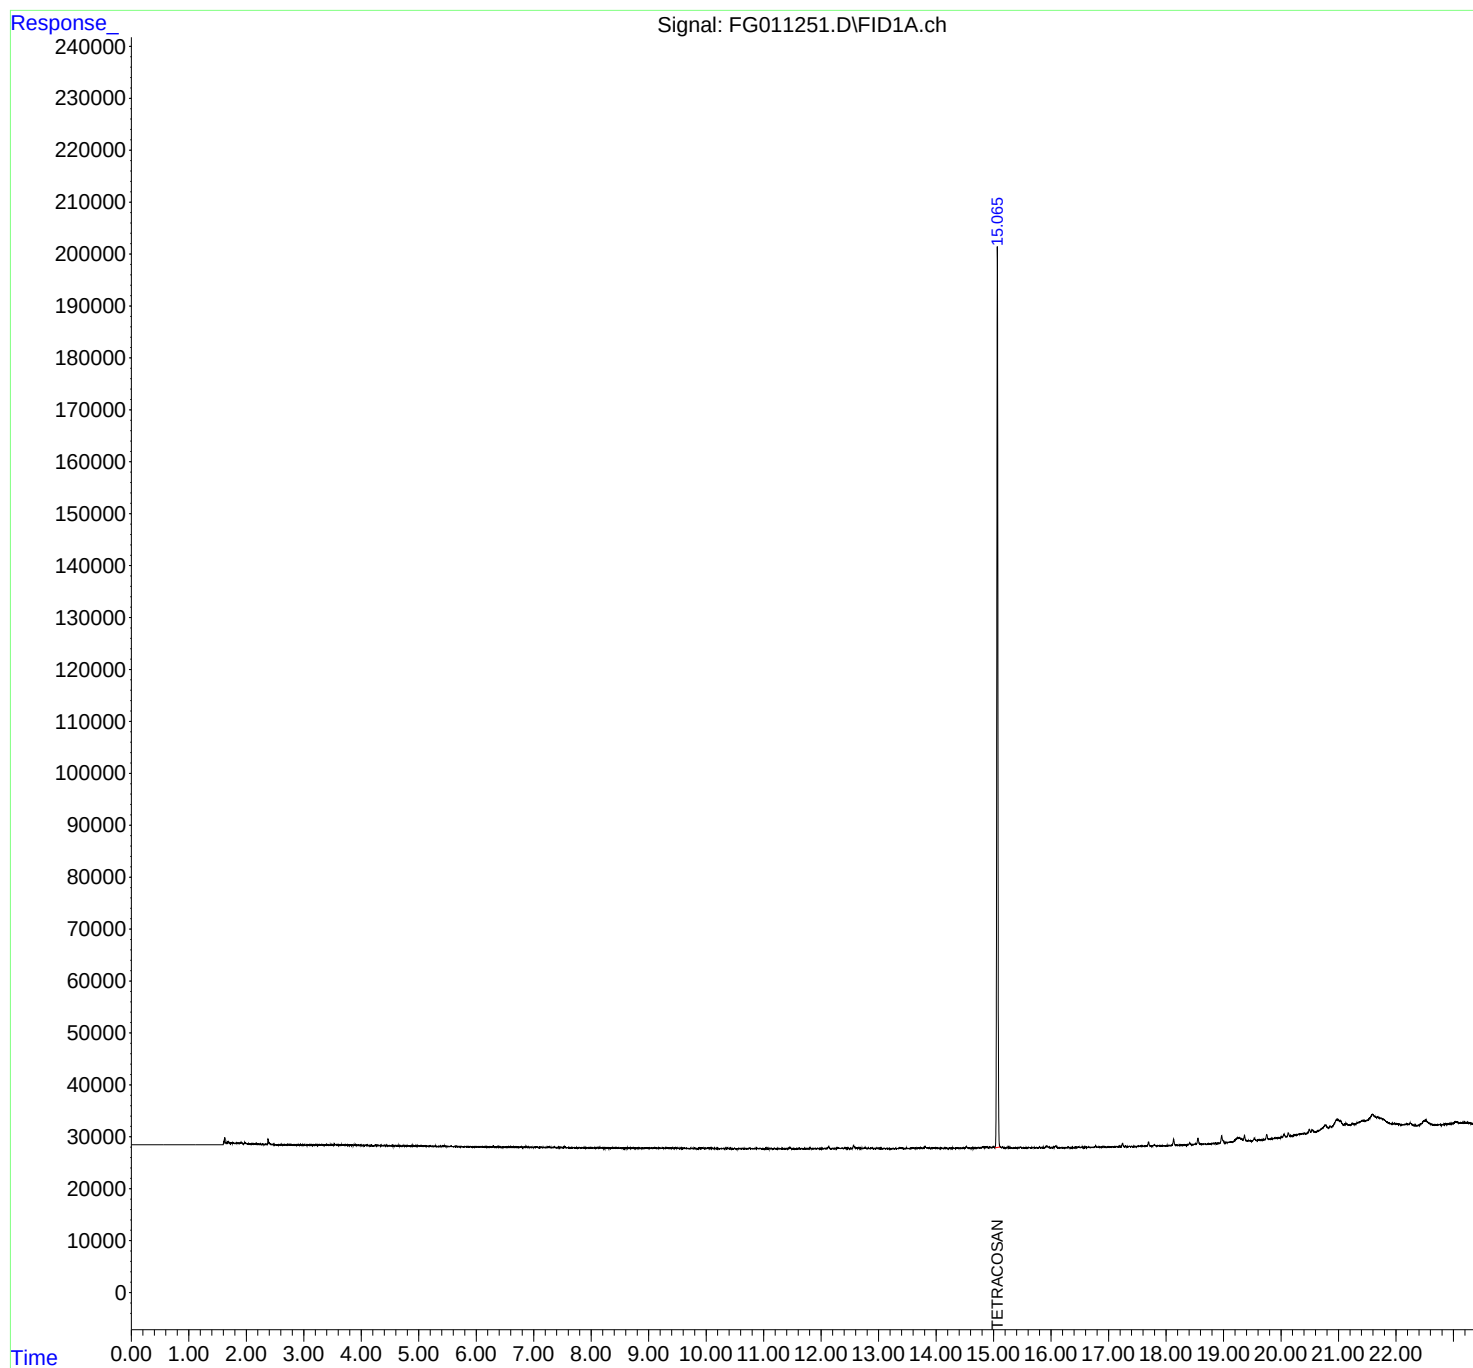

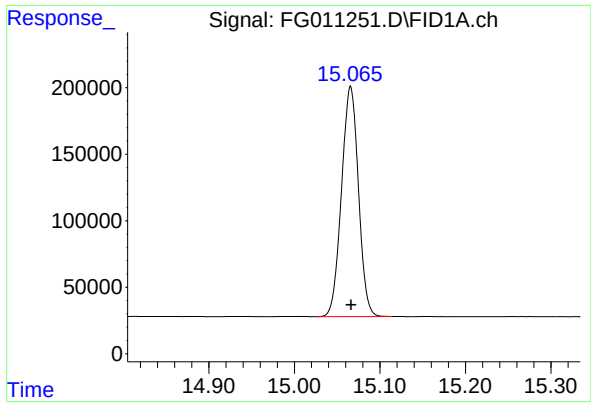

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.066 min
Delta R.T.: 0.000 min
Response: 2381415
Conc: 15.54 ug/ml

Instrument :
FID_G
ClientSampleId :
PB150079BL