

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010719\
 Data File : FG003395.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jan 2019 10:47
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 08 00:24:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
 Quant Title :
 QLast Update : Thu Dec 13 00:59:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.703	6340518	51.121 ug/ml
Target Compounds			
2) N-DECANE	4.406	7990414	59.555 ug/ml
3) N-DODECANE	6.433	8014237	58.907 ug/ml
4) N-TETRADECANE	8.233	8002426	57.986 ug/ml
5) N-HEXADECANE	9.837	7935957	56.644 ug/ml
6) N-OCTADECANE	11.283	7787819	54.968 ug/ml
7) N-EICOSANE	12.597	7523666	53.256 ug/ml
8) N-DOCOSANE	13.800	7240607	51.480 ug/ml
10) N-TETRACOSANE	14.907	6994814	49.973 ug/ml
11) N-HEXACOSANE	15.933	6819422	48.927 ug/ml
12) N-OCTACOSANE	16.887	6745561	48.273 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010719\
Data File : FG003395.D
Signal(s) : FID1A.ch
Acq On : 07 Jan 2019 10:47
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 08 00:24:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
Quant Title :
QLast Update : Thu Dec 13 00:59:54 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

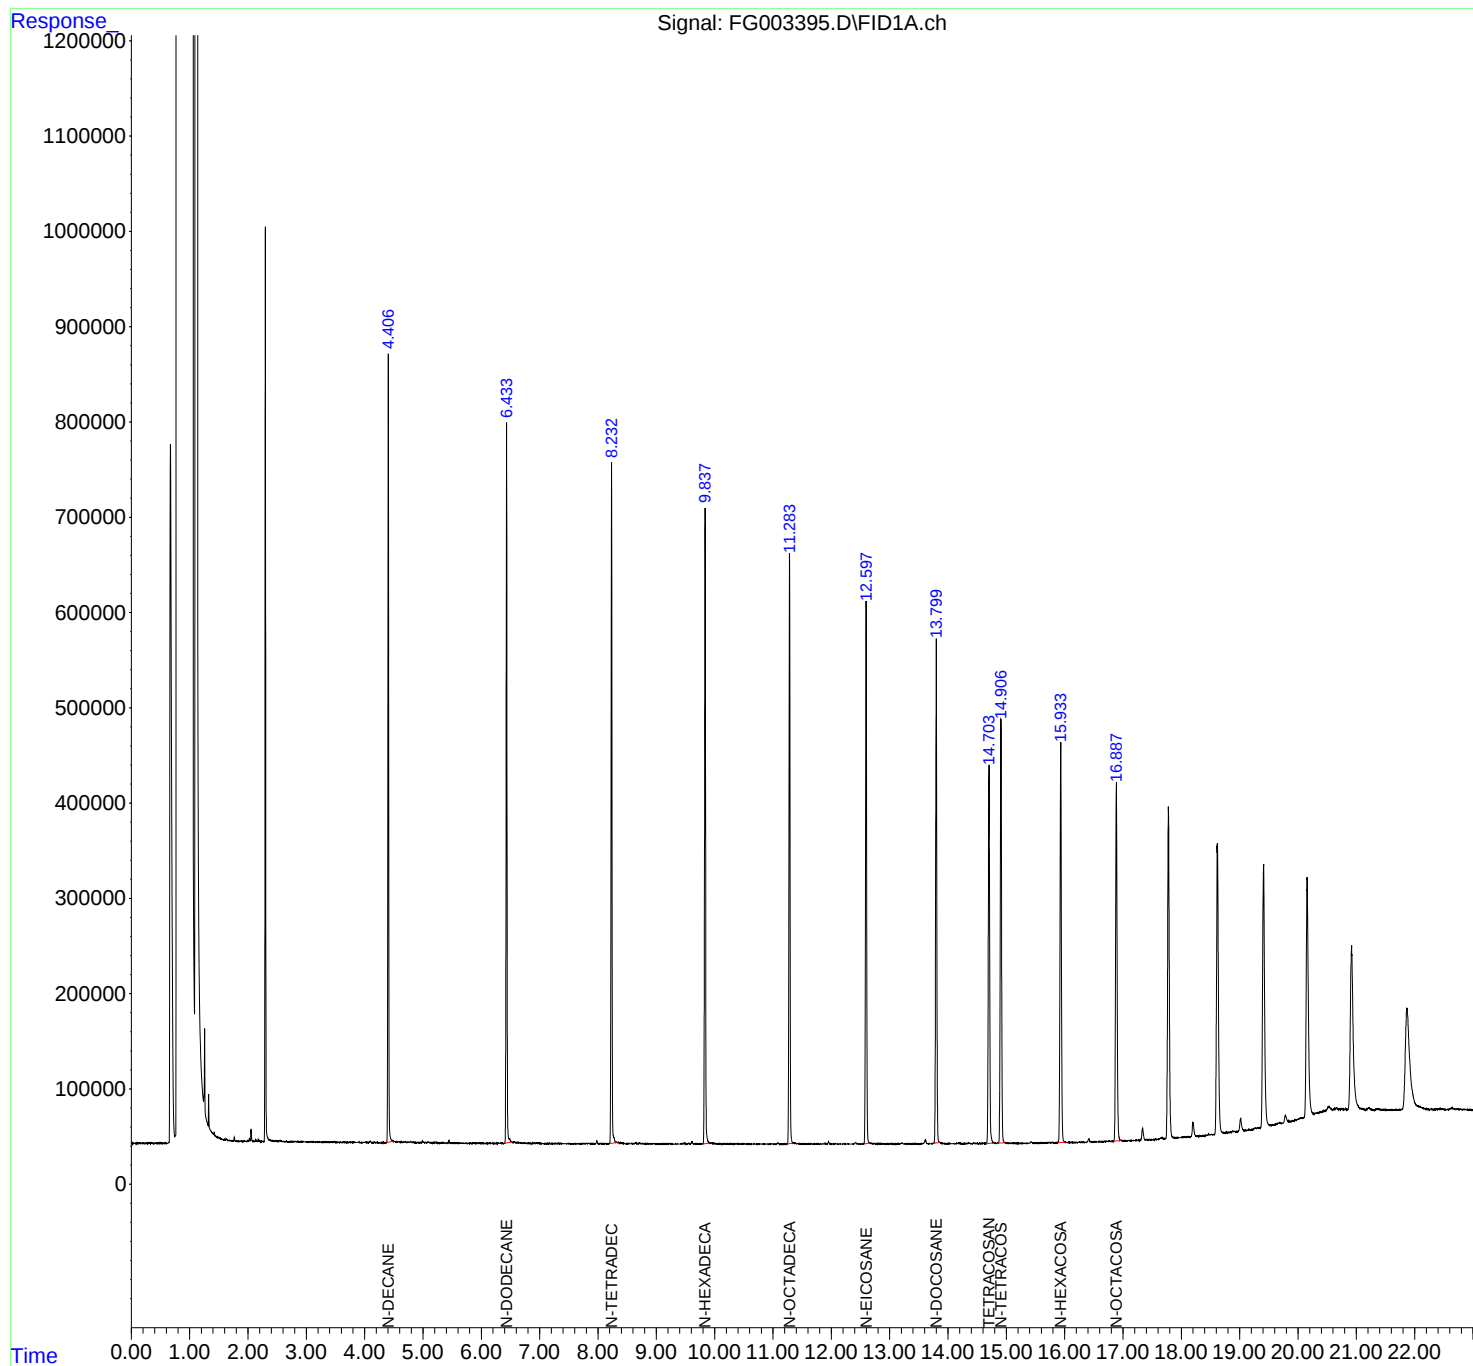

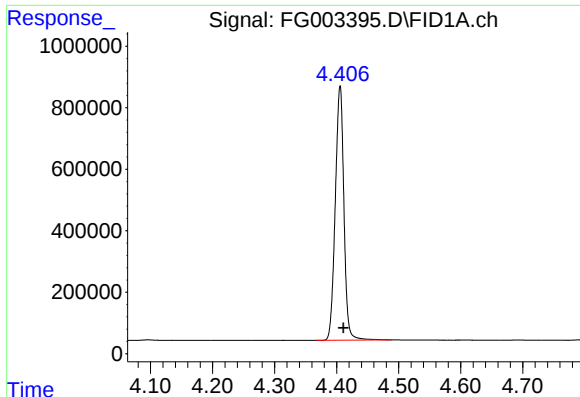


#2 N-DECANE

R.T.: 4.406 min
Delta R.T.: -0.005 min
Response: 7990414
Conc: 59.55 ug/ml

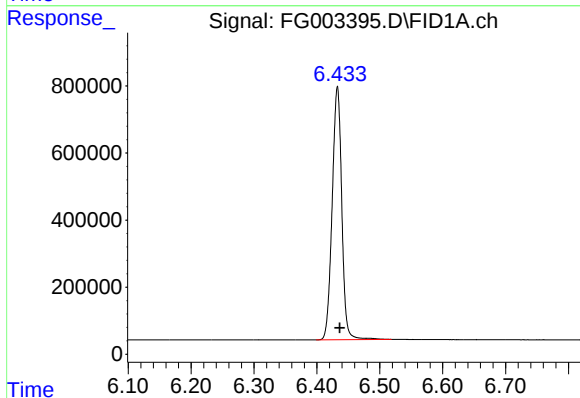


#3 N-DODECANE

R.T.: 6.433 min
Delta R.T.: -0.004 min
Response: 8014237
Conc: 58.91 ug/ml

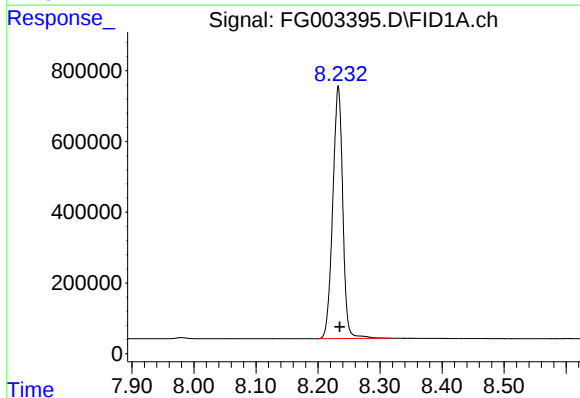


#4 N-TETRADECANE

R.T.: 8.233 min
Delta R.T.: -0.002 min
Response: 8002426
Conc: 57.99 ug/ml

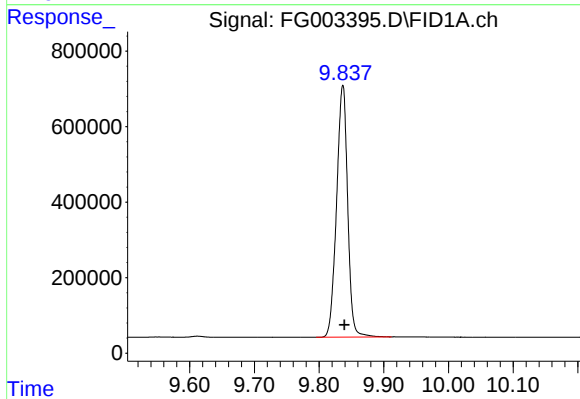


#5 N-HEXADECANE

R.T.: 9.837 min
Delta R.T.: -0.003 min
Response: 7935957
Conc: 56.64 ug/ml

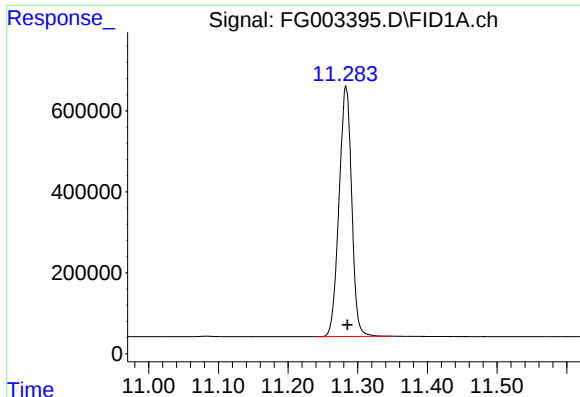


#6 N-OCTADECANE

R.T.: 11.283 min
Delta R.T.: -0.002 min
Response: 7787819
Conc: 54.97 ug/ml

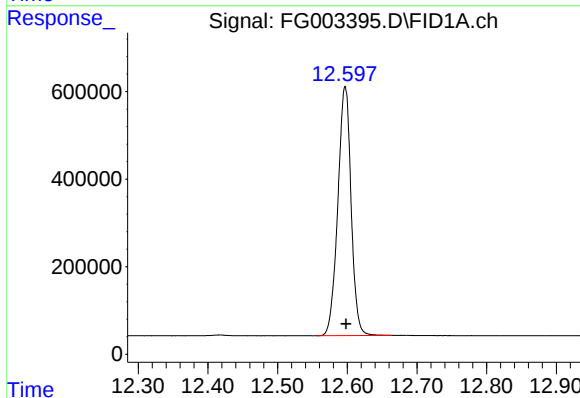


#7 N-EICOSANE

R.T.: 12.597 min
Delta R.T.: -0.001 min
Response: 7523666
Conc: 53.26 ug/ml

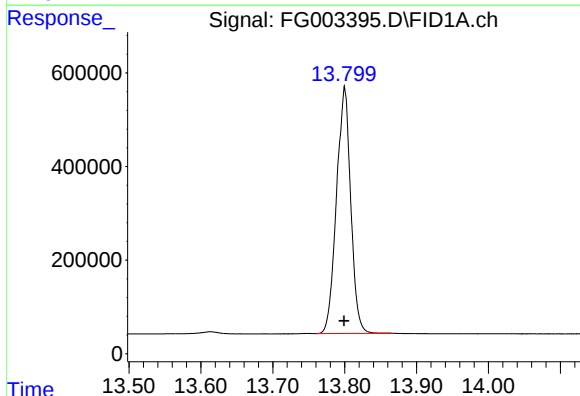


#8 N-DOCOSANE

R.T.: 13.800 min
Delta R.T.: 0.000 min
Response: 7240607
Conc: 51.48 ug/ml

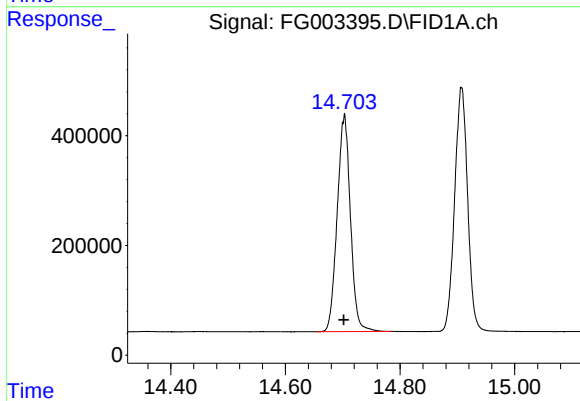


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.703 min
Delta R.T.: 0.001 min
Response: 6340518
Conc: 51.12 ug/ml

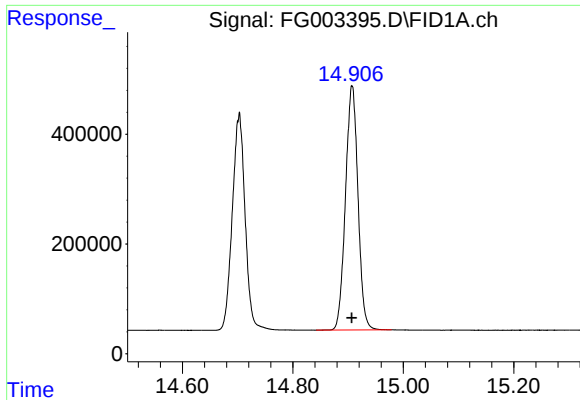


#10 N-TETRACOSANE

R.T.: 14.907 min
Delta R.T.: 0.000 min
Response: 6994814
Conc: 49.97 ug/ml

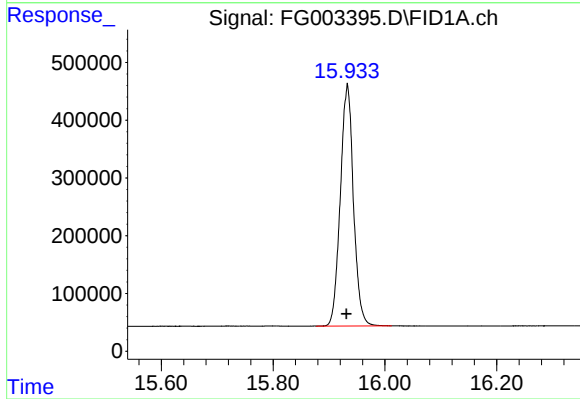

#11 N-HEXACOSANE

R.T.: 15.933 min
Delta R.T.: 0.002 min
Response: 6819422
Conc: 48.93 ug/ml

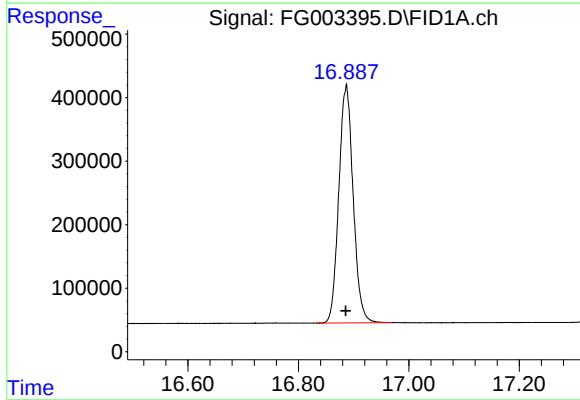

#12 N-OCTACOSANE

R.T.: 16.887 min
Delta R.T.: 0.001 min
Response: 6745561
Conc: 48.27 ug/ml