

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010721\
Data File : FG007523.D
Signal(s) : FID1A.ch
Acq On : 07 Jan 2021 09:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 08 00:13:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.635	2422330	20.213 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.544	109523	0.967 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010721\
Data File : FG007523.D
Signal(s) : FID1A.ch
Acq On : 07 Jan 2021 09:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 08 00:13:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

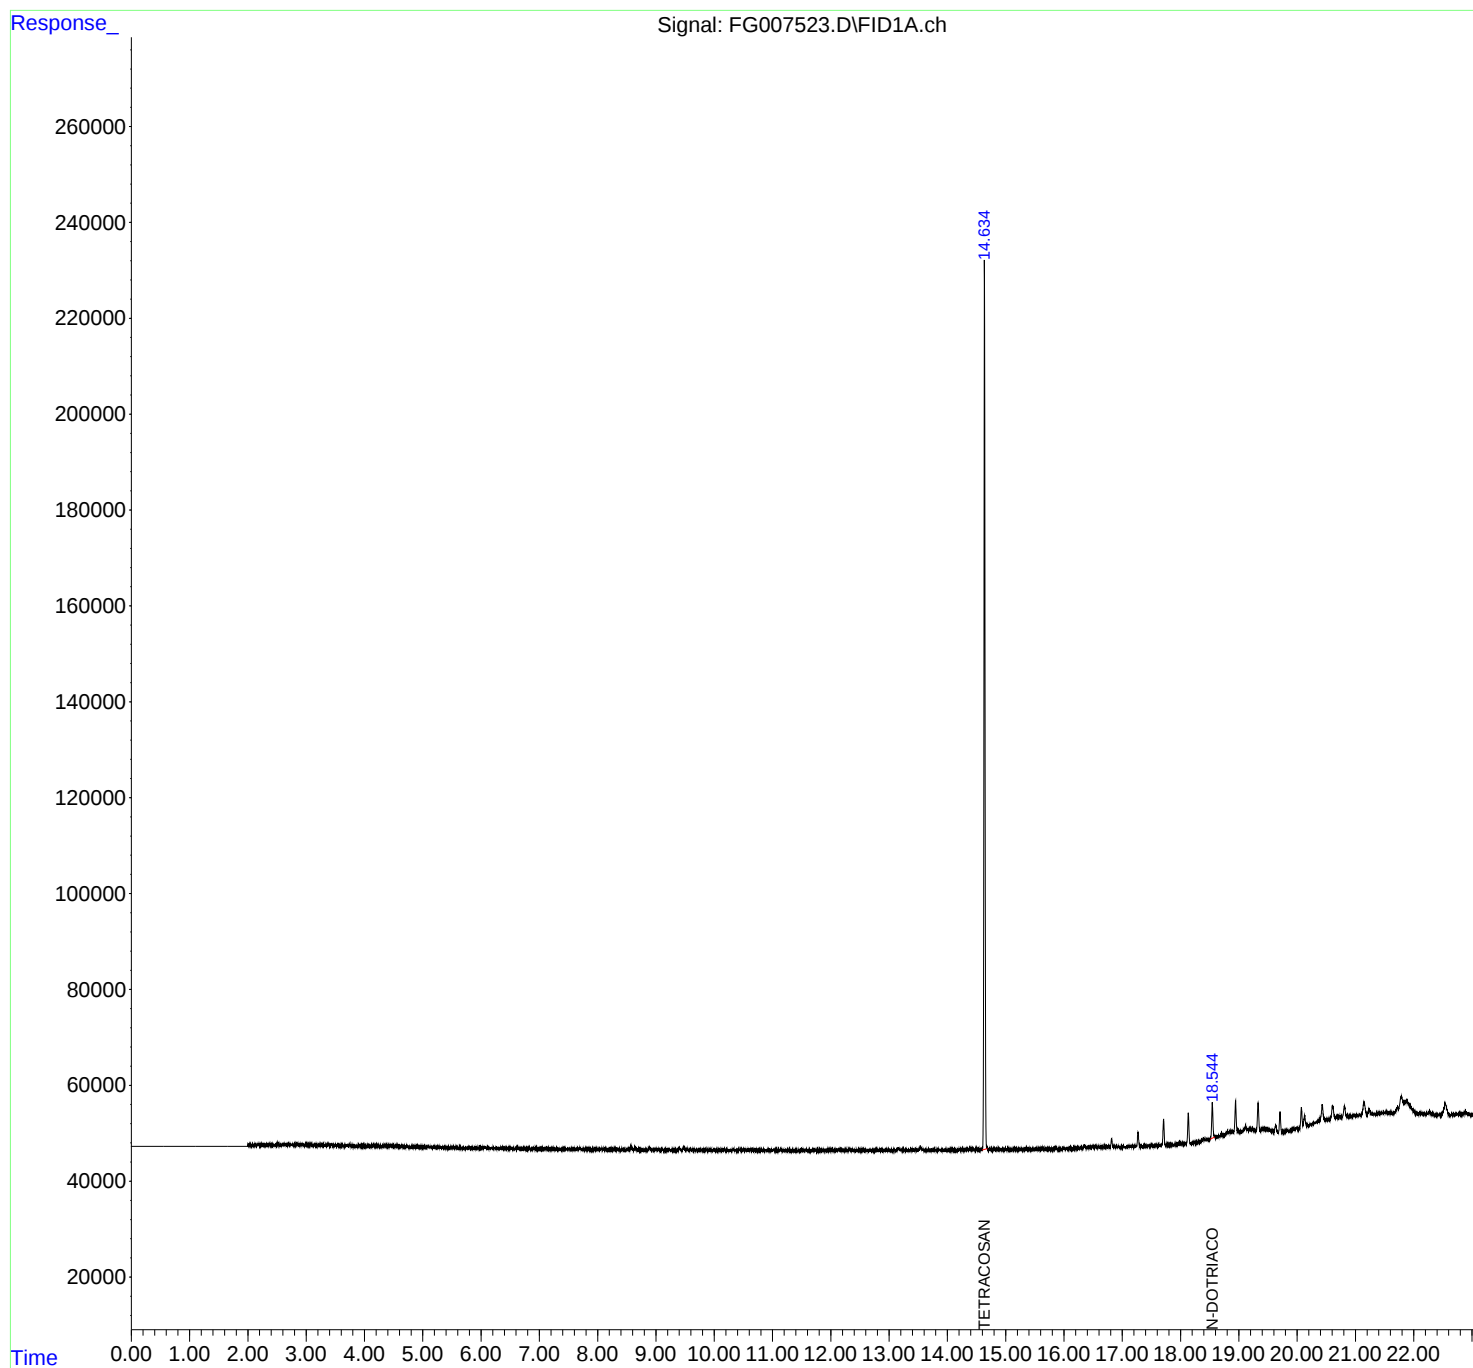


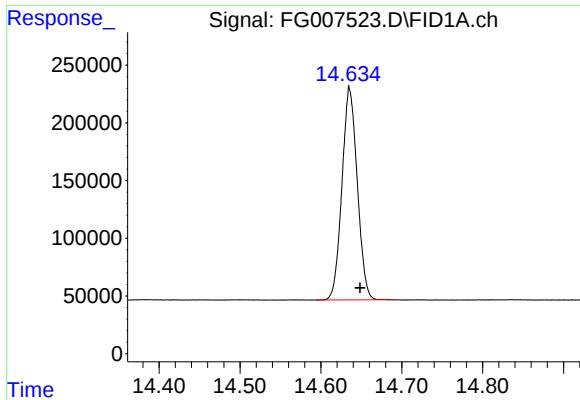

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.635 min
Delta R.T.: -0.013 min
Response: 2422330
Conc: 20.21 ug/ml

Instrument :
FID_G
ClientSampleId :

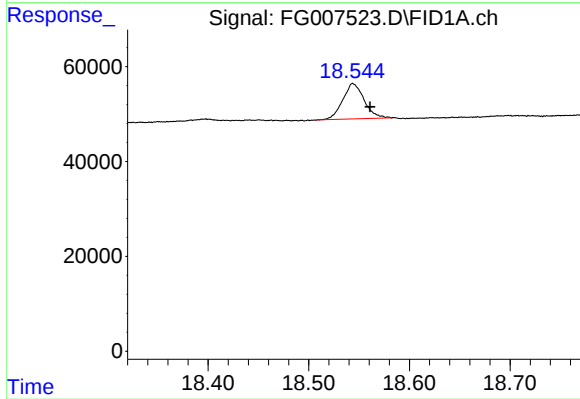

#14 N-DOTRIACONTANE

R.T.: 18.544 min
Delta R.T.: -0.017 min
Response: 109523
Conc: 0.97 ug/ml