

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010820\
 Data File : FG006468.D
 Signal(s) : FID1A.ch
 Acq On : 08 Jan 2020 15:50
 Operator : DD\AJ
 Sample : L1017-01MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Jan 09 00:22:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG122619.M
 Quant Title :
 QLast Update : Fri Dec 27 04:12:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.534	2029454	19.225 ug/ml
Target Compounds			
2) N-DECANE	4.486	2328609	23.960 ug/ml
3) N-DODECANE	6.460	2443681	23.940 ug/ml
4) N-TETRADECANE	8.213	2564713	23.519 ug/ml
5) N-HEXADECANE	9.777	2426809	20.698 ug/ml
6) N-OCTADECANE	11.189	2432113	20.117 ug/ml
7) N-EICOSANE	12.473	2798975	22.593 ug/ml
8) N-DOCOSANE	13.650	2358644	19.221 ug/ml
10) N-TETRACOSANE	14.733	2925004	24.116 ug/mlm
11) N-HEXACOSANE	15.736	2422371	20.298 ug/ml
12) N-OCTACOSANE	16.668	3128298	26.443 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010820\
Data File : FG006468.D
Signal(s) : FID1A.ch
Acq On : 08 Jan 2020 15:50
Operator : DD\AJ
Sample : L1017-01MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Jan 09 00:22:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG122619.M
Quant Title :
QLast Update : Fri Dec 27 04:12:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

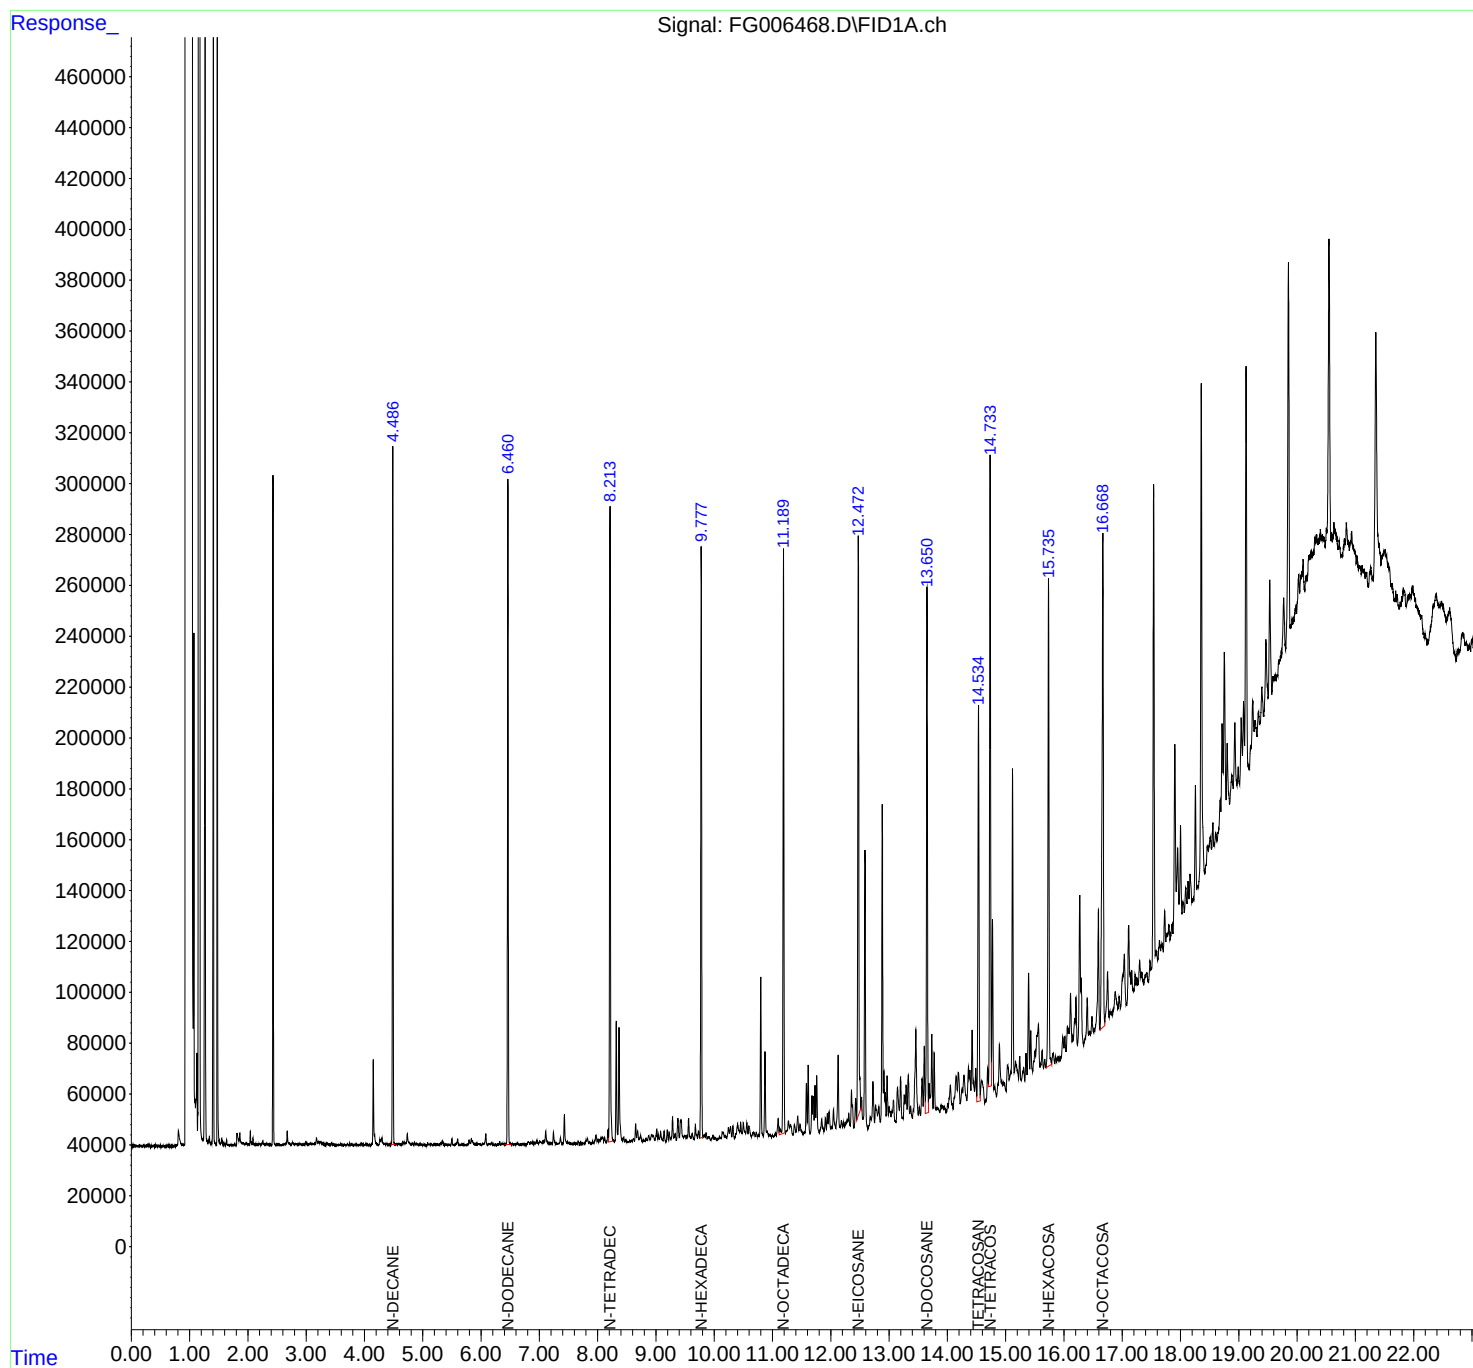

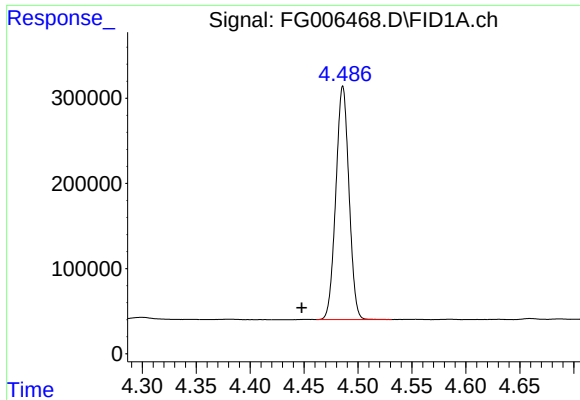


#2 N-DECANE

R.T.: 4.486 min
Delta R.T.: 0.038 min
Response: 2328609
Conc: 23.96 ug/ml

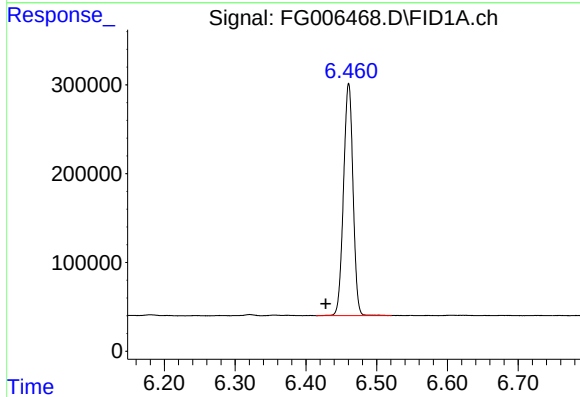


#3 N-DODECANE

R.T.: 6.460 min
Delta R.T.: 0.032 min
Response: 2443681
Conc: 23.94 ug/ml

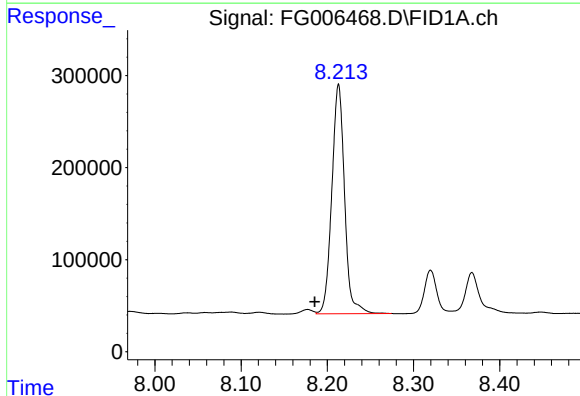


#4 N-TETRADECANE

R.T.: 8.213 min
Delta R.T.: 0.028 min
Response: 2564713
Conc: 23.52 ug/ml

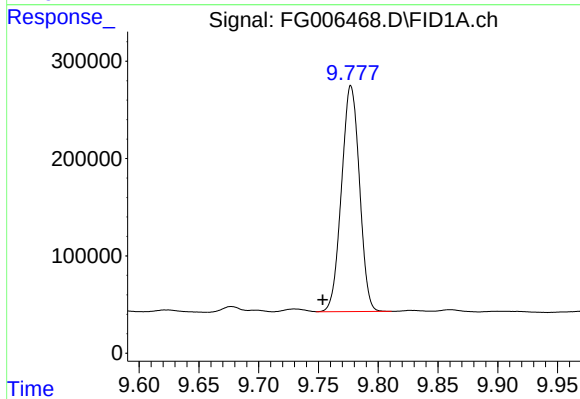


#5 N-HEXADECANE

R.T.: 9.777 min
Delta R.T.: 0.024 min
Response: 2426809
Conc: 20.70 ug/ml

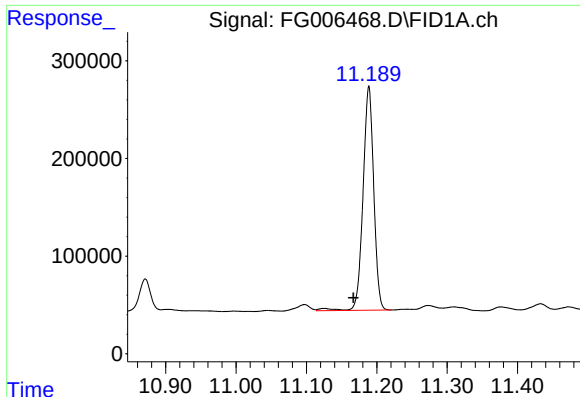


#6 N-OCTADECANE

R.T.: 11.189 min
Delta R.T.: 0.022 min
Response: 2432113
Conc: 20.12 ug/ml

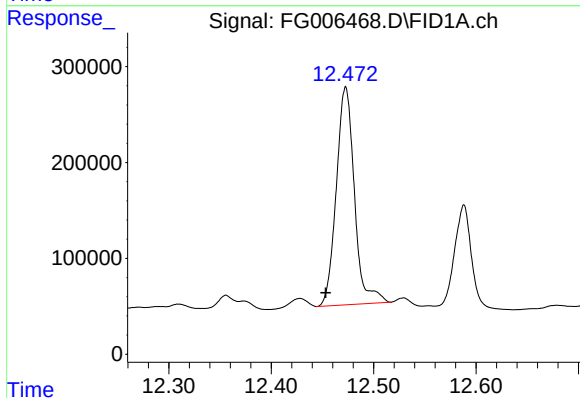


#7 N-EICOSANE

R.T.: 12.473 min
Delta R.T.: 0.019 min
Response: 2798975
Conc: 22.59 ug/ml

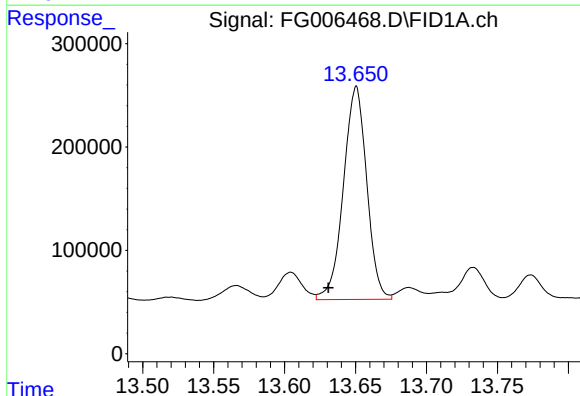


#8 N-DOCOSANE

R.T.: 13.650 min
Delta R.T.: 0.019 min
Response: 2358644
Conc: 19.22 ug/ml

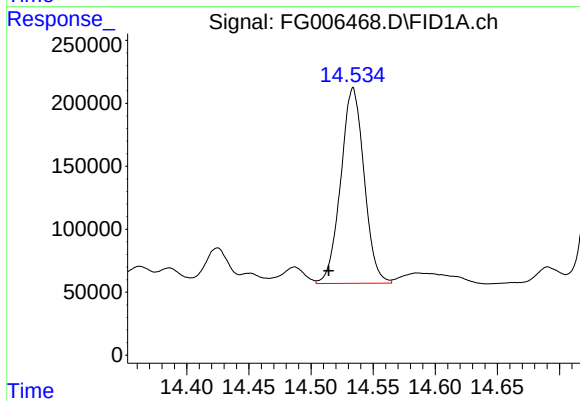


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.534 min
Delta R.T.: 0.020 min
Response: 2029454
Conc: 19.23 ug/ml

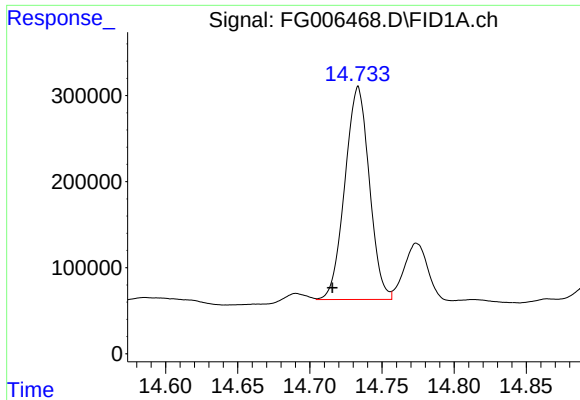


#10 N-TETRACOSANE

R.T.: 14.733 min
Delta R.T.: 0.018 min
Response: 2925004
Conc: 24.12 ug/ml m

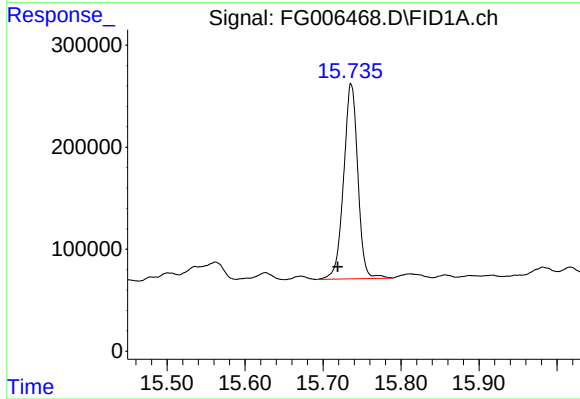

#11 N-HEXACOSANE

R.T.: 15.736 min
Delta R.T.: 0.017 min
Response: 2422371
Conc: 20.30 ug/ml

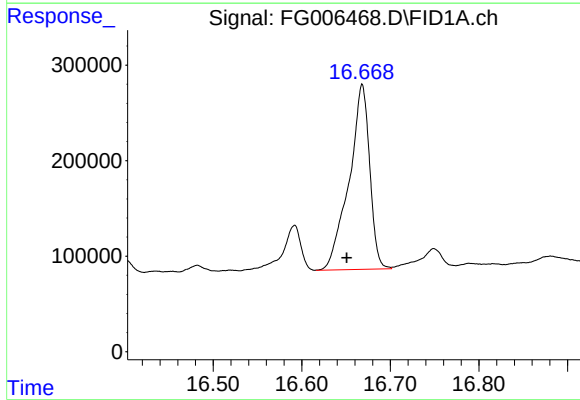

#12 N-OCTACOSANE

R.T.: 16.668 min
Delta R.T.: 0.017 min
Response: 3128298
Conc: 26.44 ug/ml