

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010821\
 Data File : FG007532.D
 Signal(s) : FID1A.ch
 Acq On : 08 Jan 2021 09:39
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 08 21:55:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
 Quant Title :
 QLast Update : Tue Jan 05 02:18:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	2432146	20.295 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.542	106671	0.942 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG010821\
Data File : FG007532.D
Signal(s) : FID1A.ch
Acq On : 08 Jan 2021 09:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 08 21:55:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

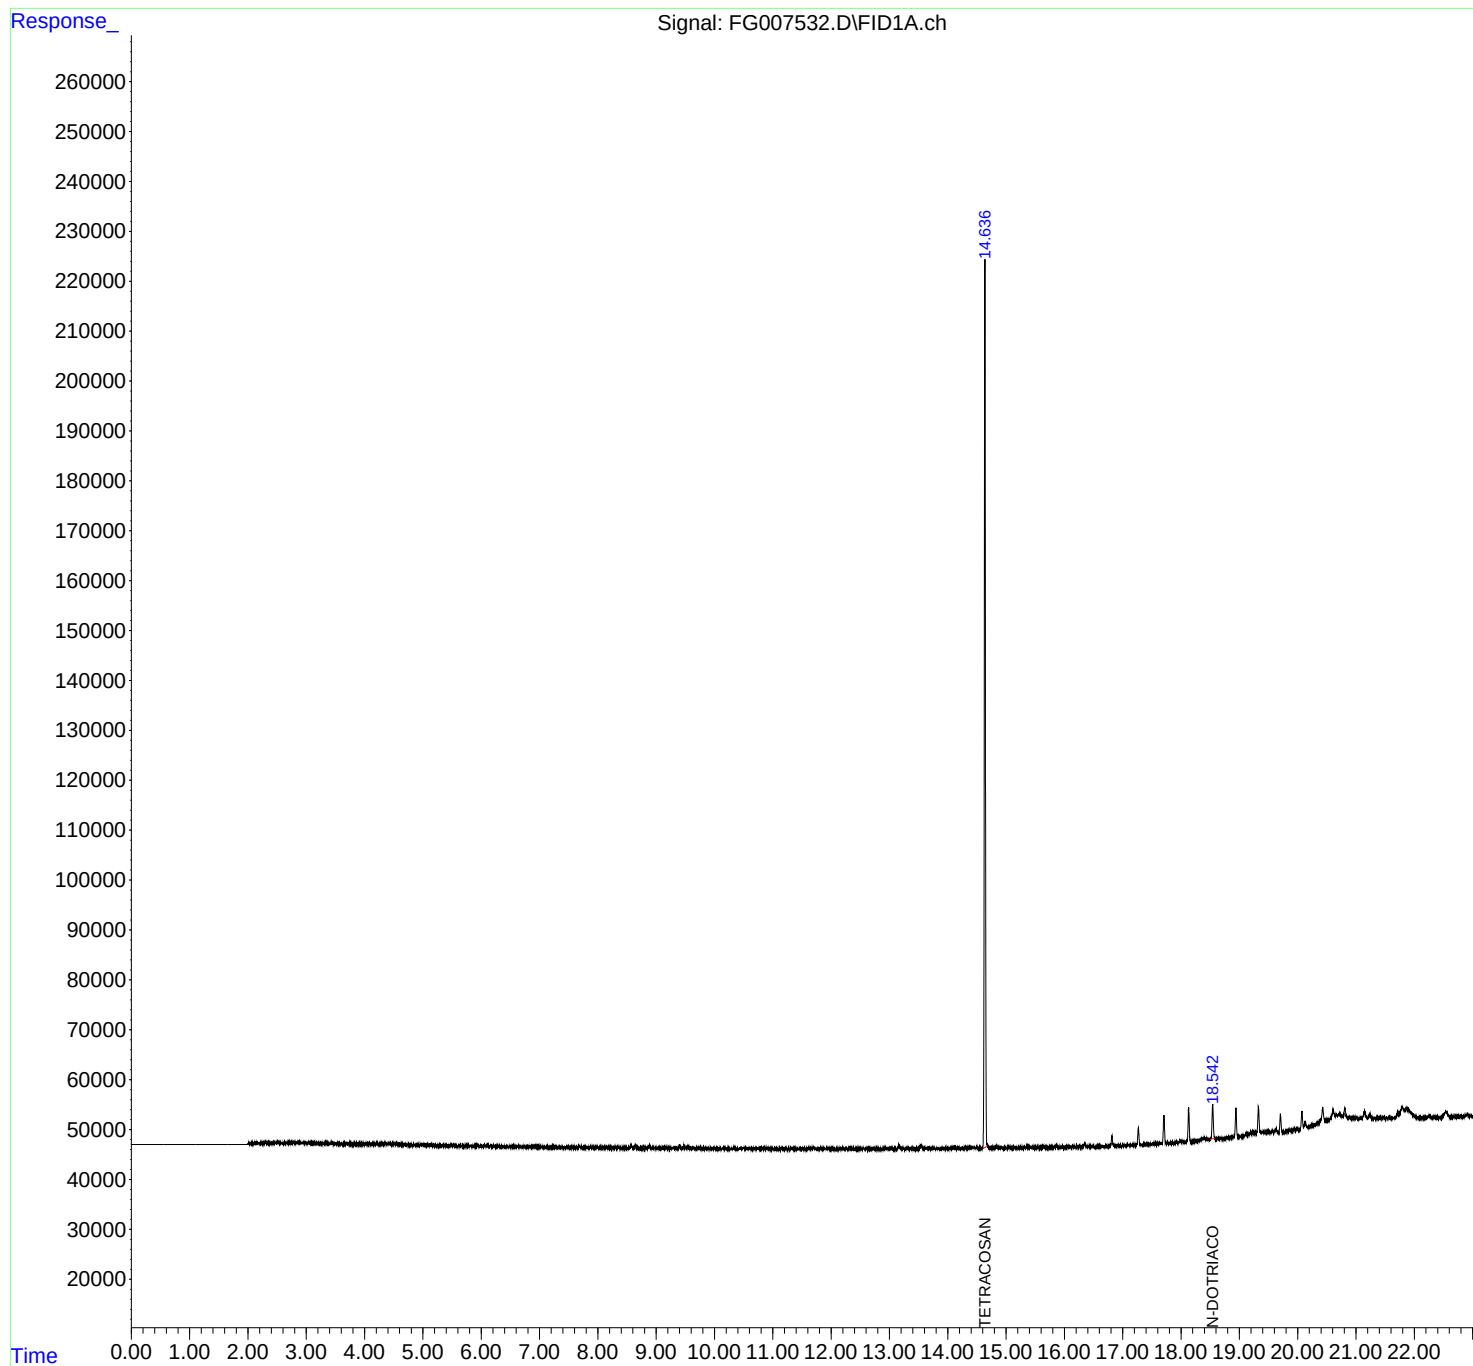


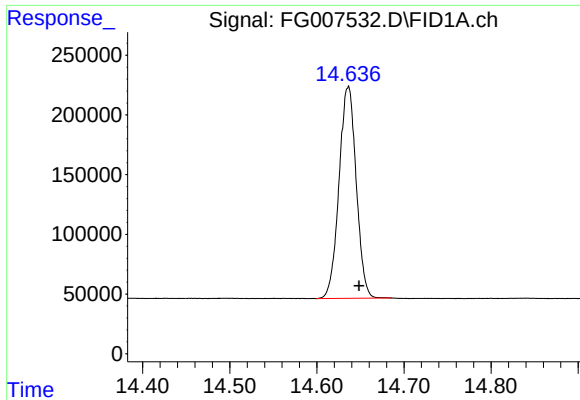

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.013 min
Response: 2432146
Conc: 20.29 ug/ml

Instrument :
FID_G
ClientSampleId :

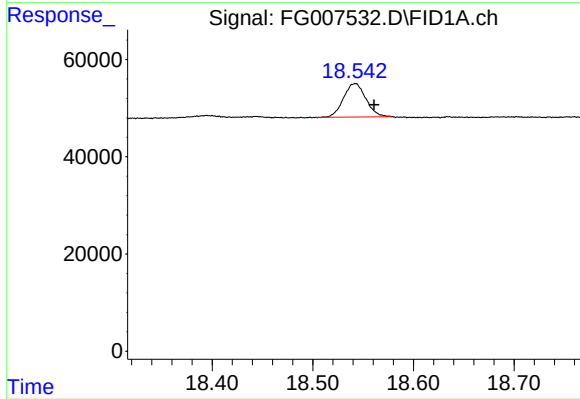

#14 N-DOTRIACONTANE

R.T.: 18.542 min
Delta R.T.: -0.019 min
Response: 106671
Conc: 0.94 ug/ml