

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011421\
 Data File : FG007553.D
 Signal(s) : FID1A.ch
 Acq On : 14 Jan 2021 15:02
 Operator : DD\AJ
 Sample : M1119-01MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 IDW-BRI-SO-011221MS

Integration File: autoint1.e
 Quant Time: Jan 14 20:56:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
 Quant Title :
 QLast Update : Tue Jan 05 02:18:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.639	1624865	13.559 ug/ml
Target Compounds			
2) N-DECANE	4.341	2620082	17.415 ug/ml
3) N-DODECANE	6.366	2681437	17.679 ug/ml
4) N-TETRADECANE	8.166	2759062	18.190 ug/ml
5) N-HEXADECANE	9.772	2682113	17.950 ug/ml
6) N-OCTADECANE	11.218	2659627	17.831 ug/ml
7) N-EICOSANE	12.534	2639734	18.112 ug/ml
8) N-DOCOSANE	13.734	2549271	18.207 ug/ml
10) N-TETRACOSANE	14.844	2427296	17.747 ug/ml
11) N-HEXACOSANE	15.869	2330790	17.747 ug/ml
12) N-OCTACOSANE	16.822	2262320	17.813 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011421\
Data File : FG007553.D
Signal(s) : FID1A.ch
Acq On : 14 Jan 2021 15:02
Operator : DD\AJ
Sample : M1119-01MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
IDW-BRI-SO-011221MS

Integration File: autoint1.e
Quant Time: Jan 14 20:56:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

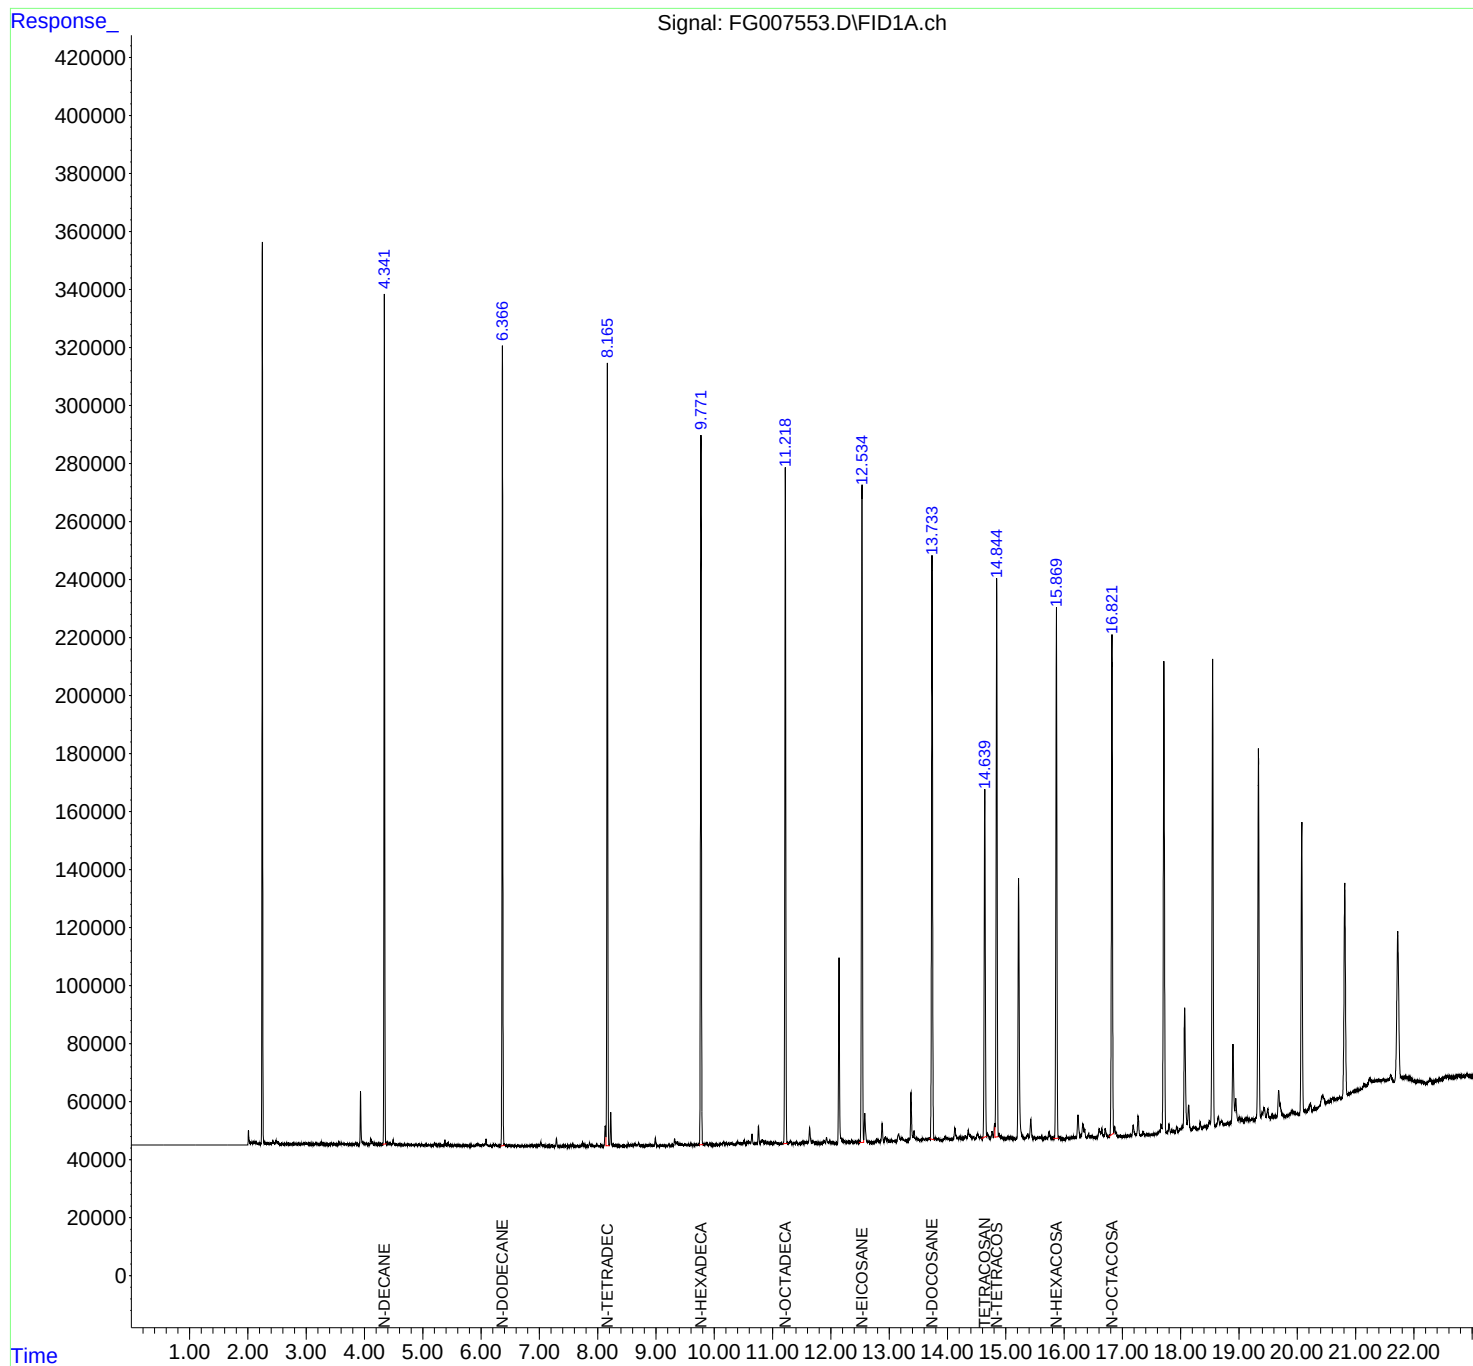


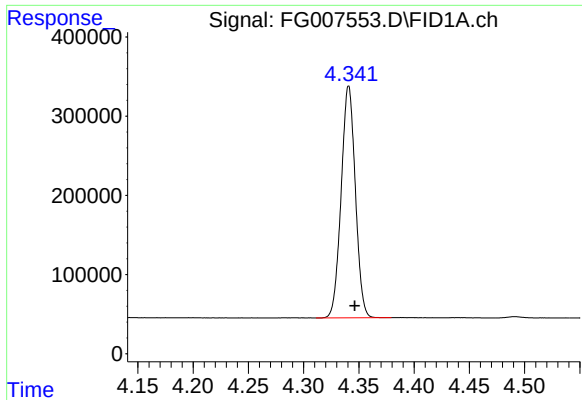

#2 N-DECANE


R.T.: 4.341 min
Delta R.T.: -0.005 min
Response: 2620082
Conc: 17.41 ug/ml

Instrument :
FID_G
ClientSampleId :
IDW-BRI-SO-011221MS

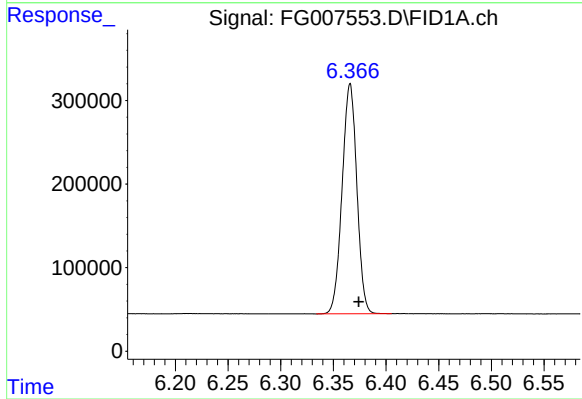


#3 N-DODECANE

R.T.: 6.366 min
Delta R.T.: -0.008 min
Response: 2681437
Conc: 17.68 ug/ml

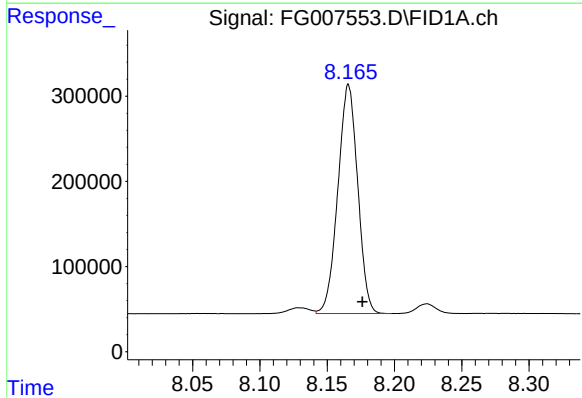


#4 N-TETRADECANE

R.T.: 8.166 min
Delta R.T.: -0.010 min
Response: 2759062
Conc: 18.19 ug/ml

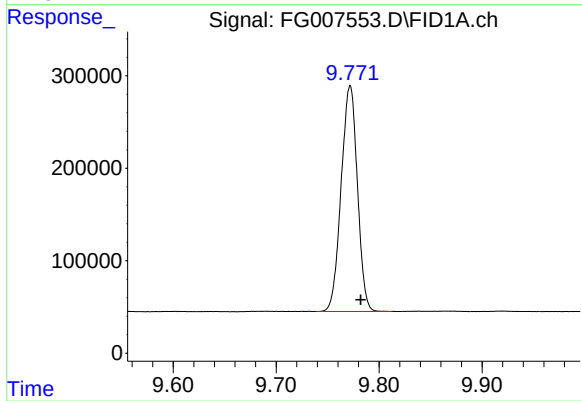

#5 N-HEXADECANE


R.T.: 9.772 min
Delta R.T.: -0.010 min
Response: 2682113
Conc: 17.95 ug/ml

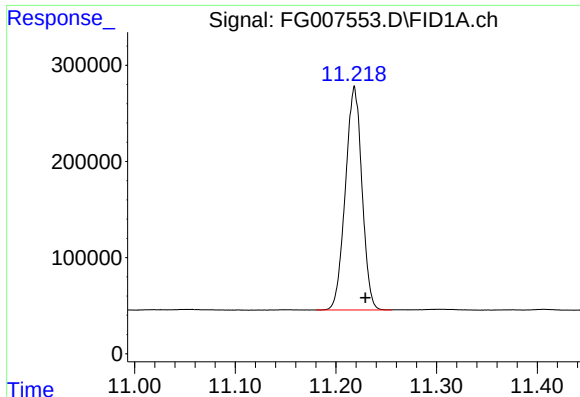

#6 N-OCTADECANE


R.T.: 11.218 min
Delta R.T.: -0.011 min
Response: 2659627
Conc: 17.83 ug/ml

Instrument :
FID_G
ClientSampleId :
IDW-BRI-SO-011221MS

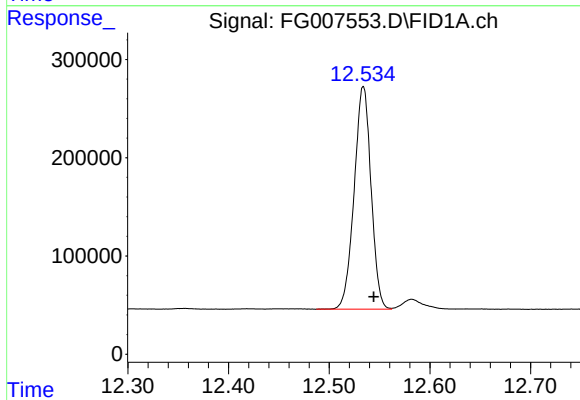


#7 N-EICOSANE

R.T.: 12.534 min
Delta R.T.: -0.010 min
Response: 2639734
Conc: 18.11 ug/ml

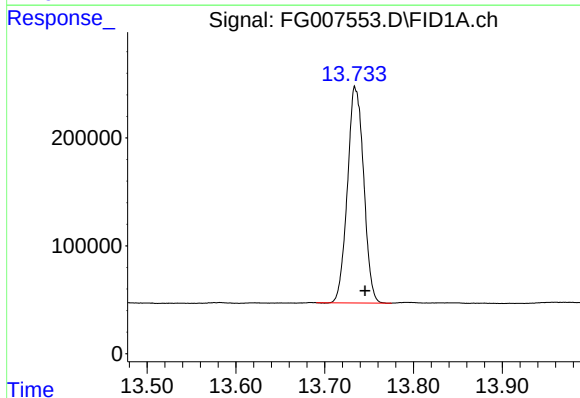


#8 N-DOCOSANE

R.T.: 13.734 min
Delta R.T.: -0.011 min
Response: 2549271
Conc: 18.21 ug/ml

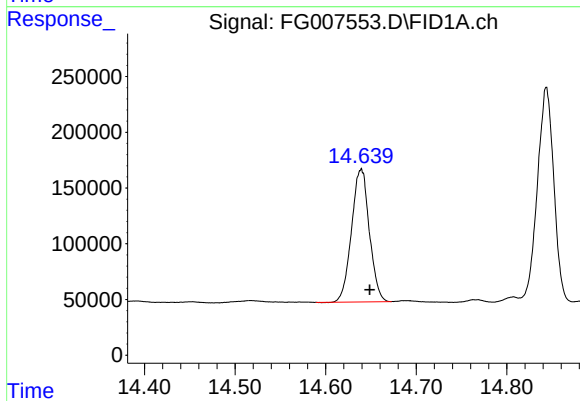

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.639 min
Delta R.T.: -0.009 min
Response: 1624865
Conc: 13.56 ug/ml

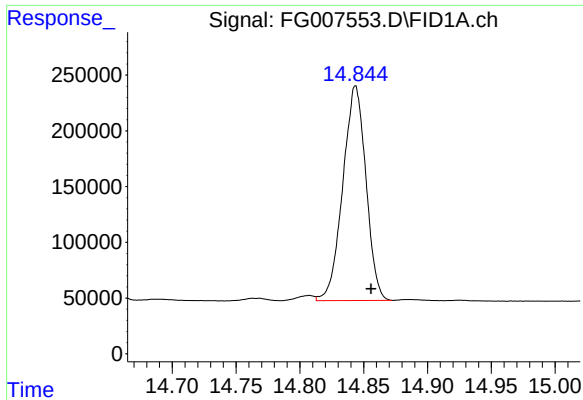

#10 N-TETRACOSANE


R.T.: 14.844 min
Delta R.T.: -0.012 min
Response: 2427296
Conc: 17.75 ug/ml

Instrument :
FID_G
ClientSampleId :
IDW-BRI-SO-011221MS

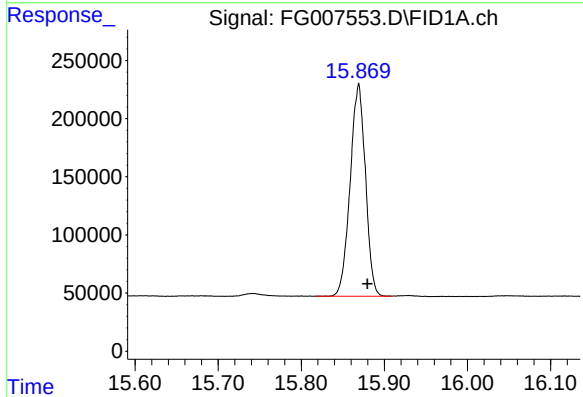

#11 N-HEXACOSANE

R.T.: 15.869 min
Delta R.T.: -0.010 min
Response: 2330790
Conc: 17.75 ug/ml

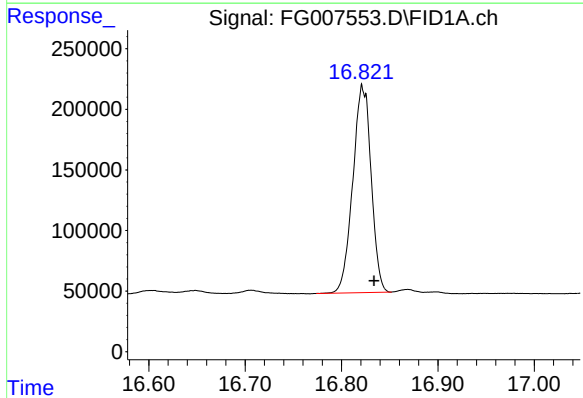

#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.012 min
Response: 2262320
Conc: 17.81 ug/ml