

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003528.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 09:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jan 19 02:53:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.225	3553057	27.280 ug/ml
12)	N-OCTACOSANE	16.656	3237946	22.813 ug/ml
13)	N-TRIACONTANE	17.542	280146	1.988 ug/ml
14)	N-DOTRIACONTANE	18.376	297802	2.202 ug/ml
15)	N-TETRATRIACONTANE	19.163	207768	1.614 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003528.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 09:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jan 19 02:53:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

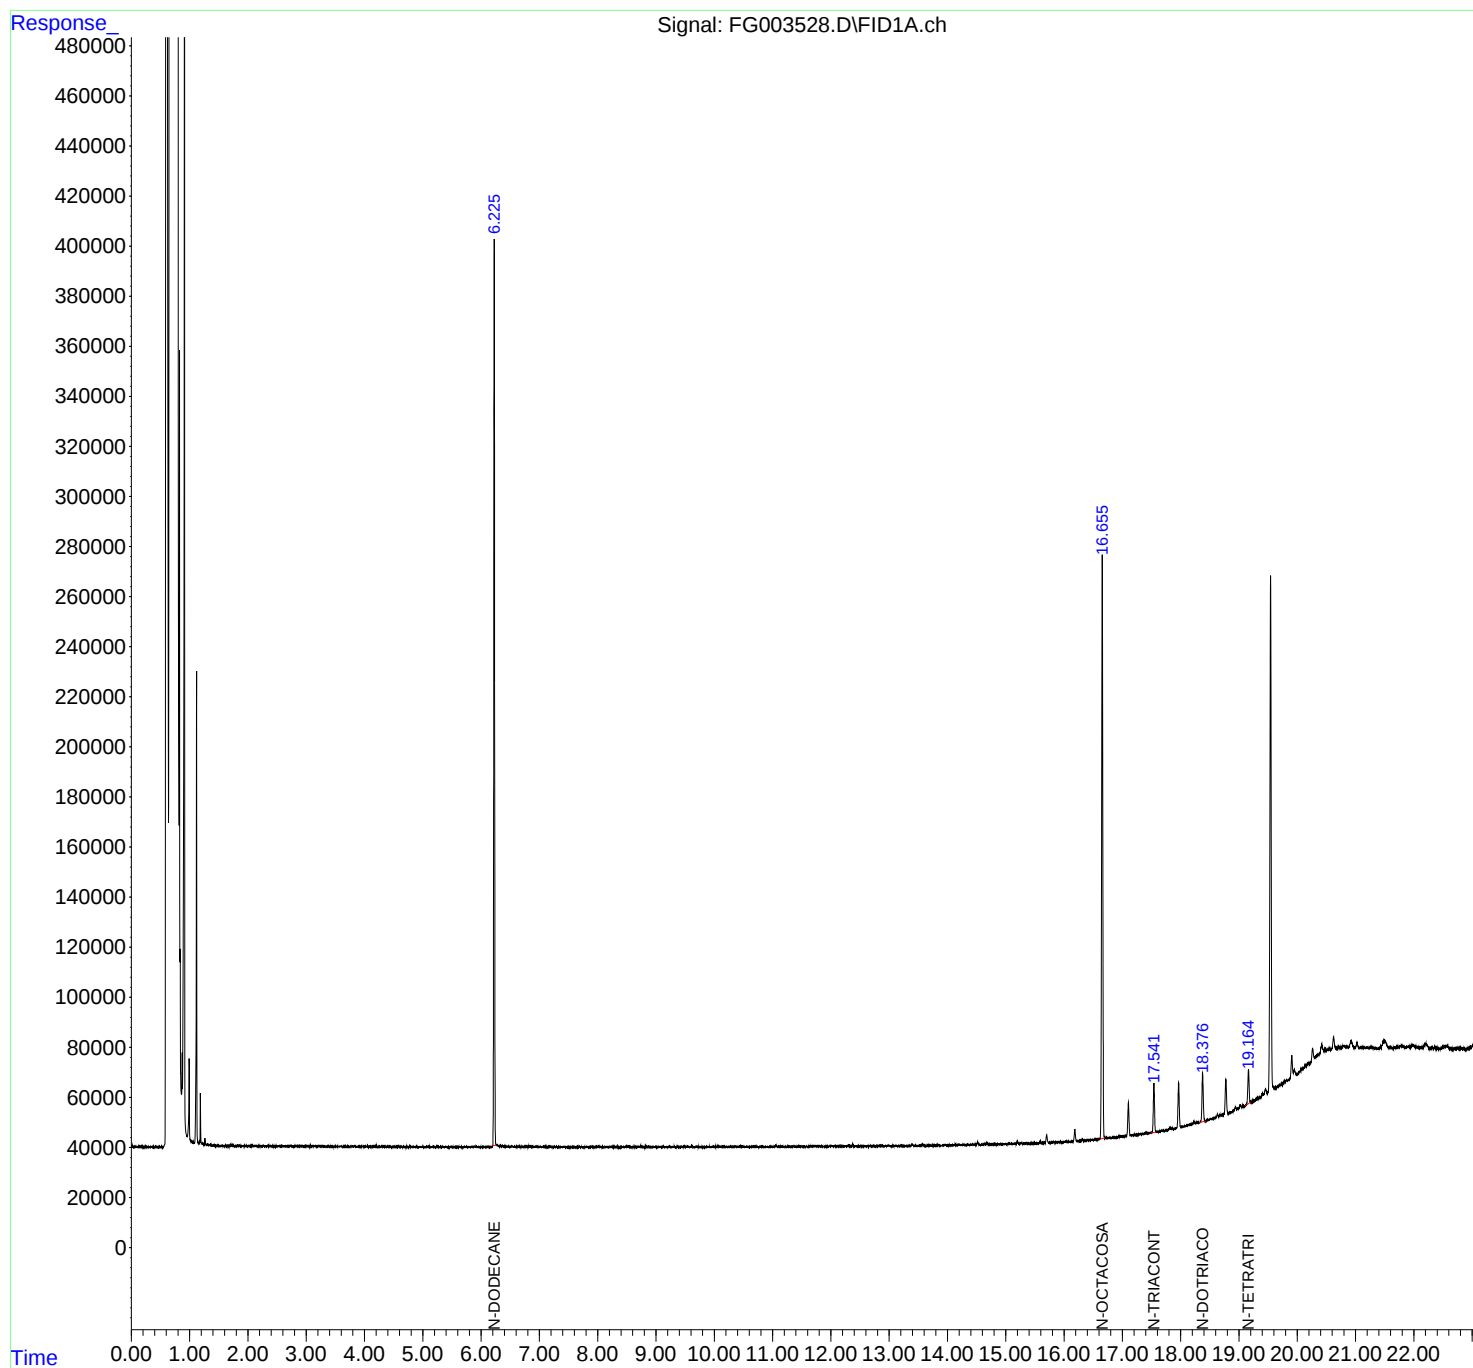


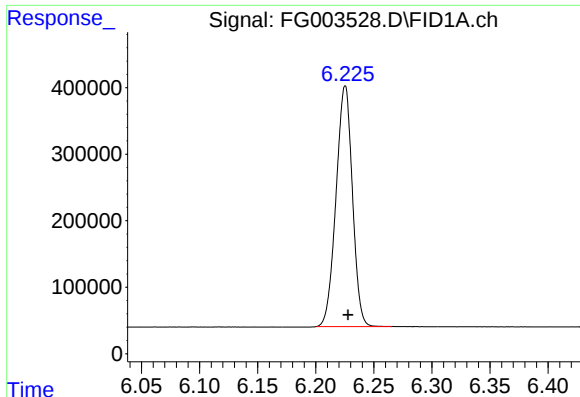

#3 N-DODECANE


R.T.: 6.225 min
Delta R.T.: -0.002 min
Response: 3553057
Conc: 27.28 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

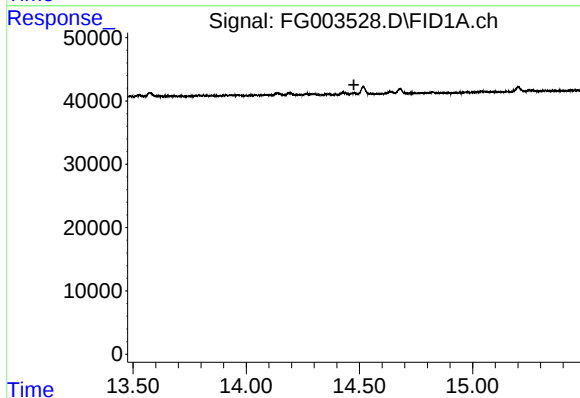


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.476 min
Response: 0
Conc: N.D.

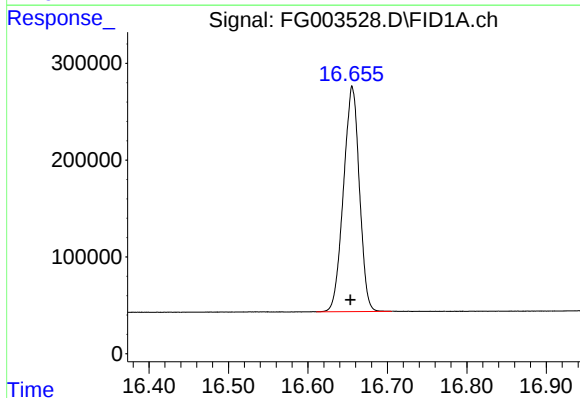


#12 N-OCTACOSANE

R.T.: 16.656 min
Delta R.T.: 0.003 min
Response: 3237946
Conc: 22.81 ug/ml

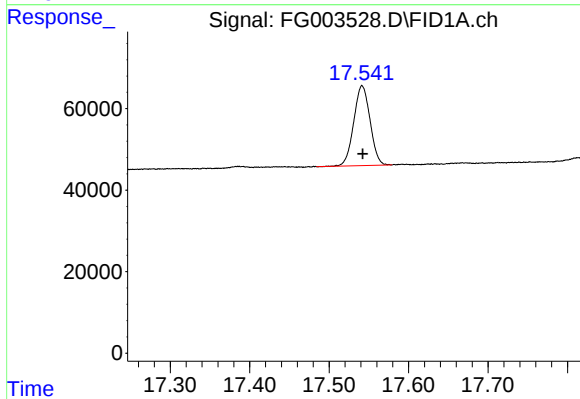

#13 N-TRIACONTANE


R.T.: 17.542 min
Delta R.T.: 0.000 min
Response: 280146
Conc: 1.99 ug/ml

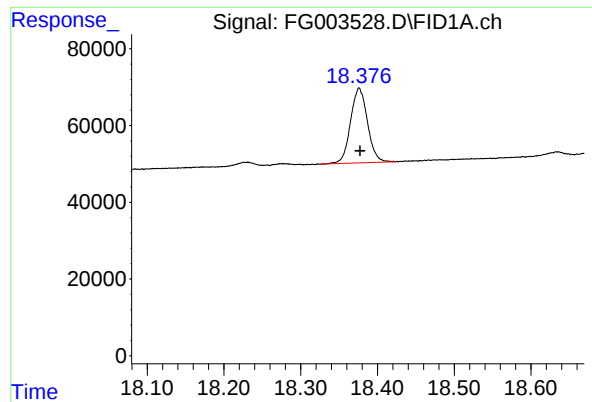

#14 N-DOTRIACONTANE

R.T.: 18.376 min
Delta R.T.: -0.001 min
Response: 297802
Conc: 2.20 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

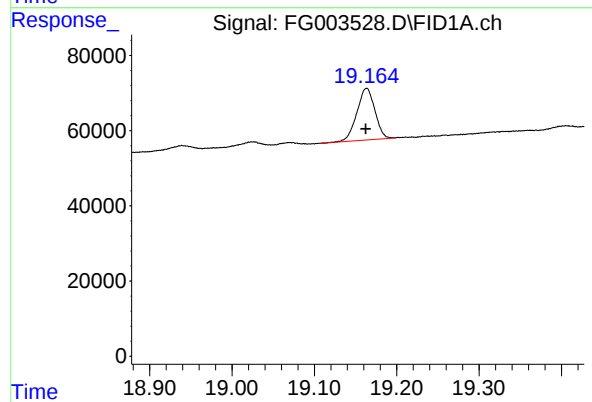

#15 N-TETRATRIACONTANE

R.T.: 19.163 min
Delta R.T.: 0.000 min
Response: 207768
Conc: 1.61 ug/ml