

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003532.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 11:59
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jan 19 02:54:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.476	2286039	17.619 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.376	216442	1.600 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003532.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 11:59
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jan 19 02:54:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

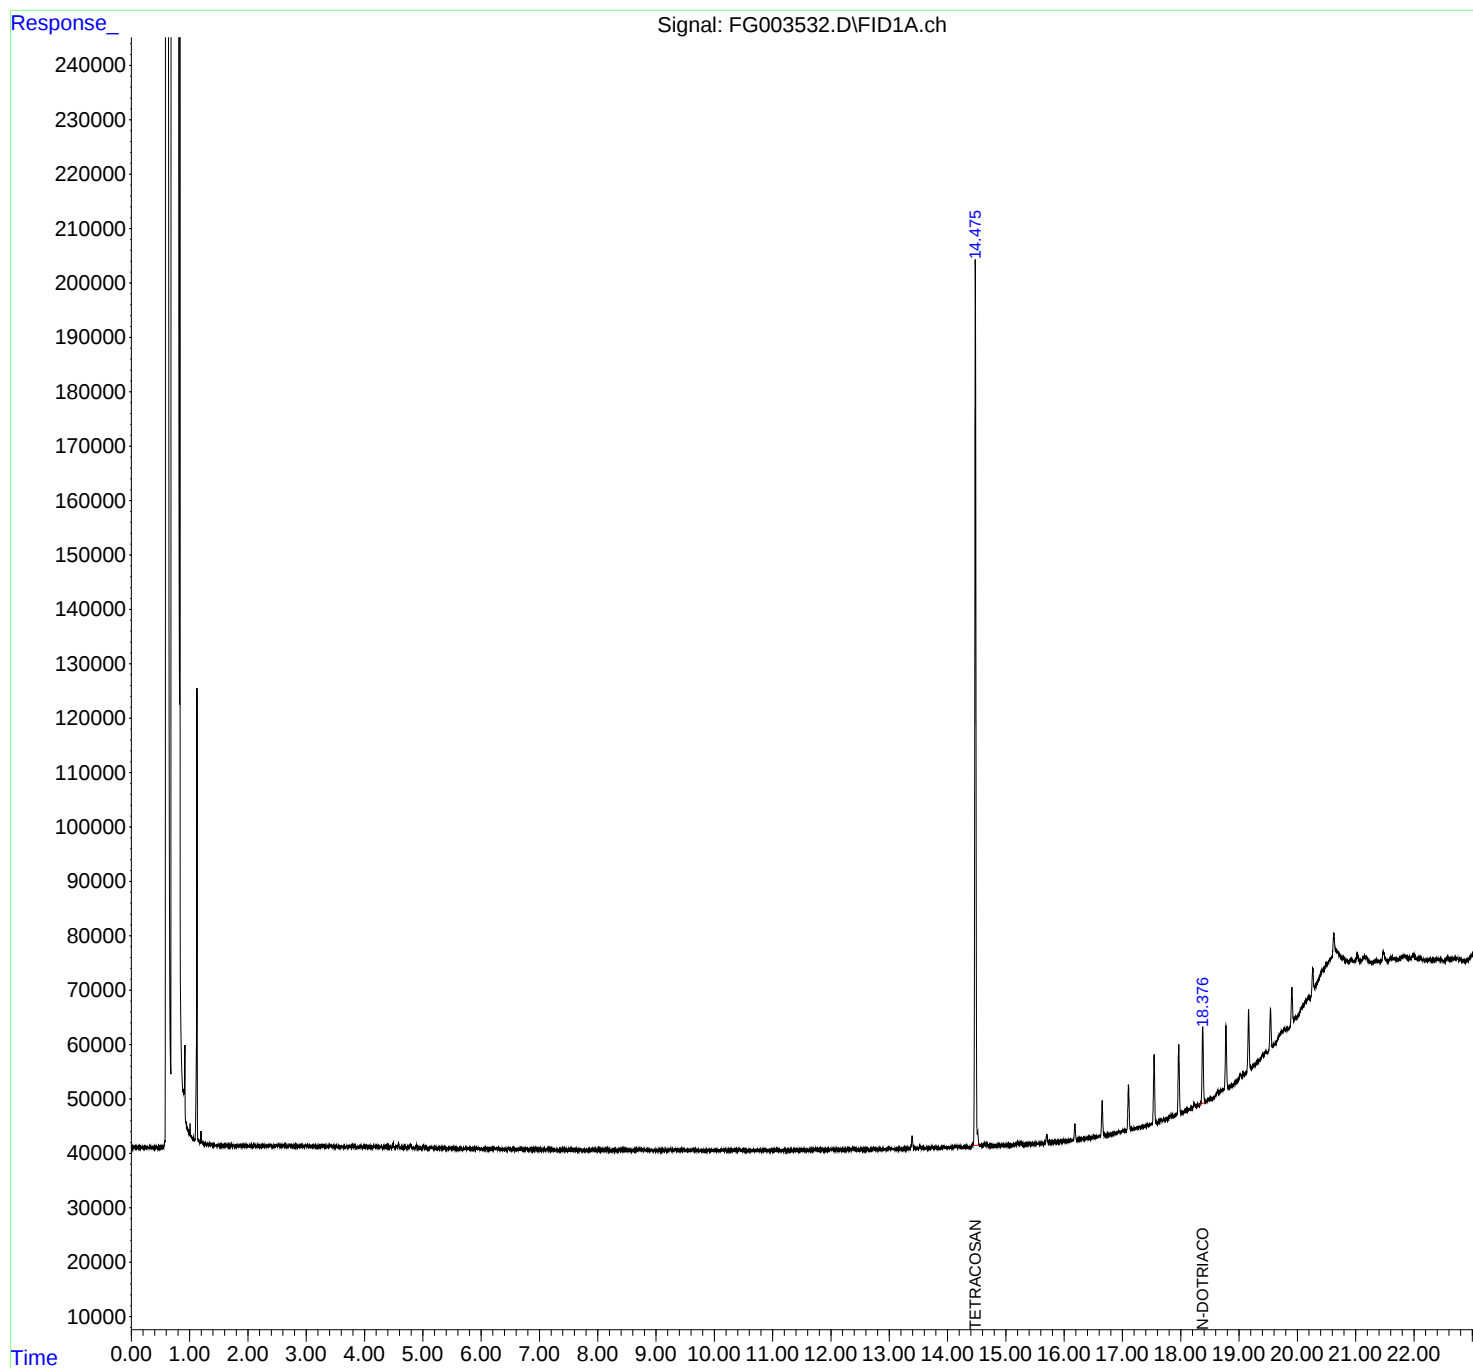


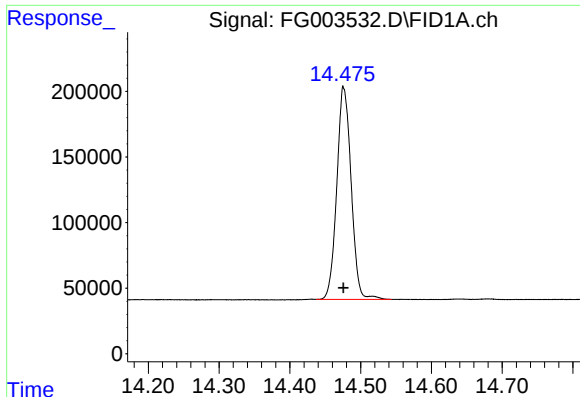

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.476 min
Delta R.T.: 0.000 min
Response: 2286039
Conc: 17.62 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

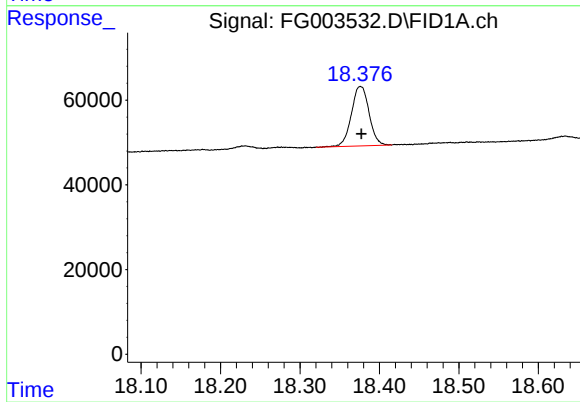

#14 N-DOTRIACONTANE

R.T.: 18.376 min
Delta R.T.: -0.001 min
Response: 216442
Conc: 1.60 ug/ml