

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003536.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 13:59
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jan 19 02:55:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.226	3625893	27.839 ug/ml
12)	N-OCTACOSANE	16.655	3342702	23.552 ug/ml
13)	N-TRIACONTANE	17.539	305648	2.169 ug/ml
14)	N-DOTRIACONTANE	18.376	315854	2.335 ug/ml
15)	N-TETRATRIACONTANE	19.161	229425	1.782 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003536.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 13:59
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jan 19 02:55:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

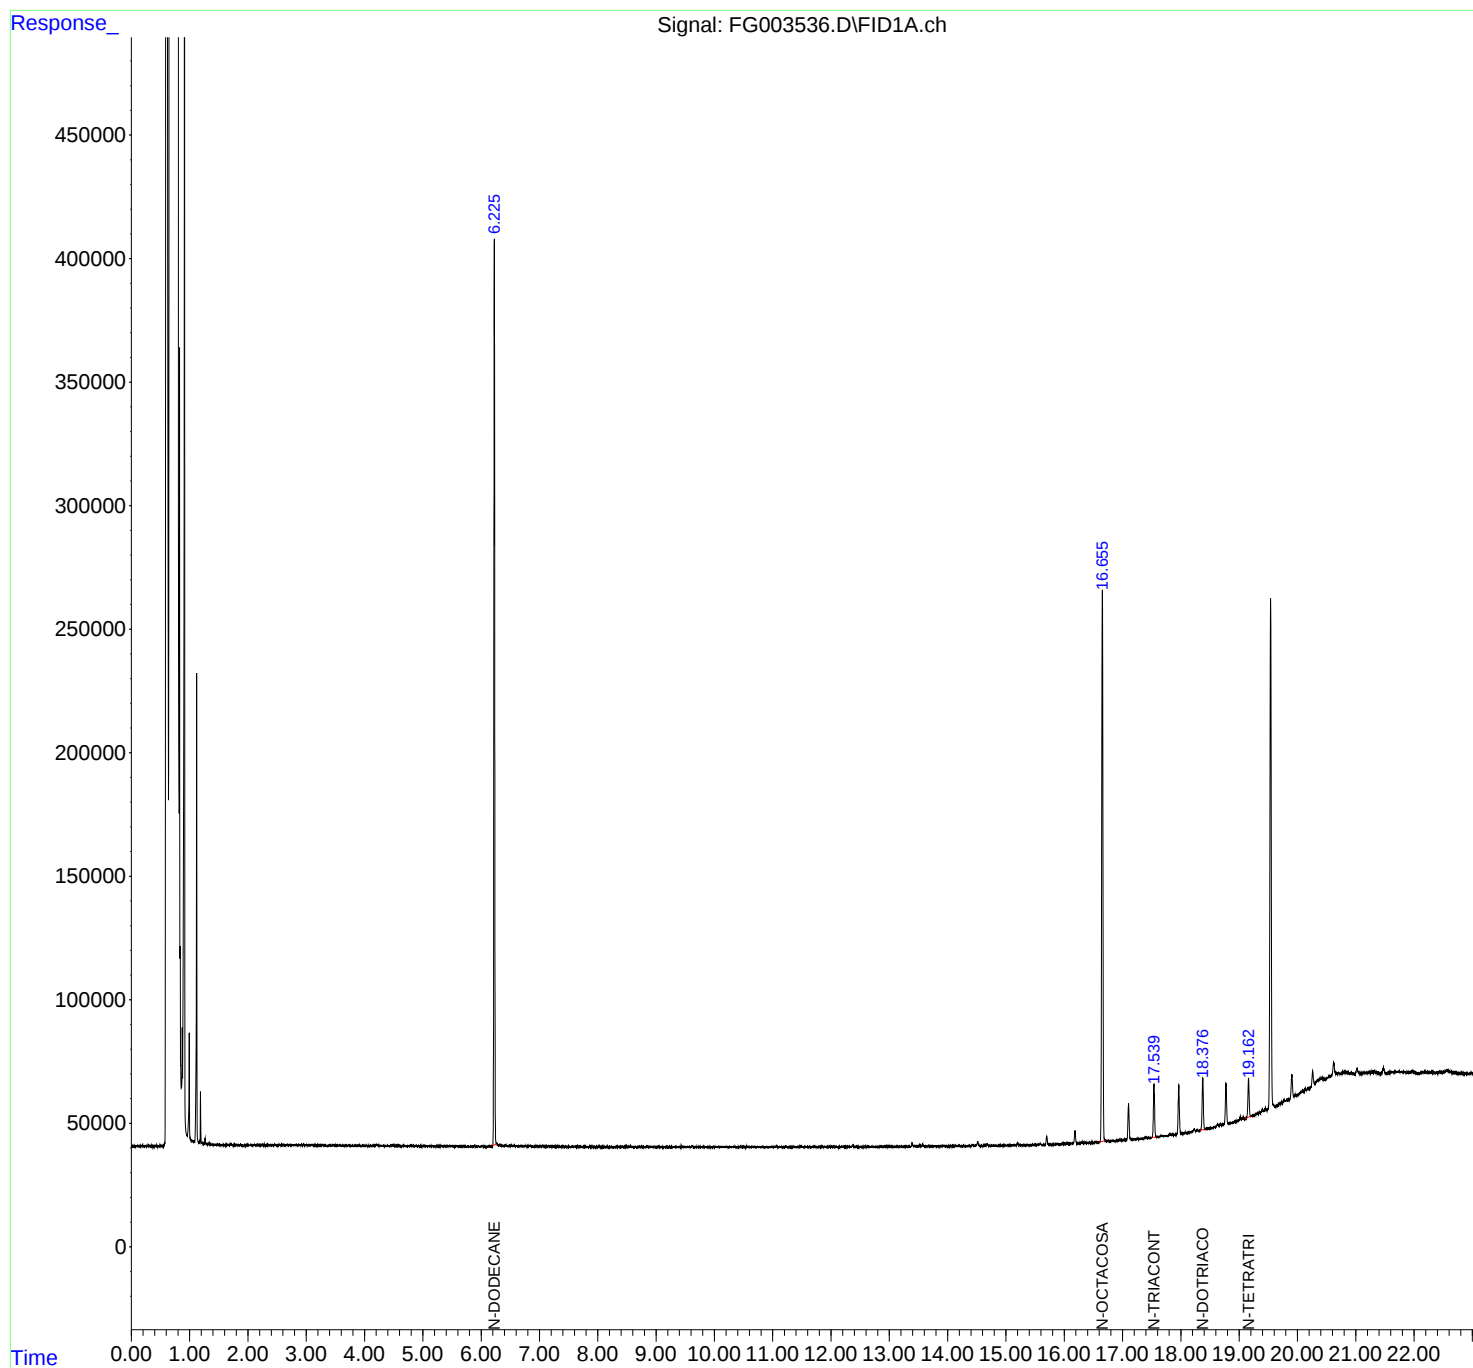


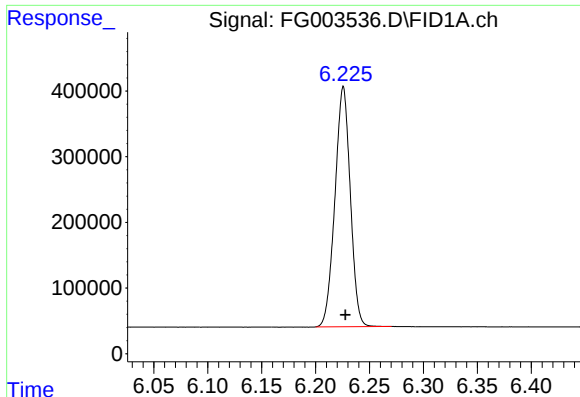

#3 N-DODECANE


R.T.: 6.226 min
Delta R.T.: -0.002 min
Response: 3625893
Conc: 27.84 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

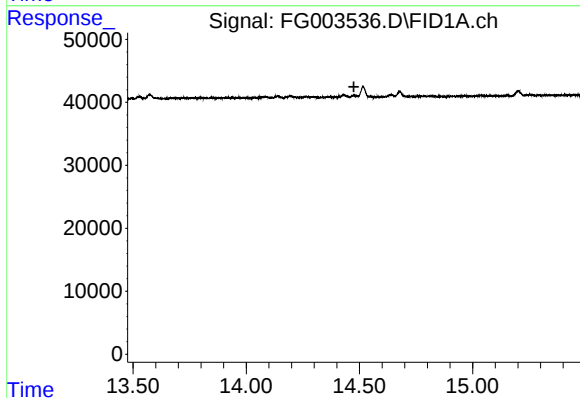


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.476 min
Response: 0
Conc: N.D.

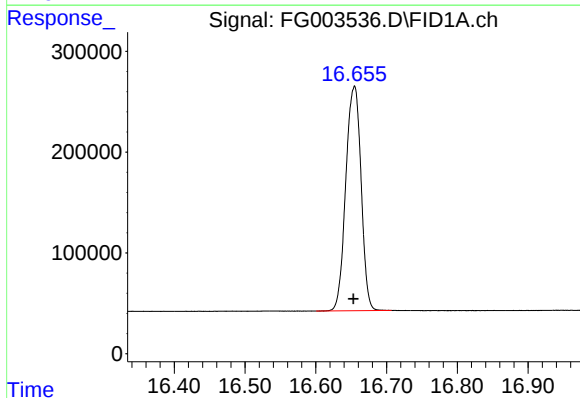


#12 N-OCTACOSANE

R.T.: 16.655 min
Delta R.T.: 0.001 min
Response: 3342702
Conc: 23.55 ug/ml

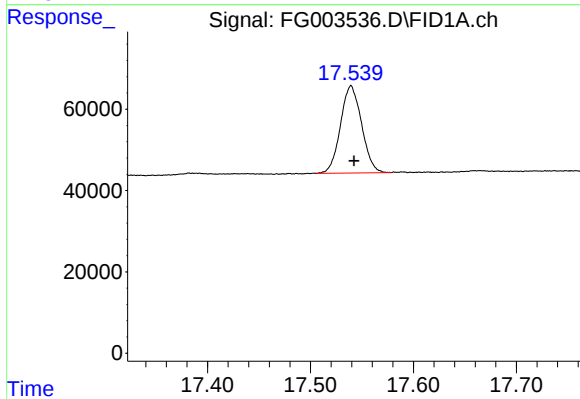

#13 N-TRIACONTANE


R.T.: 17.539 min
Delta R.T.: -0.003 min
Response: 305648
Conc: 2.17 ug/ml

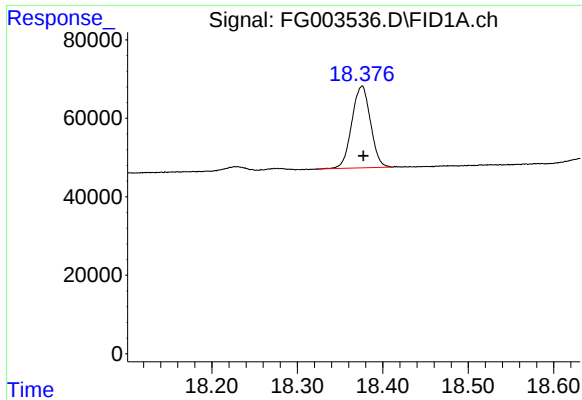

#14 N-DOTRIACONTANE

R.T.: 18.376 min
Delta R.T.: -0.002 min
Response: 315854
Conc: 2.34 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

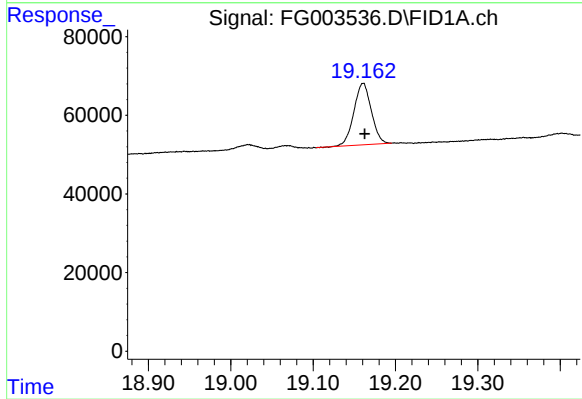

#15 N-TETRATRIACONTANE

R.T.: 19.161 min
Delta R.T.: -0.002 min
Response: 229425
Conc: 1.78 ug/ml