

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003537.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 14:29
Operator : AJ\SJ
Sample : K1180-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 22 09:12:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.476	2010146	15.492 ug/ml
Target Compounds			
4) N-TETRADECANE	8.073f	610055	4.470 ug/ml
12) N-OCTACOSANE	16.651	328221	2.313 ug/ml
13) N-TRIACONTANE	17.541	369597	2.623 ug/ml
14) N-DOTRIACONTANE	18.375	218646	1.616 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003537.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 14:29
Operator : AJ\SJ
Sample : K1180-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 22 09:12:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

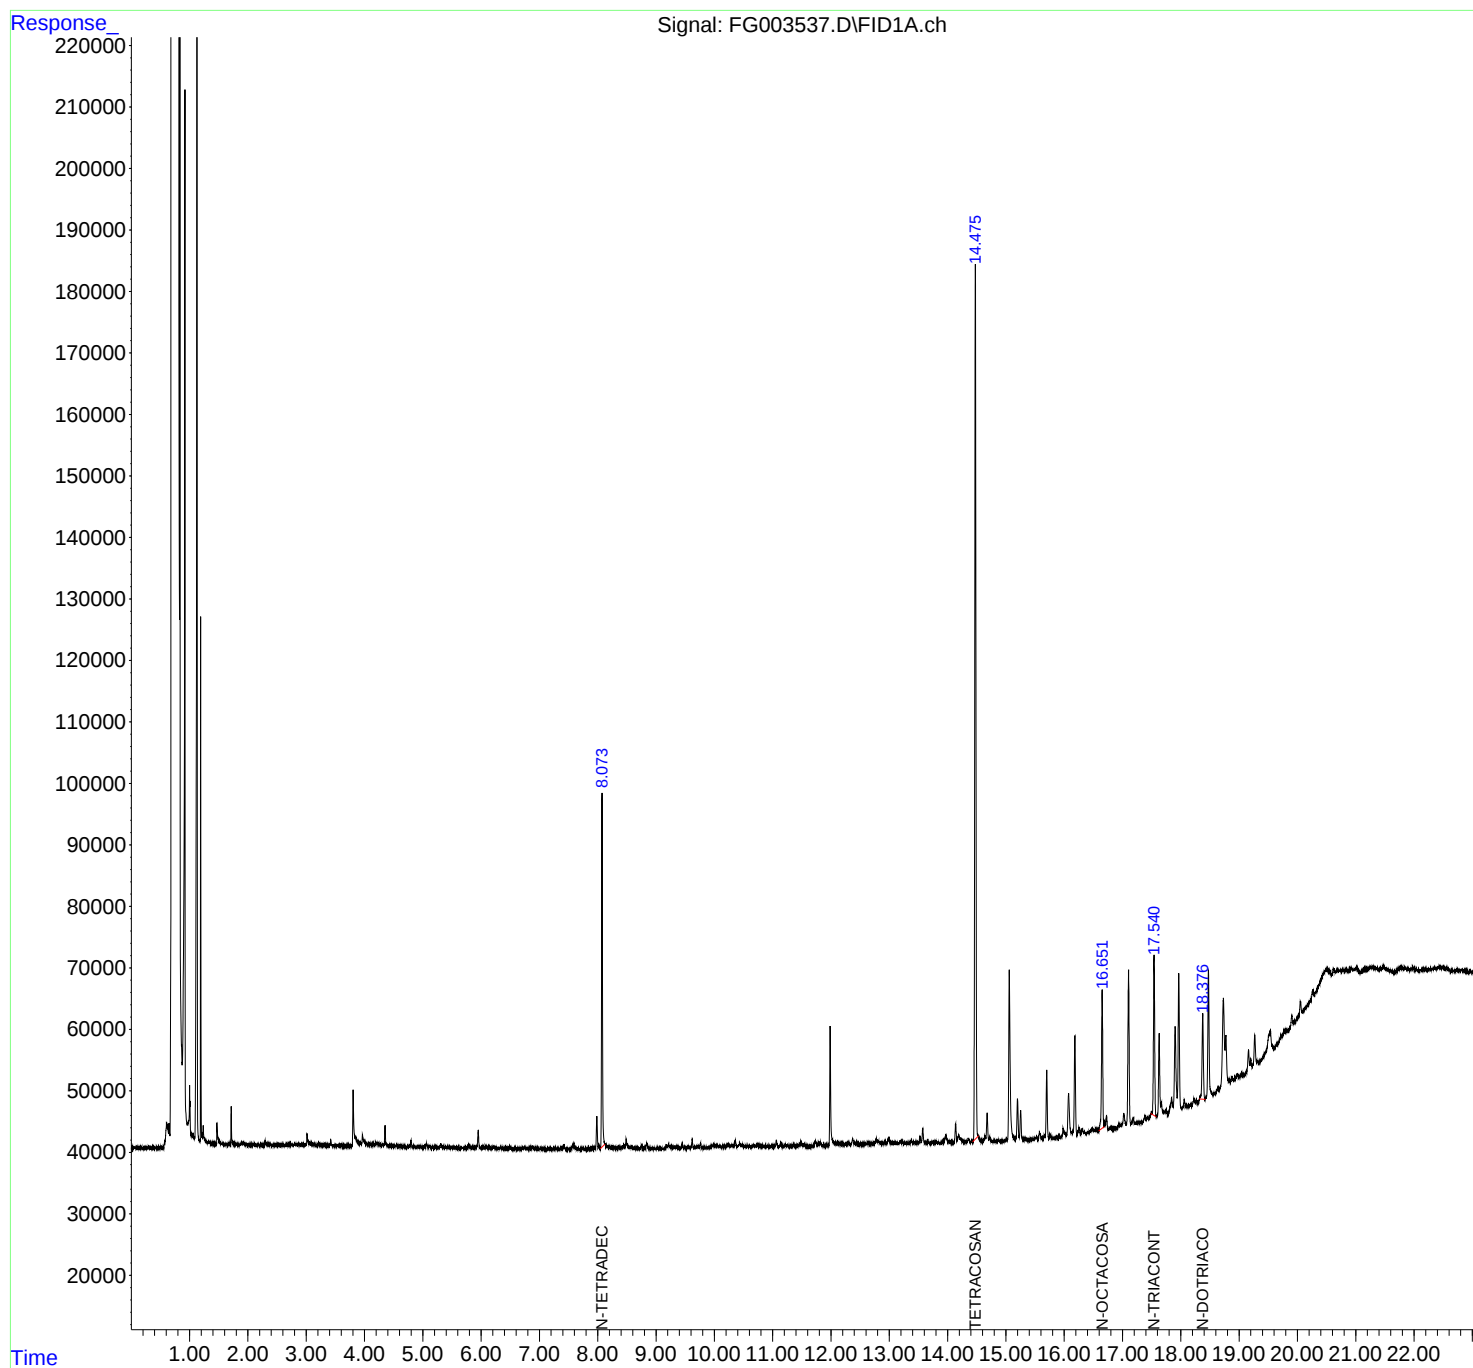

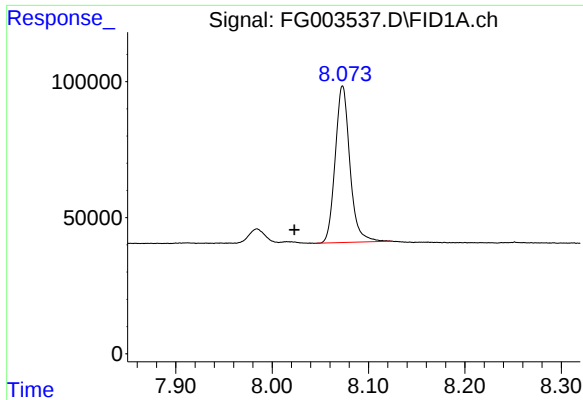


#4 N-TETRADECANE

R.T.: 8.073 min
Delta R.T.: 0.050 min
Response: 610055
Conc: 4.47 ug/ml

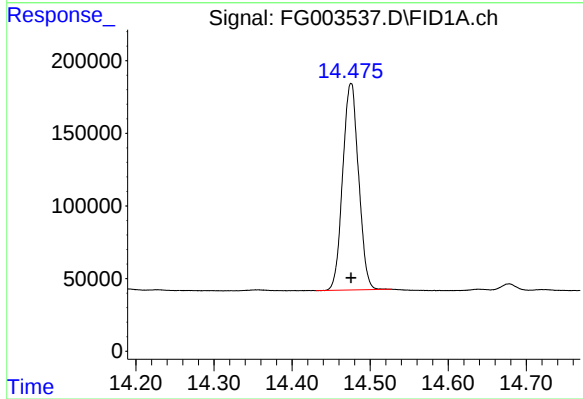


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.476 min
Delta R.T.: 0.000 min
Response: 2010146
Conc: 15.49 ug/ml

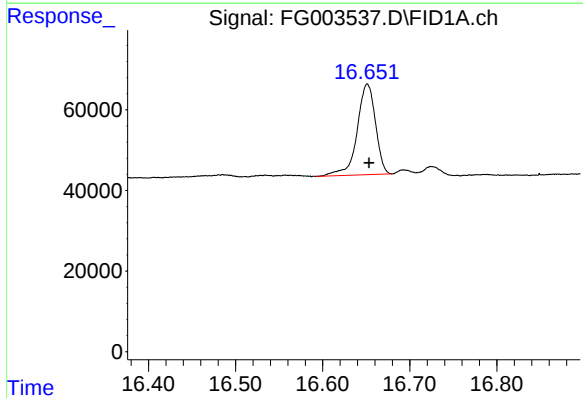


#12 N-OCTACOSANE

R.T.: 16.651 min
Delta R.T.: -0.002 min
Response: 328221
Conc: 2.31 ug/ml

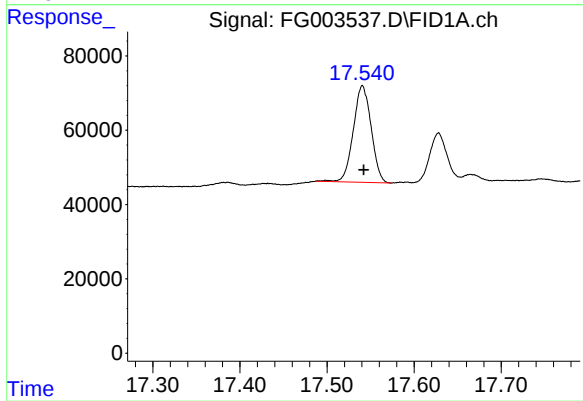

#13 N-TRIACONTANE

R.T.: 17.541 min
Delta R.T.: -0.002 min
Response: 369597
Conc: 2.62 ug/ml

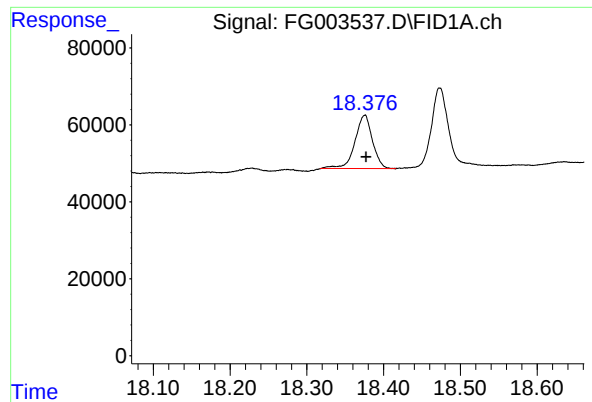

#14 N-DOTRIACONTANE

R.T.: 18.375 min
Delta R.T.: -0.002 min
Response: 218646
Conc: 1.62 ug/ml