

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
 Data File : FG003544.D
 Signal(s) : FID1A.ch
 Acq On : 18 Jan 2019 17:58
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Jan 19 02:57:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
 Quant Title :
 QLast Update : Wed Jan 09 08:22:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.475	2346773	18.087 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.540	226319	1.606 ug/ml
14) N-DOTRIACONTANE	18.375	270668	2.001 ug/ml
15) N-TETRATRIACONTANE	19.160	200592	1.558 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011819\
Data File : FG003544.D
Signal(s) : FID1A.ch
Acq On : 18 Jan 2019 17:58
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jan 19 02:57:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010819.M
Quant Title :
QLast Update : Wed Jan 09 08:22:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

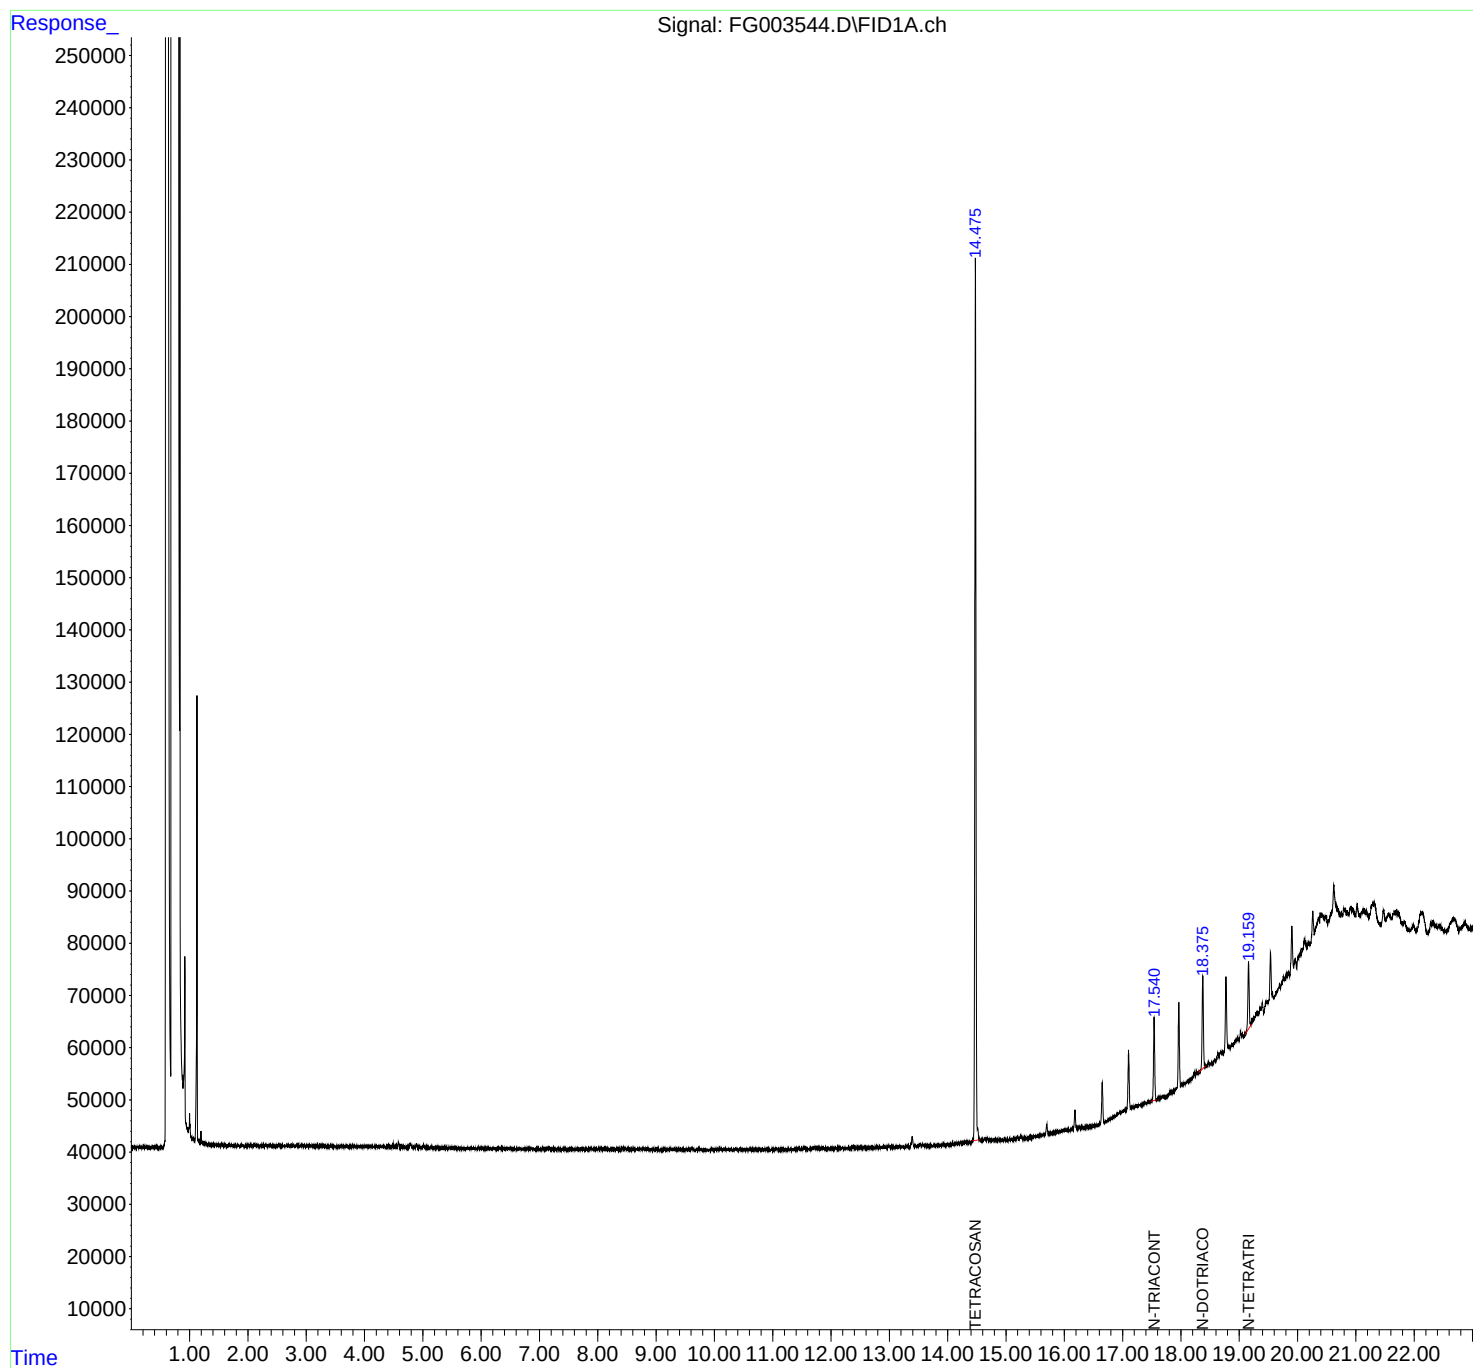


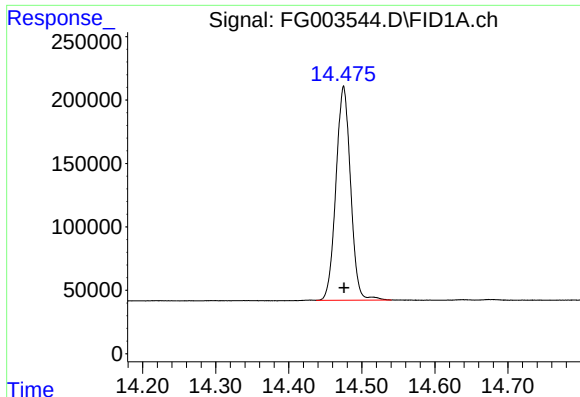

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.475 min
Delta R.T.: 0.000 min
Response: 2346773
Conc: 18.09 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

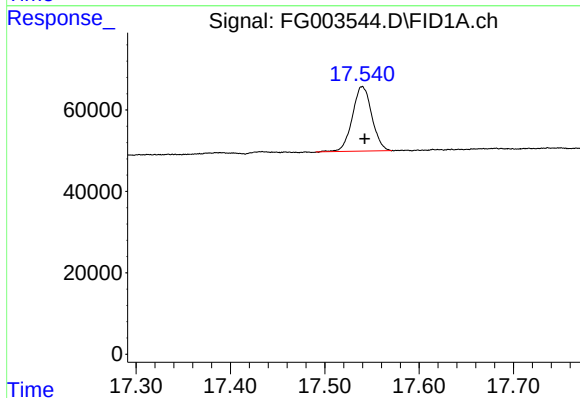


#13 N-TRIACONTANE

R.T.: 17.540 min
Delta R.T.: -0.003 min
Response: 226319
Conc: 1.61 ug/ml

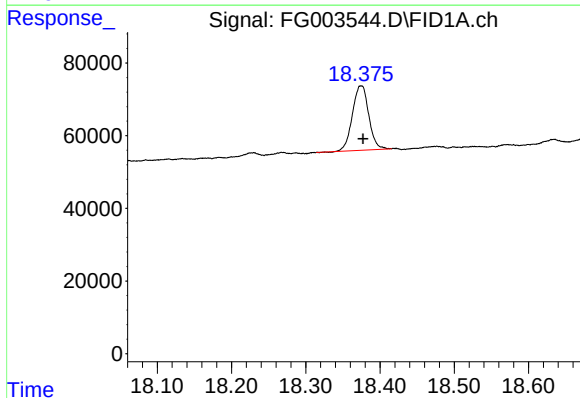

#14 N-DOTRIACONTANE

R.T.: 18.375 min
Delta R.T.: -0.003 min
Response: 270668
Conc: 2.00 ug/ml

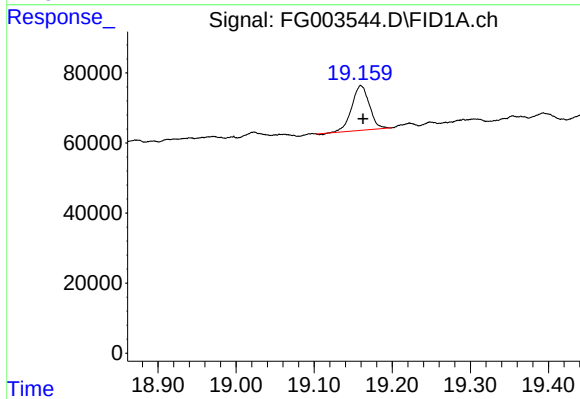

#15 N-TETRATRIACONTANE

R.T.: 19.160 min
Delta R.T.: -0.003 min
Response: 200592
Conc: 1.56 ug/ml