

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012221\
Data File : FG007561.D
Signal(s) : FID1A.ch
Acq On : 22 Jan 2021 12:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 21:43:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.636	2284710	19.065 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.810	91911	0.672 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012221\
Data File : FG007561.D
Signal(s) : FID1A.ch
Acq On : 22 Jan 2021 12:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 22 21:43:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

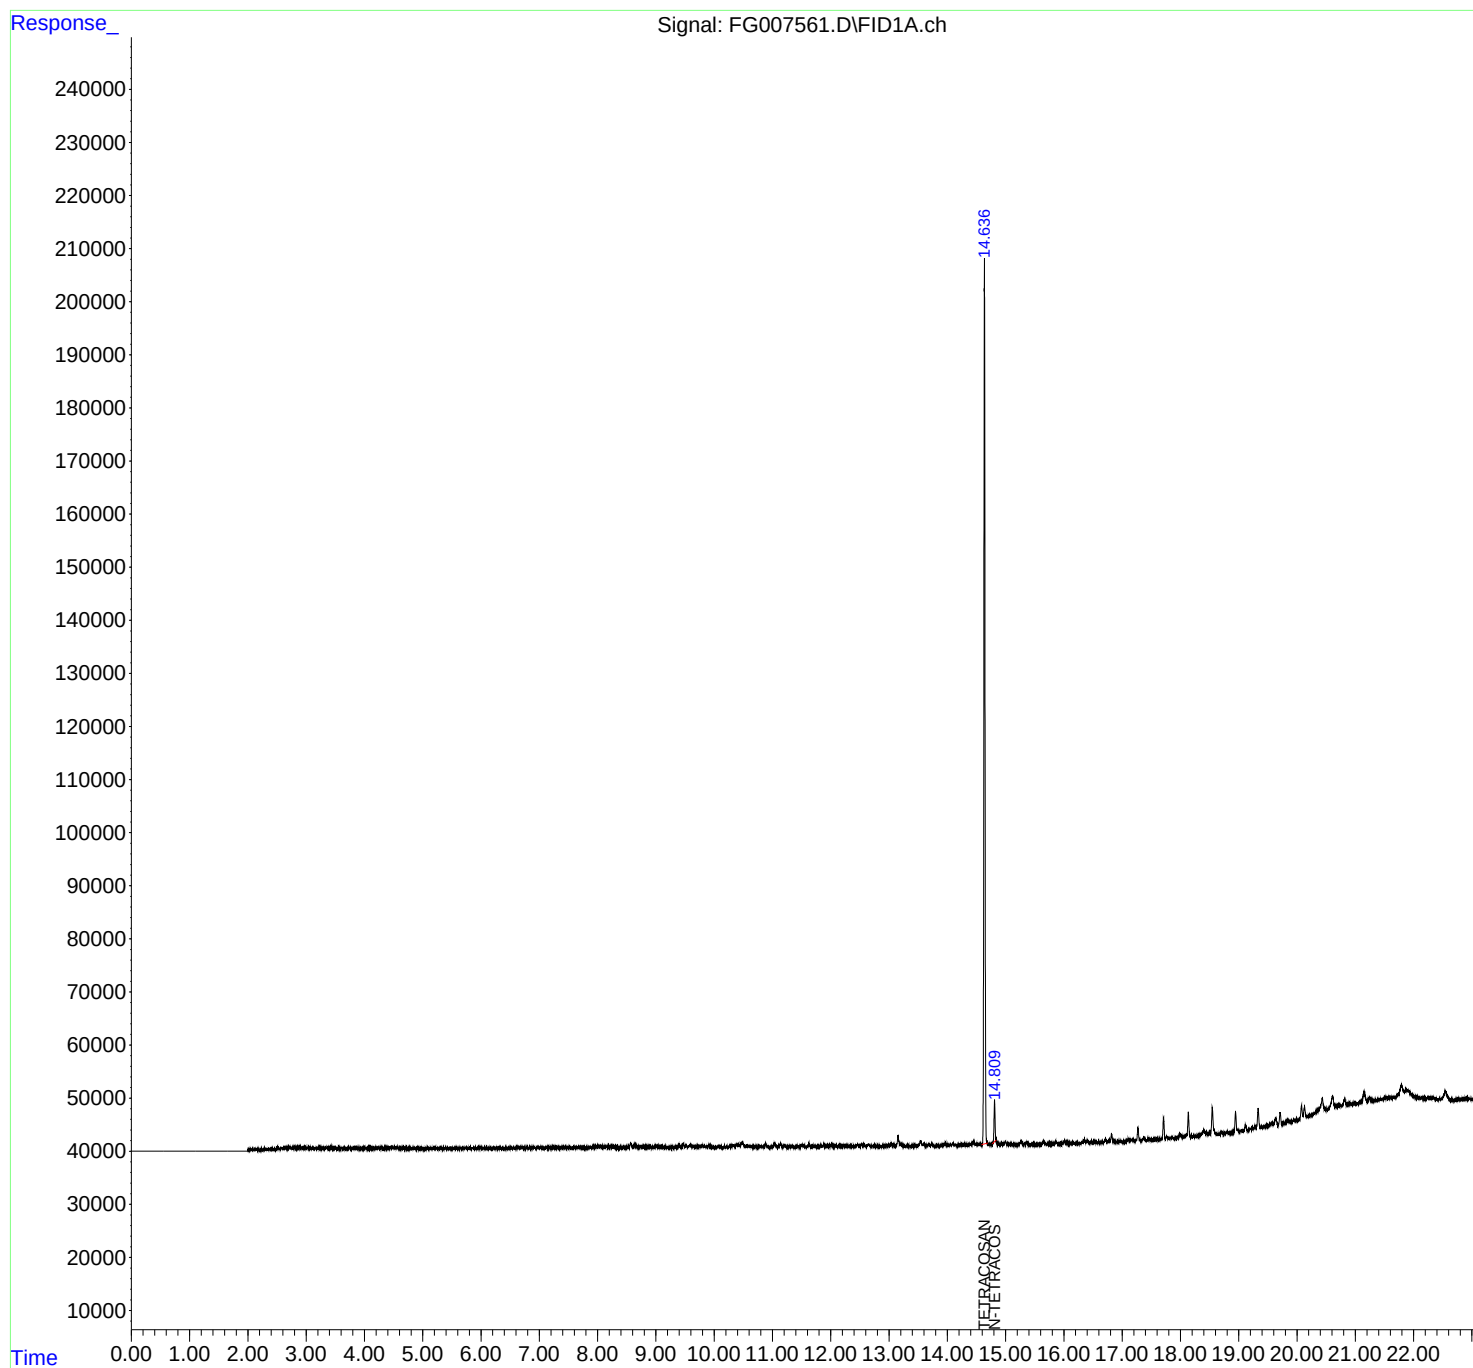


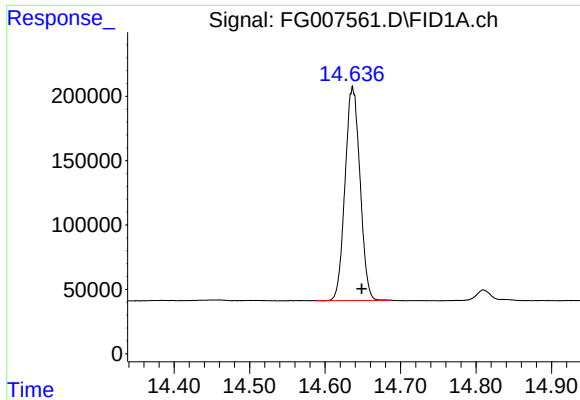

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.012 min
Response: 2284710
Conc: 19.06 ug/ml

Instrument :
FID_G
ClientSampleId :

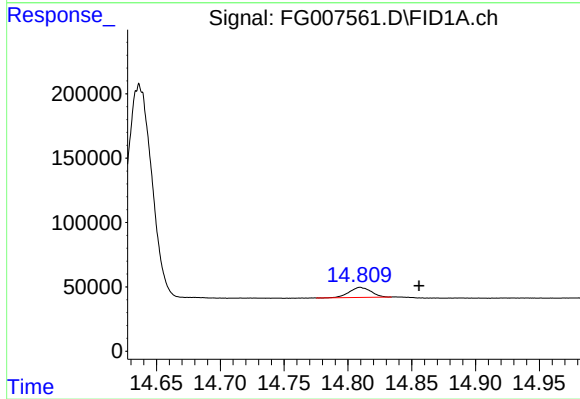

#10 N-TETRACOSANE

R.T.: 14.810 min
Delta R.T.: -0.046 min
Response: 91911
Conc: 0.67 ug/ml