

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012325\
Data File : FG015155.D
Signal(s) : FID1A.ch
Acq On : 24 Jan 2025 02:35
Operator : YP\AJ
Sample : Q1168-07
Misc : 1 PPM WATER LOD
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 04:08:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG011325.M
Quant Title :
QLast Update : Mon Jan 13 11:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.045	2105834	16.417 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012325\
Data File : FG015155.D
Signal(s) : FID1A.ch
Acq On : 24 Jan 2025 02:35
Operator : YP\AJ
Sample : Q1168-07
Misc : 1 PPM WATER LOD
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 24 04:08:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG011325.M
Quant Title :
QLast Update : Mon Jan 13 11:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

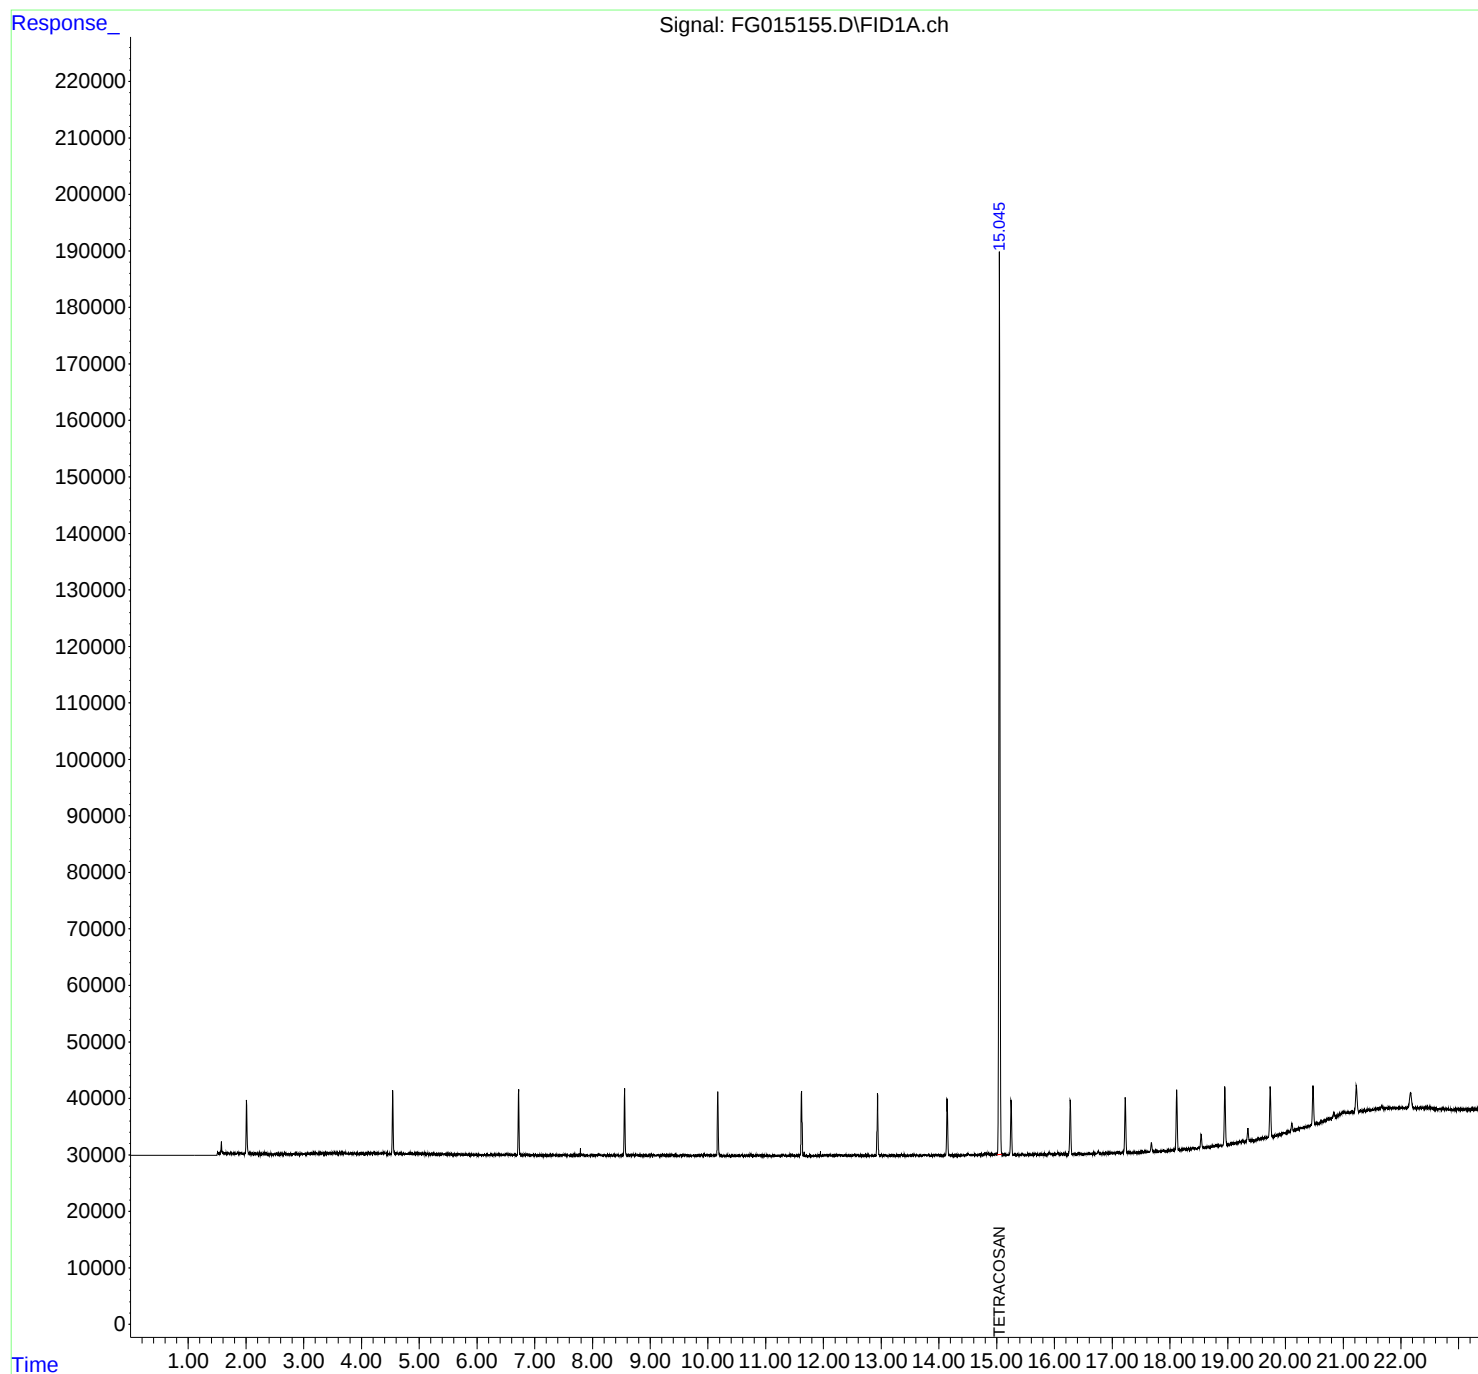

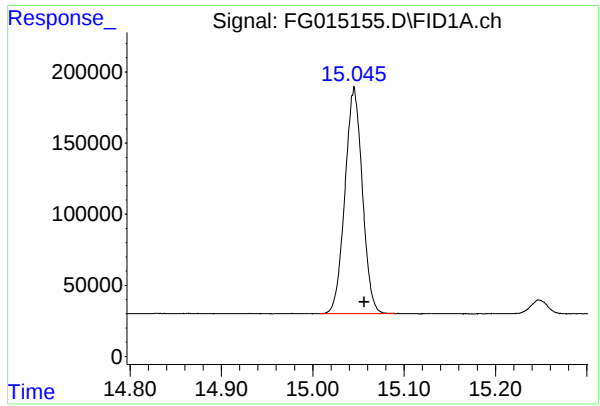

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.045 min
Delta R.T.: -0.011 min
Response: 2105834
Conc: 16.42 ug/ml

Instrument :
FID_G
ClientSampleId :