

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012325AL\
Data File : FG015128.D
Signal(s) : FID1A.ch
Acq On : 23 Jan 2025 04:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 23 07:18:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 011425.M
Quant Title : GC Extractables
QLast Update : Tue Jan 14 11:45:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.117	63648	0.480 ug/ml
18) T	n-Dotriacontane (C32)	18.953	75721	0.600 ug/ml
19) T	n-Tetratriacontane (C34)	19.738	54358	0.499 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012325AL\
Data File : FG015128.D
Signal(s) : FID1A.ch
Acq On : 23 Jan 2025 04:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 23 07:18:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 011425.M
Quant Title : GC Extractables
QLast Update : Tue Jan 14 11:45:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

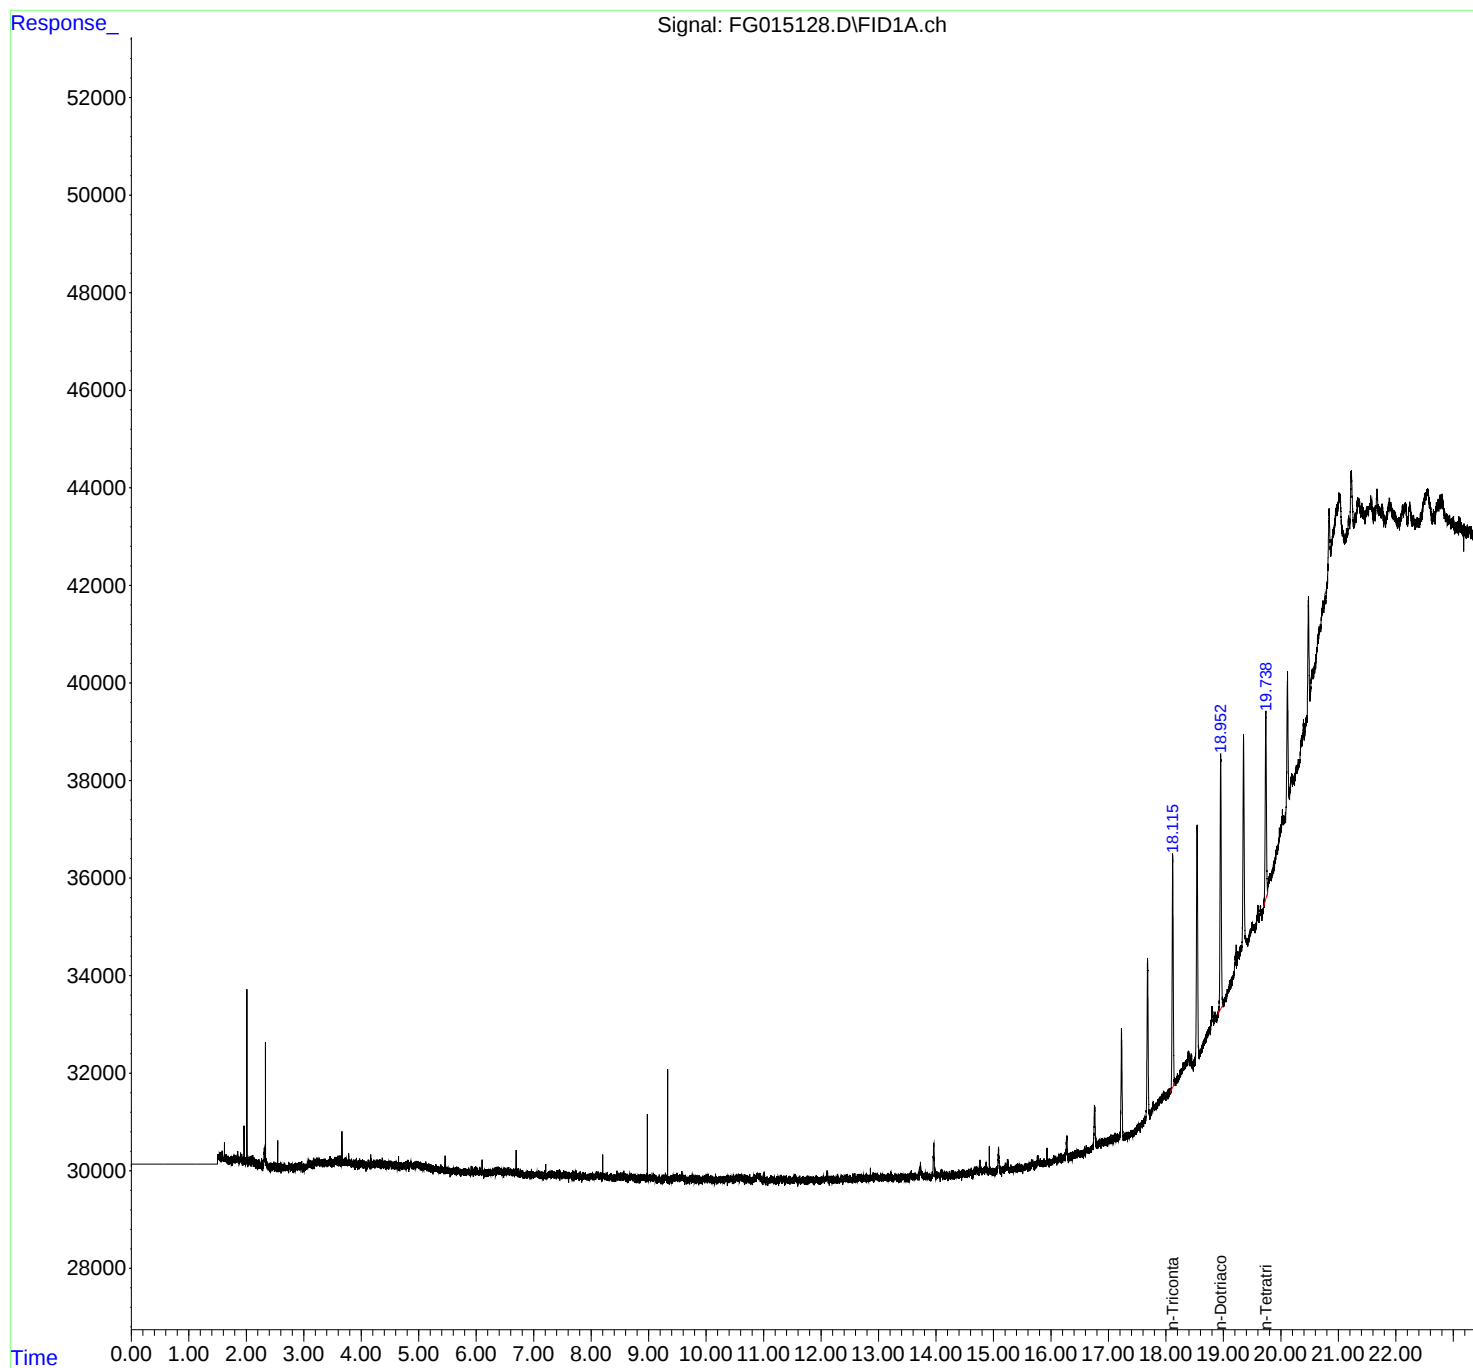


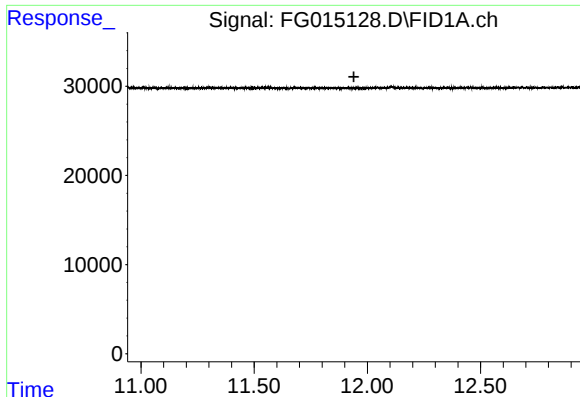

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.940 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

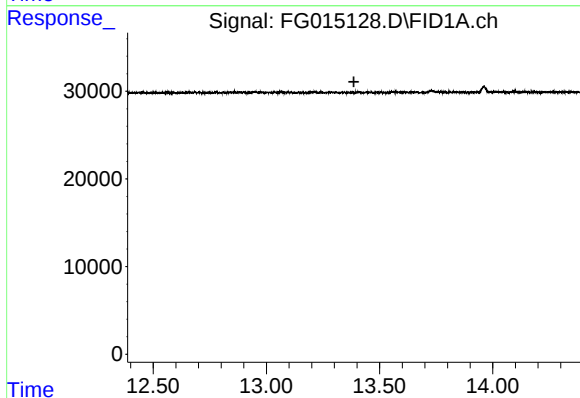


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.387 min
Response: 0
Conc: N.D.

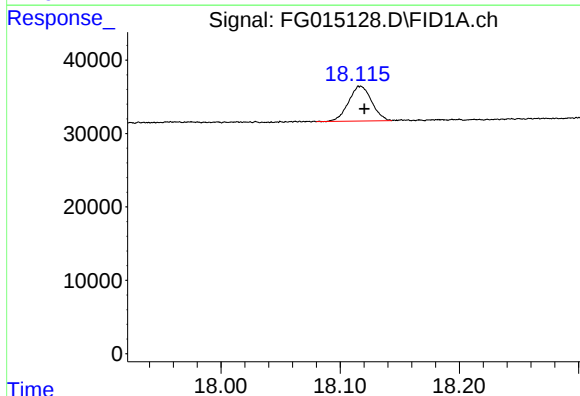


#17 n-Tricontane (C30)

R.T.: 18.117 min
Delta R.T.: -0.003 min
Response: 63648
Conc: 0.48 ug/ml

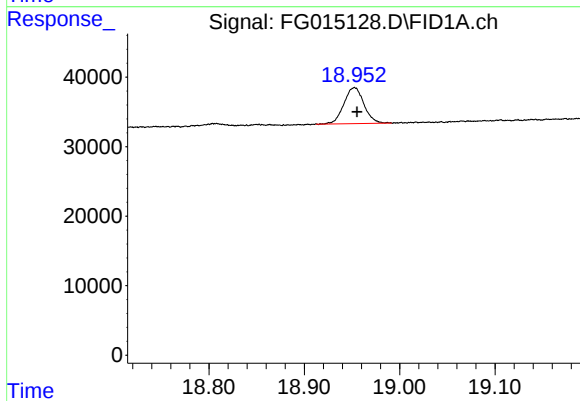

#18 n-Dotriacontane (C32)

R.T.: 18.953 min
Delta R.T.: -0.002 min
Response: 75721
Conc: 0.60 ug/ml

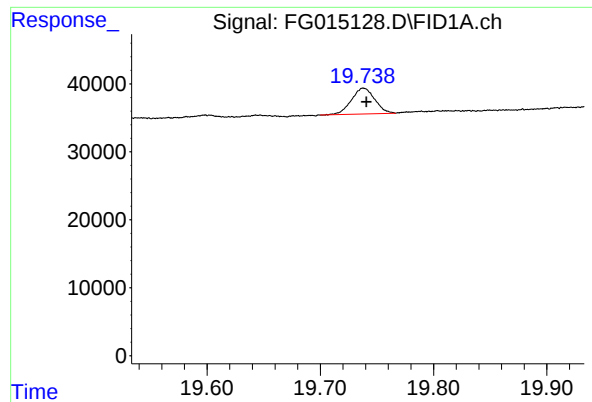

#19 n-Tetratriacontane (C34)

R.T.: 19.738 min
Delta R.T.: -0.003 min
Response: 54358
Conc: 0.50 ug/ml

Instrument :

FID_G

ClientSampleId :