

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012621\
Data File : FG007580.D
Signal(s) : FID1A.ch
Acq On : 26 Jan 2021 15:01
Operator : DD\AJ
Sample : PB134331BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB134331BL

Integration File: Sample.e
Quant Time: Jan 27 00:29:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	2084909	17.397 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012621\
Data File : FG007580.D
Signal(s) : FID1A.ch
Acq On : 26 Jan 2021 15:01
Operator : DD\AJ
Sample : PB134331BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB134331BL

Integration File: Sample.e
Quant Time: Jan 27 00:29:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

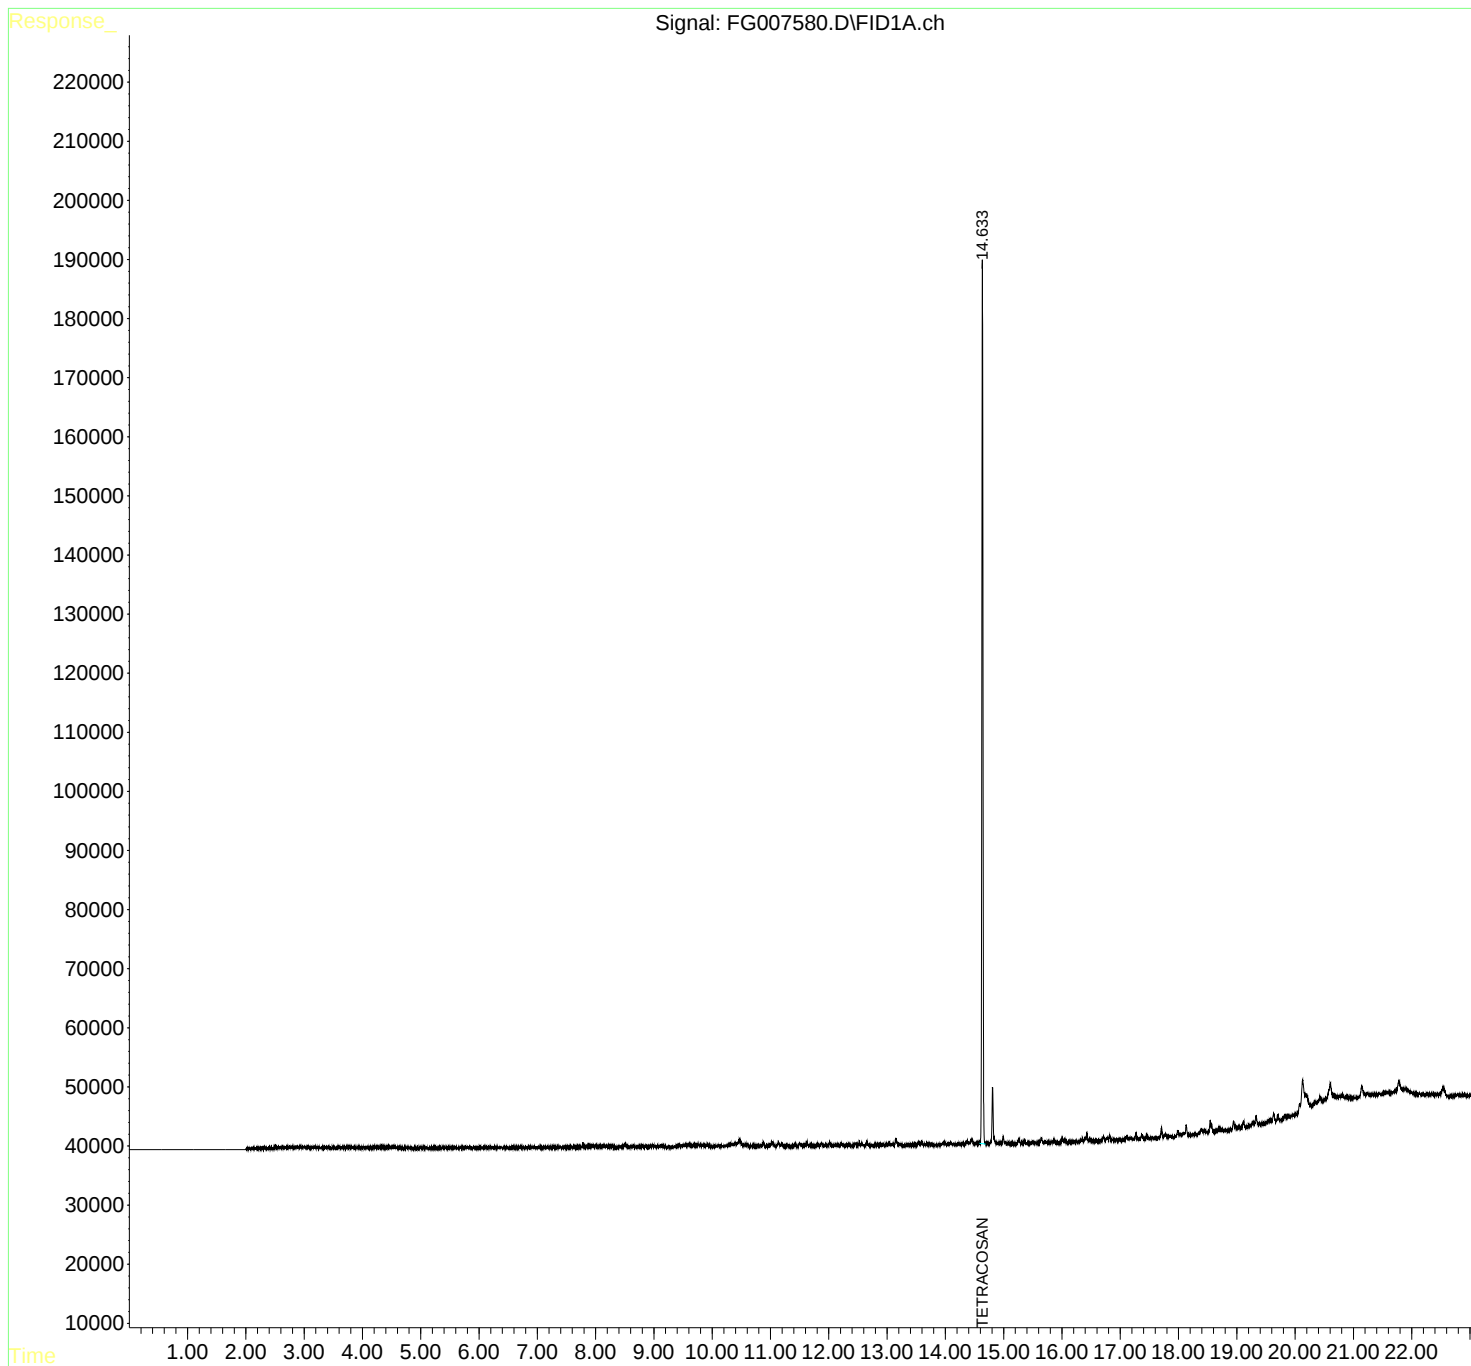

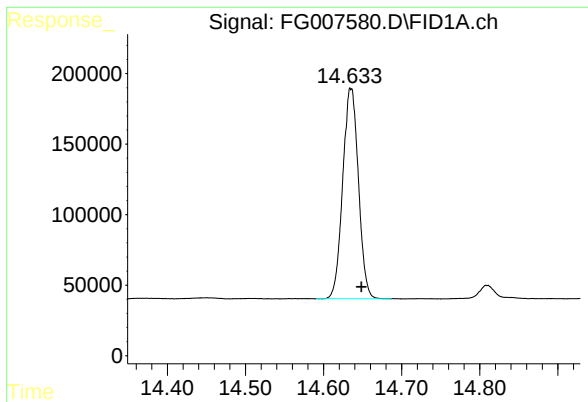

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.635 min
Delta R.T.: -0.014 min
Response: 2084909
Conc: 17.40 ug/ml

Instrument :
FID_G
ClientSampleId :
PB134331BL