

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012621\
Data File : FG007582.D
Signal(s) : FID1A.ch
Acq On : 26 Jan 2021 16:03
Operator : DD\AJ
Sample : M1234-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
HOLLAND-TUNNEL-TEST-PIT-5

Manual Integrations
APPROVED

mohammad
1/27/2021 5:23:25 PM

Integration File: autoint1.e
Quant Time: Jan 27 00:29:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	2619427	21.858 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012621\
Data File : FG007582.D
Signal(s) : FID1A.ch
Acq On : 26 Jan 2021 16:03
Operator : DD\AJ
Sample : M1234-01
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
HOLLAND-TUNNEL-TEST-PIT-5


Manual Integrations
APPROVED

mohammad
1/27/2021 5:23:25 PM

Integration File: autoint1.e
Quant Time: Jan 27 00:29:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

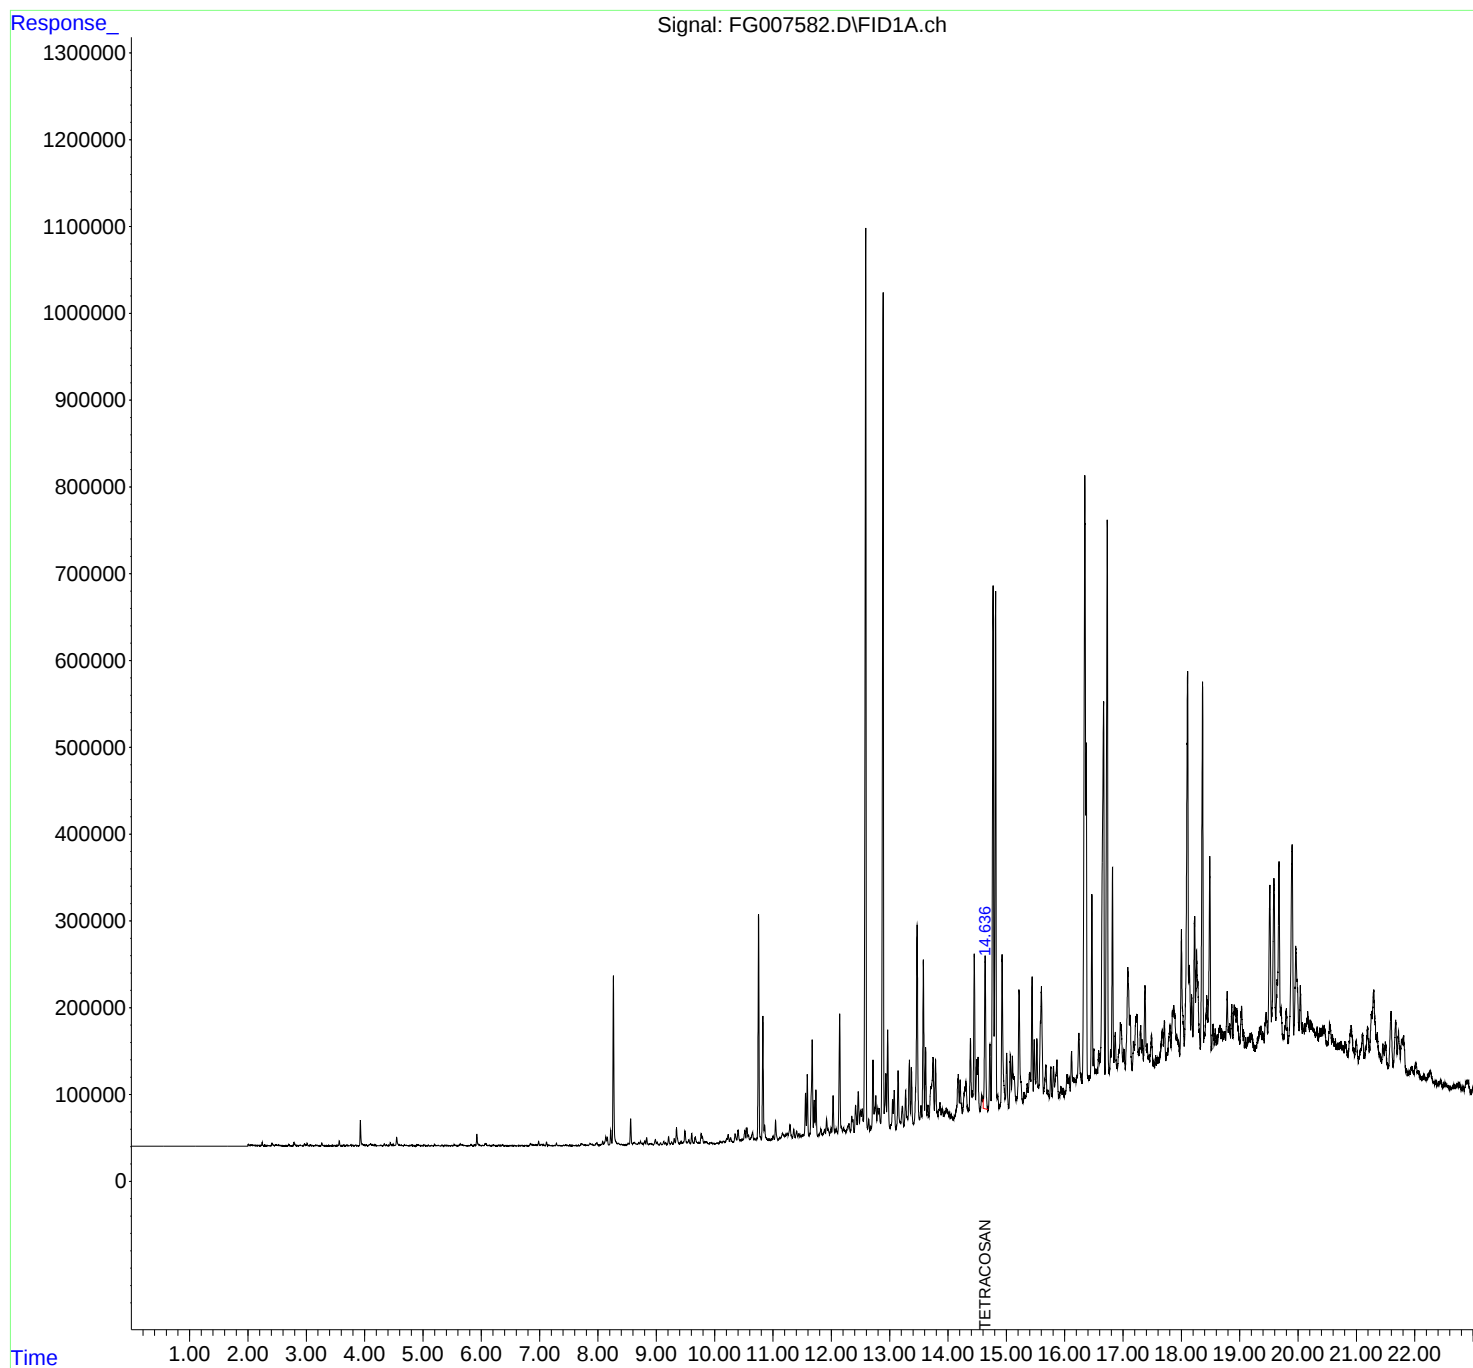

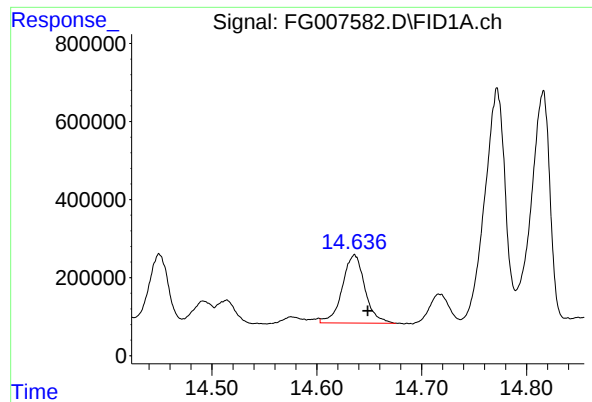

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.013 min
Response: 2619427
Conc: 21.86 ug/ml m

Instrument :
FID_G
ClientSampleId :
HOLLAND-TUNNEL-TEST-PIT-5

Manual Integrations
APPROVED

mohammad
1/27/2021 5:23:25 PM