

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012621\
 Data File : FG007586.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jan 2021 18:07
 Operator : DD\AJ
 Sample : M1234-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 HOLLAND-TUNNEL-TEST-PIT-5

Manual Integrations
 APPROVED

mohammad
 1/27/2021 5:23:38 PM

Integration File: Sample.e
 Quant Time: Jan 27 00:30:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
 Quant Title :
 QLast Update : Tue Jan 05 02:18:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.642	229593	1.916 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012621\
Data File : FG007586.D
Signal(s) : FID1A.ch
Acq On : 26 Jan 2021 18:07
Operator : DD\AJ
Sample : M1234-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
HOLLAND-TUNNEL-TEST-PIT-5


Manual Integrations
APPROVED

mohammad
1/27/2021 5:23:38 PM

Integration File: Sample.e
Quant Time: Jan 27 00:30:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

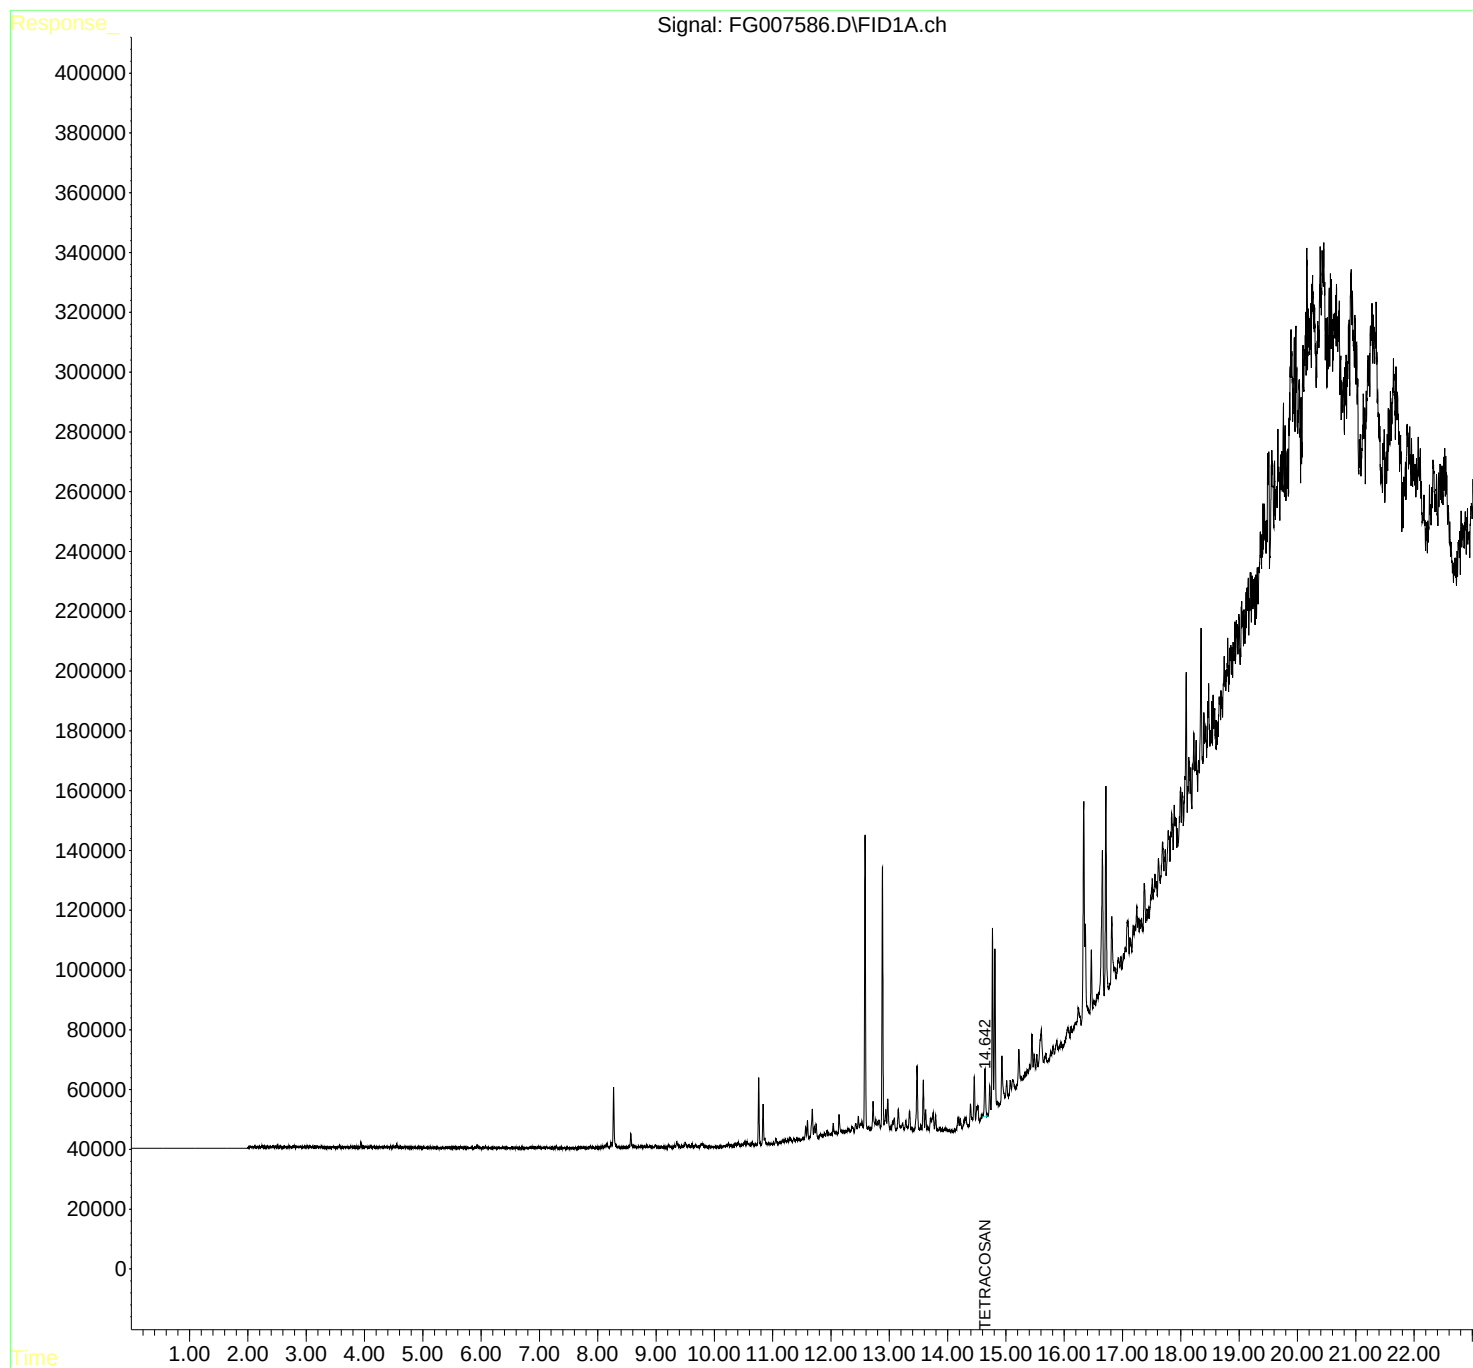

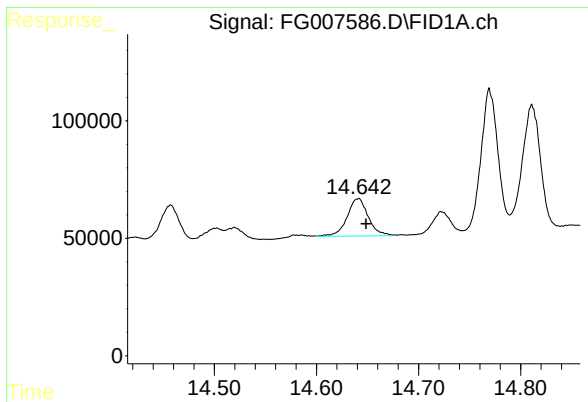

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min
Delta R.T.: -0.007 min
Response: 229593
Conc: 1.92 ug/ml m

Instrument :
FID_G
ClientSampleId :
HOLLAND-TUNNEL-TEST-PIT-5

Manual Integrations
APPROVED

mohammad
1/27/2021 5:23:38 PM