

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012825AL\
 Data File : FG015190.D
 Signal(s) : FID1A.ch
 Acq On : 28 Jan 2025 19:11
 Operator : YP\AJ
 Sample : Q1194-01D
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 02:36:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 011425.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 14 11:45:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.385	5747946	47.206 ug/ml
Spiked Amount 50.000		Recovery =	94.41%
Target Compounds			
4) T n-Dodecane (C12)	6.719	41995	0.309 ug/ml
6) T n-Tetradecane (C14)	8.555	40499	0.294 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012825AL\
Data File : FG015190.D
Signal(s) : FID1A.ch
Acq On : 28 Jan 2025 19:11
Operator : YP\AJ
Sample : Q1194-01D
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 02:36:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 011425.M
Quant Title : GC Extractables
QLast Update : Tue Jan 14 11:45:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

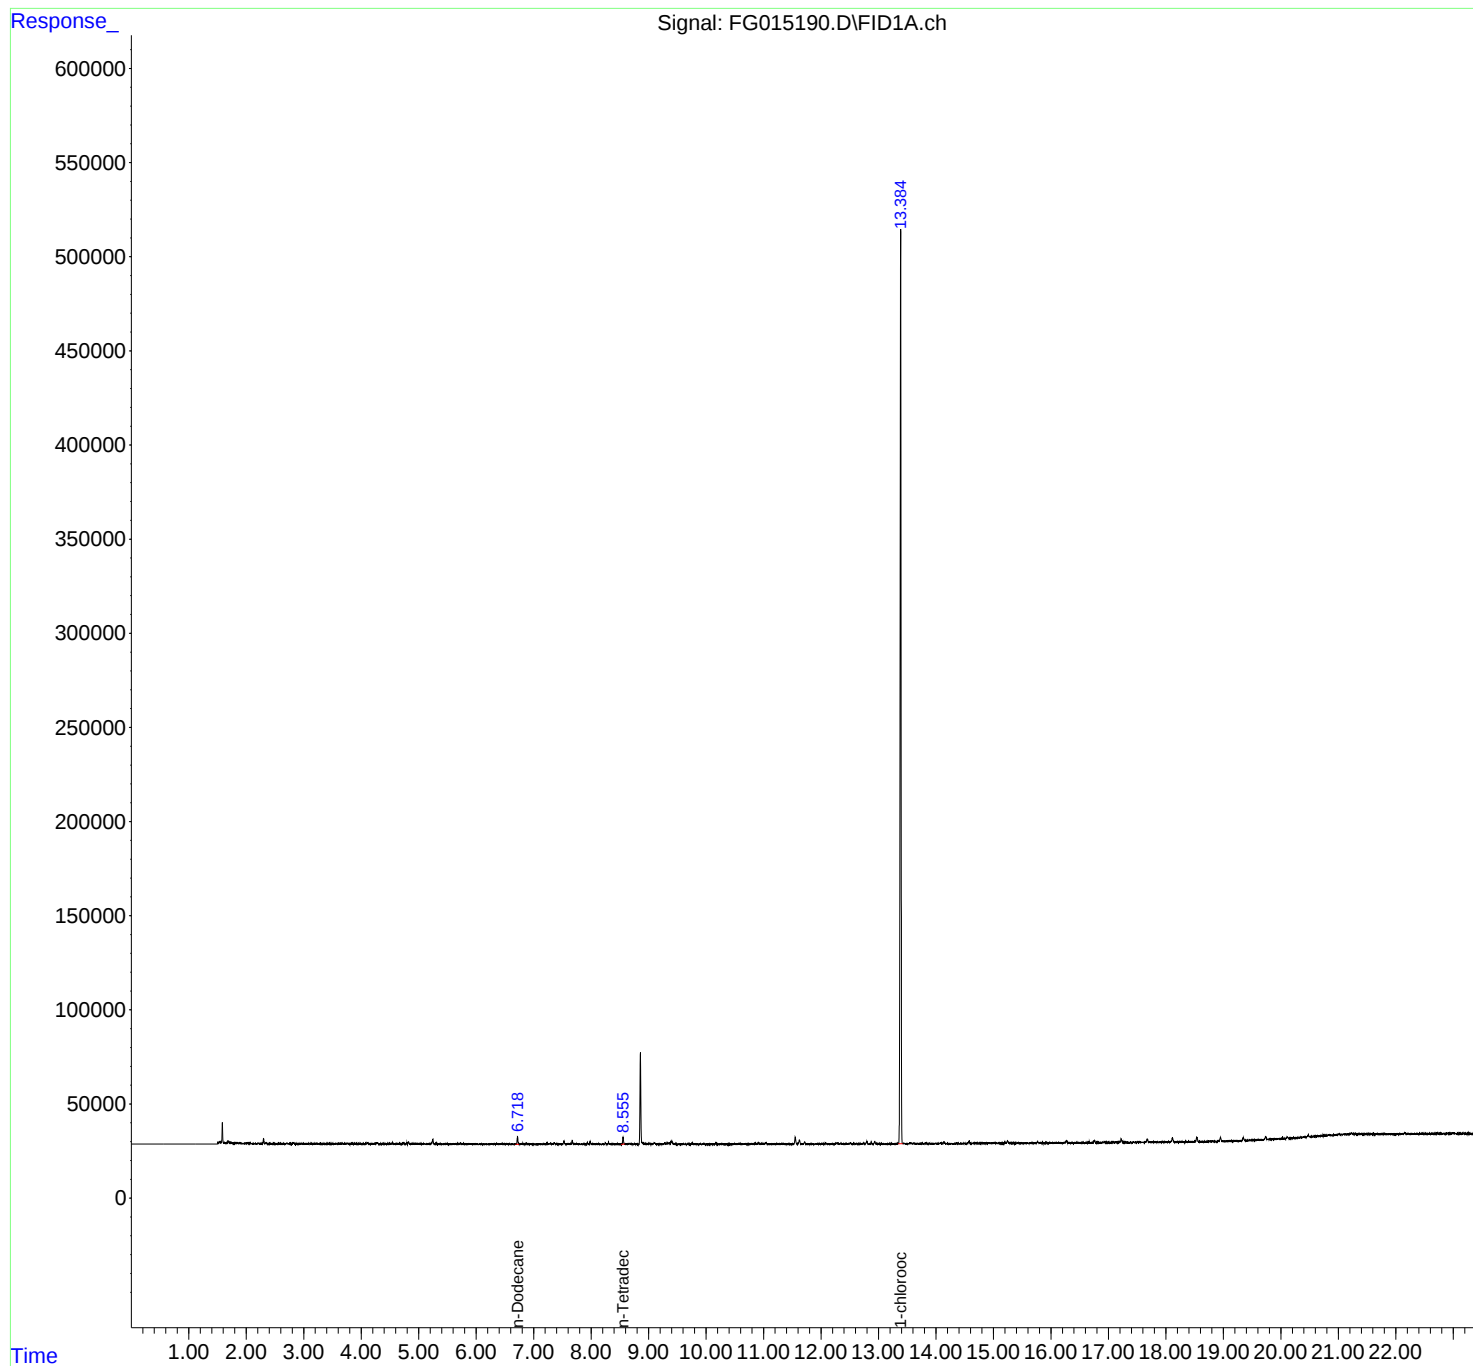


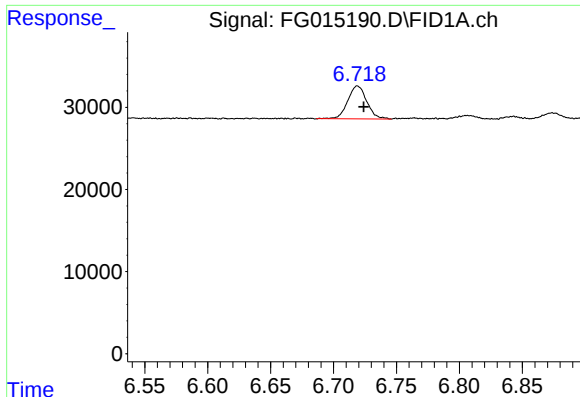

#4 n-Dodecane (C12)


R.T.: 6.719 min
Delta R.T.: -0.005 min
Response: 41995
Conc: 0.31 ug/ml

Instrument :
FID_G
ClientSampleId :

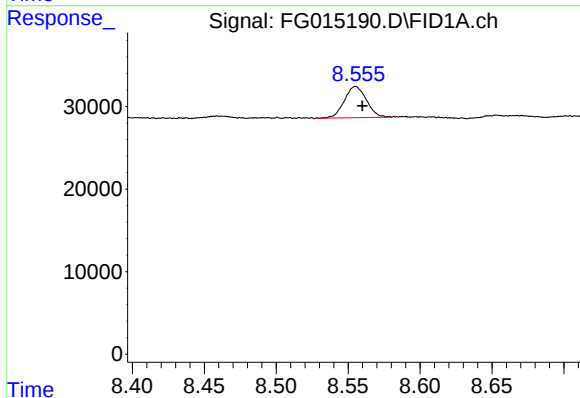


#6 n-Tetradecane (C14)

R.T.: 8.555 min
Delta R.T.: -0.005 min
Response: 40499
Conc: 0.29 ug/ml

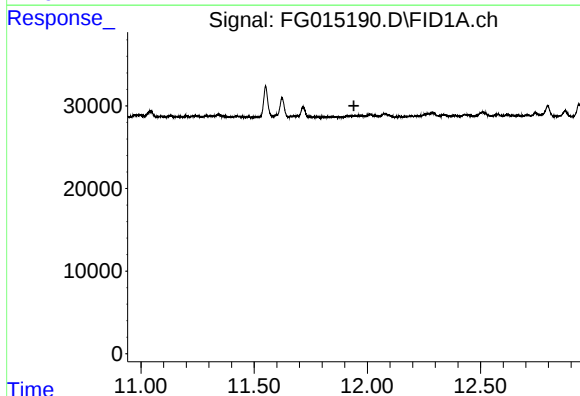

#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.940 min
Response: 0
Conc: N.D.

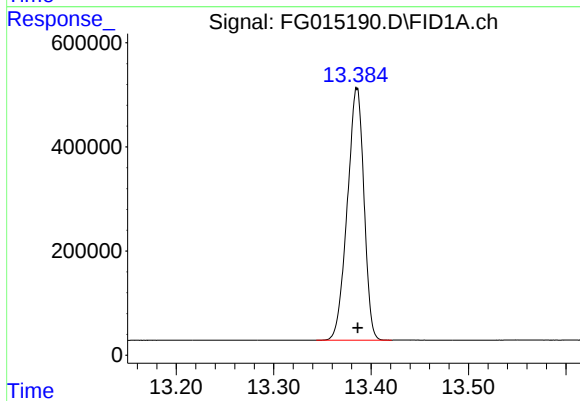

#12 1-chlorooctadecane (SURRE)

R.T.: 13.385 min
Delta R.T.: -0.001 min
Response: 5747946
Conc: 47.21 ug/ml