

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012921\
 Data File : FG007605.D
 Signal(s) : FID1A.ch
 Acq On : 29 Jan 2021 13:28
 Operator : DD\AJ
 Sample : M1262-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 22:15:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
 Quant Title :
 QLast Update : Tue Jan 05 02:18:25 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.637	2484189	20.729 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.222	174068	1.148 ug/ml
10)	N-TETRACOSANE	14.797f	282635	2.066 ug/ml
13)	N-TRIACONTANE	17.712	159021	1.293 ug/ml
14)	N-DOTRIACONTANE	18.539	187280	1.653 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012921\
Data File : FG007605.D
Signal(s) : FID1A.ch
Acq On : 29 Jan 2021 13:28
Operator : DD\AJ
Sample : M1262-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 22:15:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010421.M
Quant Title :
QLast Update : Tue Jan 05 02:18:25 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

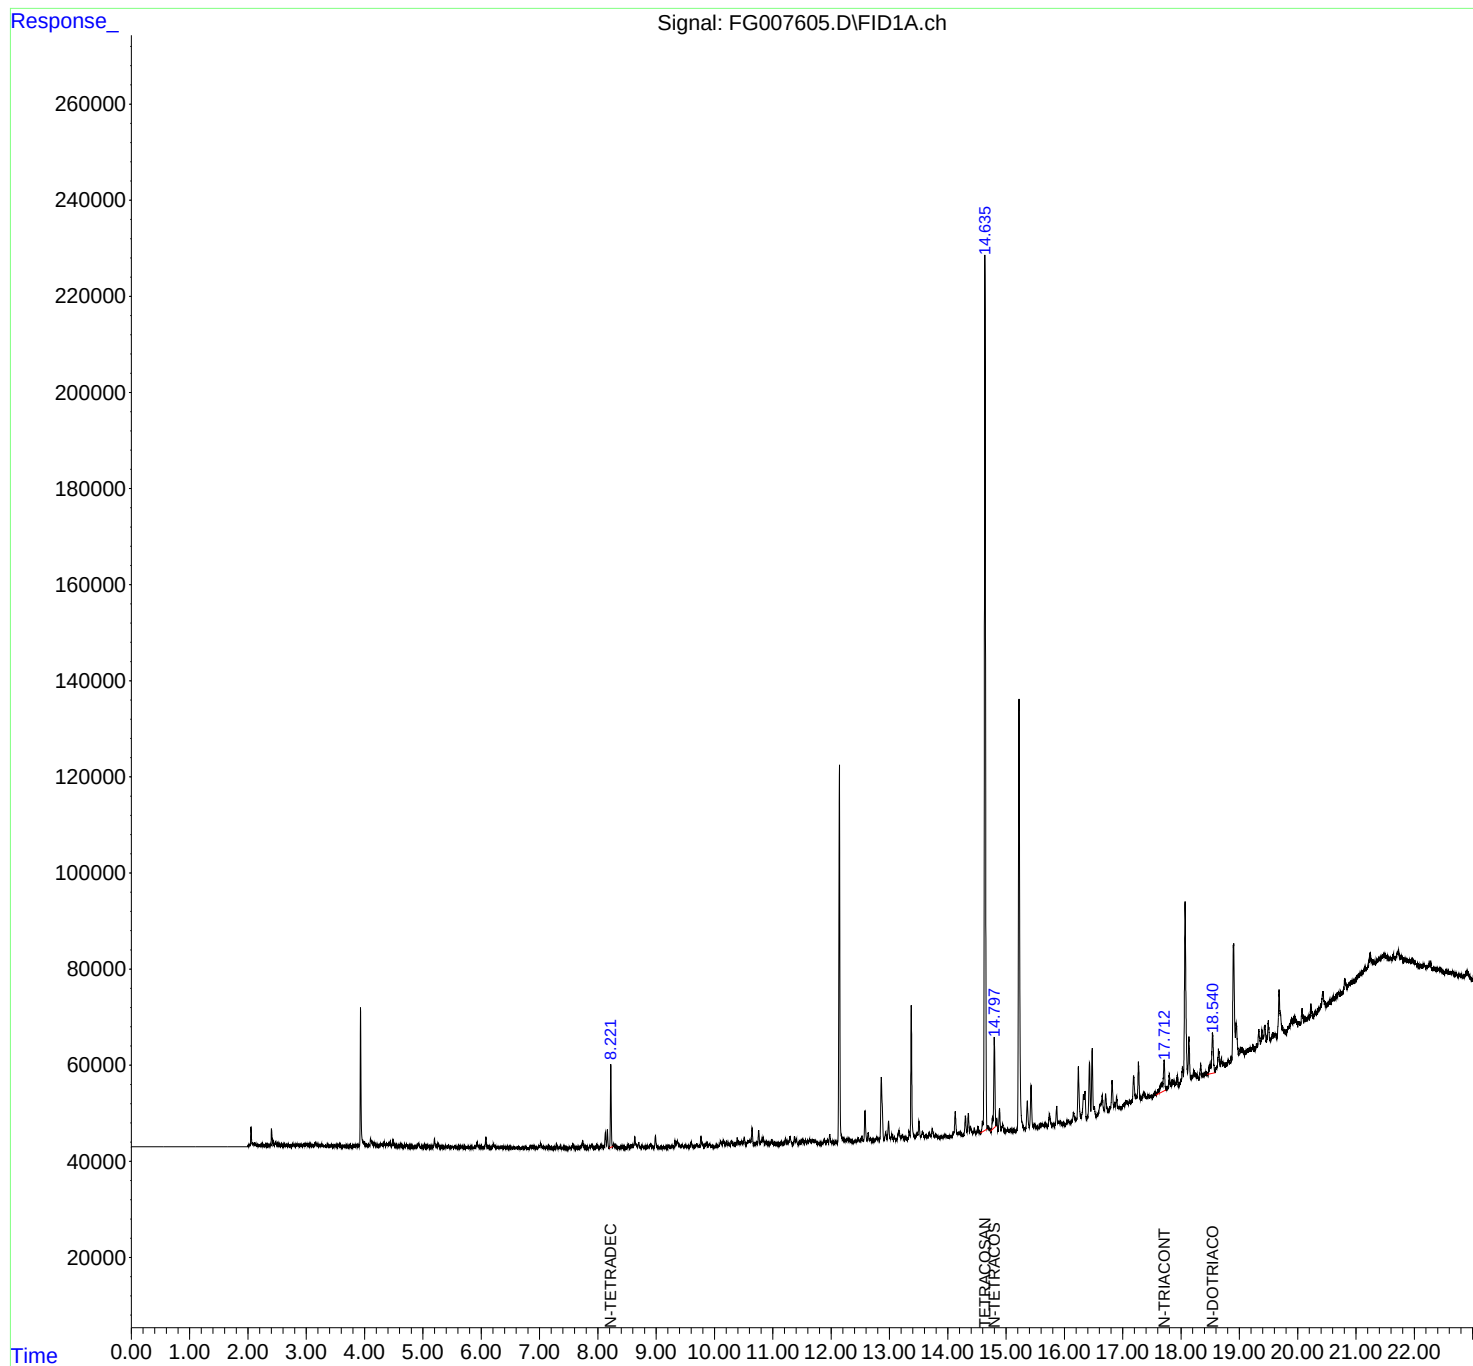


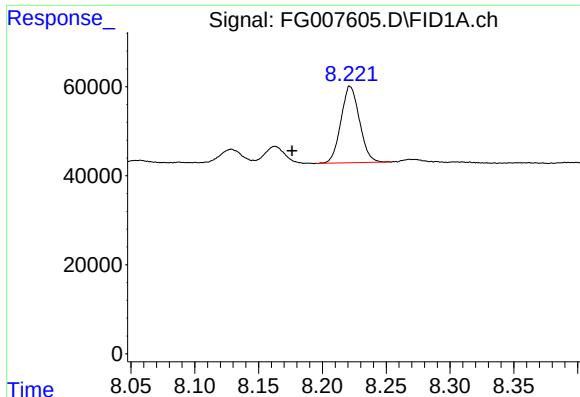

#4 N-TETRADECANE


R.T.: 8.222 min
Delta R.T.: 0.046 min
Response: 174068
Conc: 1.15 ug/ml

Instrument :
FID_G
ClientSampleId :

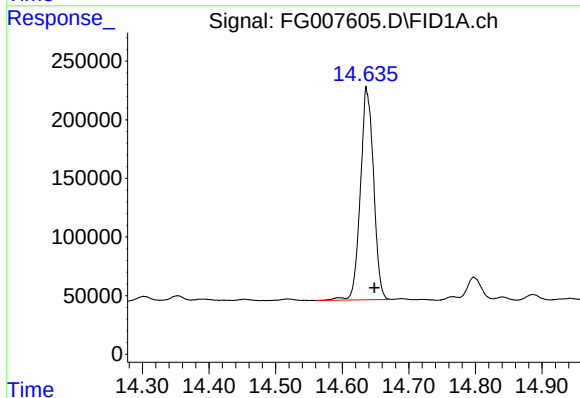


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: -0.012 min
Response: 2484189
Conc: 20.73 ug/ml

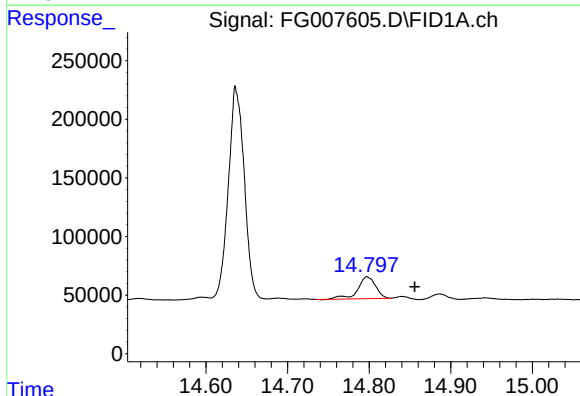


#10 N-TETRACOSANE

R.T.: 14.797 min
Delta R.T.: -0.058 min
Response: 282635
Conc: 2.07 ug/ml

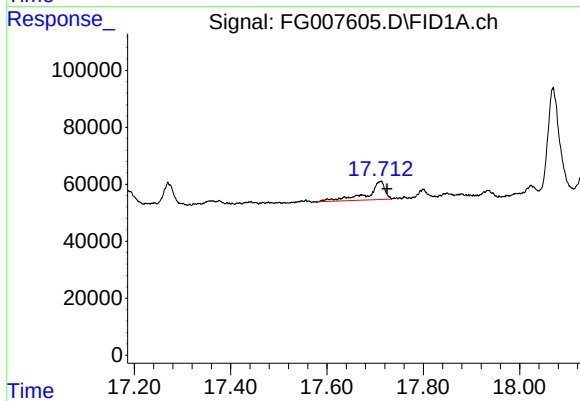

#13 N-TRIACONTANE

R.T.: 17.712 min
Delta R.T.: -0.013 min
Response: 159021
Conc: 1.29 ug/ml

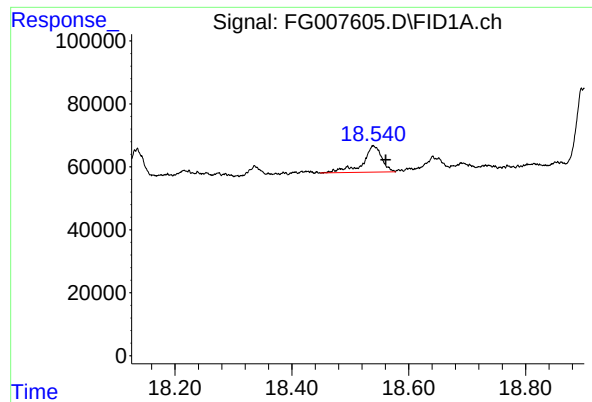

#14 N-DOTRIACONTANE

R.T.: 18.539 min
Delta R.T.: -0.022 min
Response: 187280
Conc: 1.65 ug/ml

Instrument :
FID_G
ClientSampleId :