

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG012924\  
 Data File : FG013382.D  
 Signal(s) : FID1A.ch  
 Acq On : 29 Jan 2024 14:52  
 Operator : YP\AJ  
 Sample : P1271-01  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :  
 SB-03-20231213-6.0-7.0

Manual Integrations  
 APPROVED

Reviewed By :Ankita Jodhani 01/30/2024  
 Supervised By :Sohil Jodhani 01/30/2024

Integration File: autoint1.e  
 Quant Time: Jan 30 00:48:13 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG010824.M  
 Quant Title :  
 QLast Update : Mon Jan 08 14:52:14 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 15.071 | 1681870  | 13.755 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG012924\  
Data File : FG013382.D  
Signal(s) : FID1A.ch  
Acq On : 29 Jan 2024 14:52  
Operator : YP\AJ  
Sample : P1271-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
SB-03-20231213-6.0-7.0


Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 01/30/2024  
Supervised By :Sohil Jodhani 01/30/2024

Integration File: autoint1.e  
Quant Time: Jan 30 00:48:13 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG010824.M  
Quant Title :  
QLast Update : Mon Jan 08 14:52:14 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

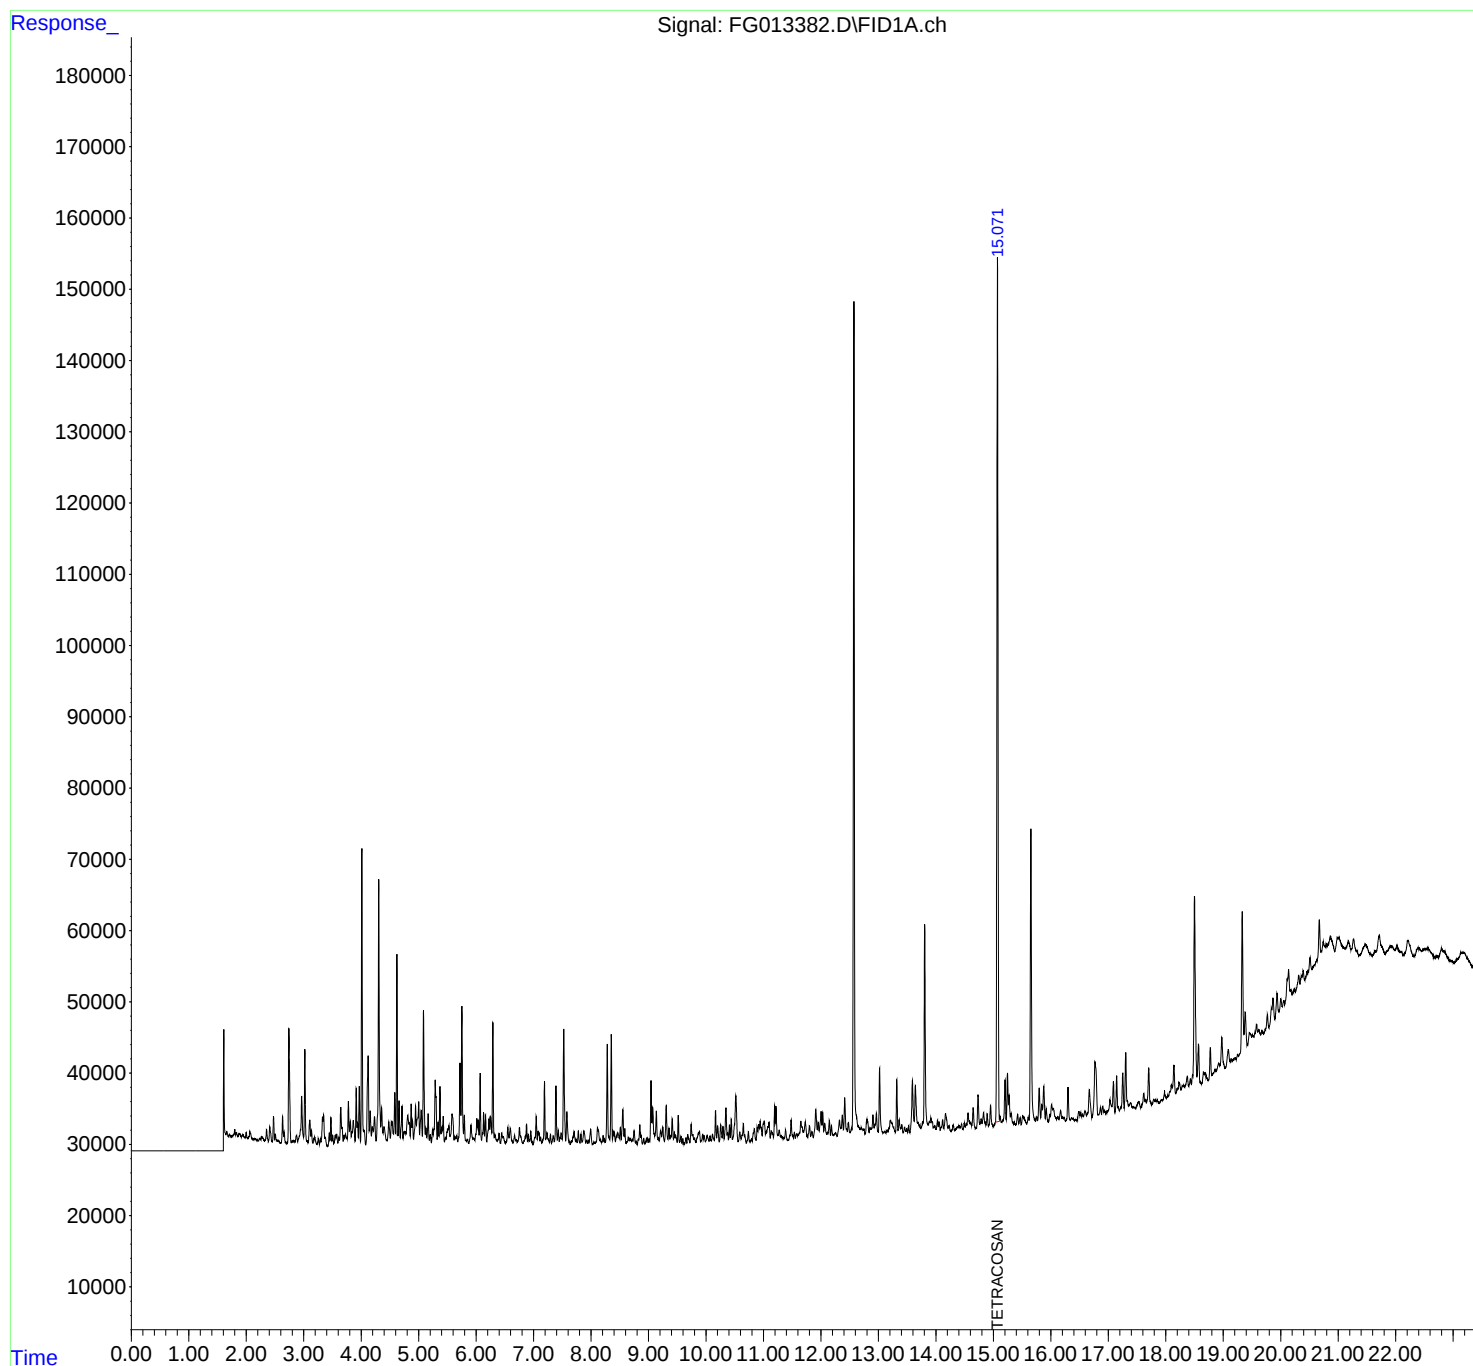

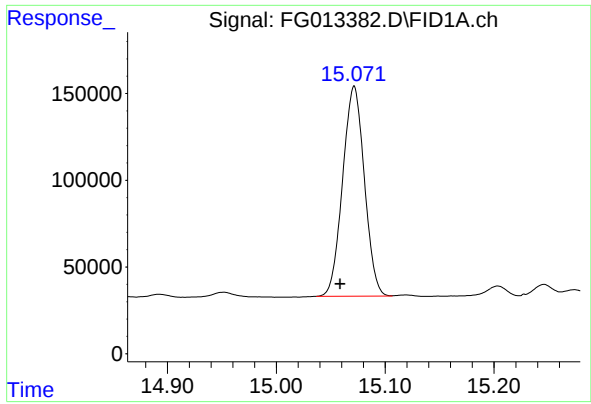

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.071 min  
Delta R.T.: 0.013 min  
Response: 1681870  
Conc: 13.76 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
SB-03-20231213-6.0-7.0

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 01/30/2024  
Supervised By :Sohil Jodhani 01/30/2024