

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG020224\  
Data File : FG013432.D  
Signal(s) : FID1A.ch  
Acq On : 02 Feb 2024 16:48  
Operator : YP\AJ  
Sample : P1304-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
BRIGHTON-WEST-8TH-STREET

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 02/05/2024  
Supervised By :Sohil Jodhani 02/05/2024

Integration File: autoint1.e  
Quant Time: Feb 05 05:04:27 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG020124.M  
Quant Title :  
QLast Update : Thu Feb 01 14:07:32 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 15.071 | 3518224  | 31.425 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG020224\  
Data File : FG013432.D  
Signal(s) : FID1A.ch  
Acq On : 02 Feb 2024 16:48  
Operator : YP\AJ  
Sample : P1304-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
BRIGHTON-WEST-8TH-STREET


Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 02/05/2024  
Supervised By :Sohil Jodhani 02/05/2024

Integration File: autoint1.e  
Quant Time: Feb 05 05:04:27 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG020124.M  
Quant Title :  
QLast Update : Thu Feb 01 14:07:32 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

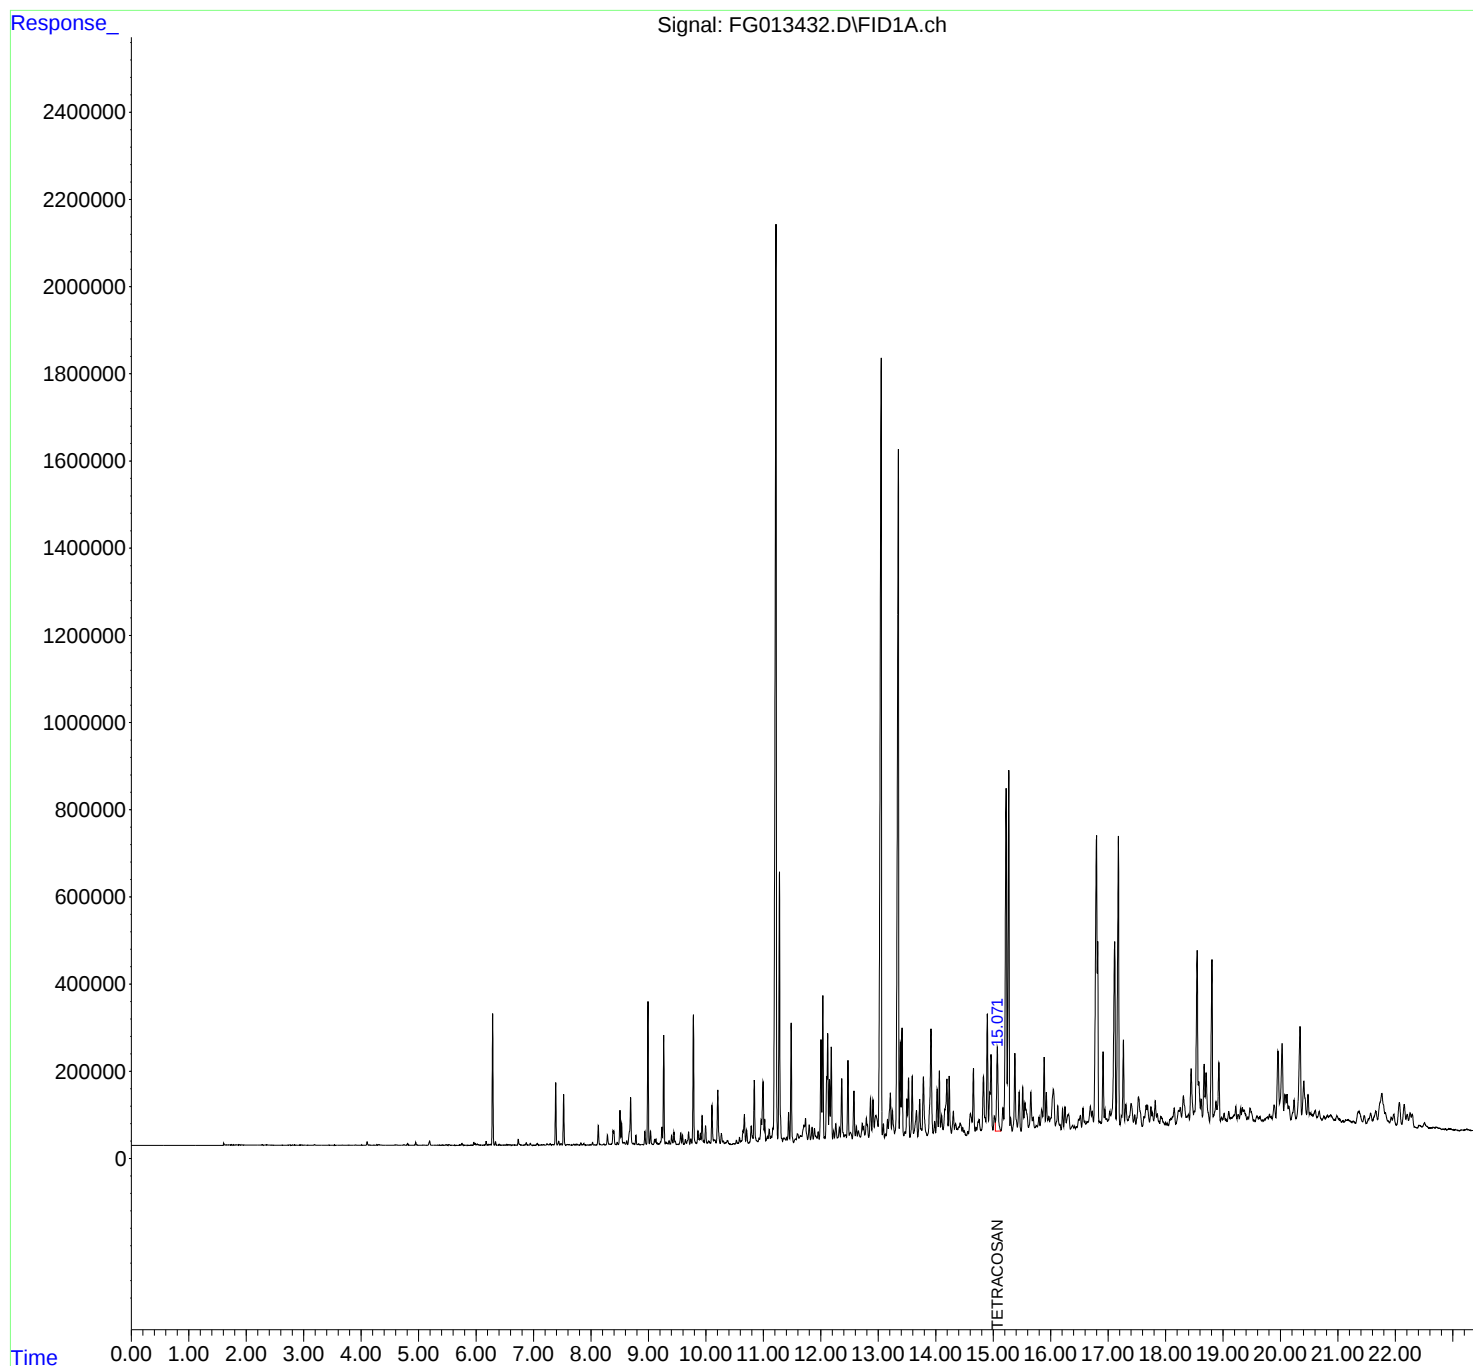

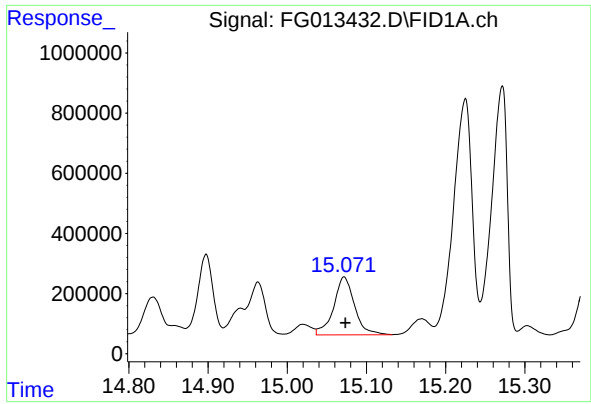

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.071 min  
Delta R.T.: -0.002 min  
Response: 3518224  
Conc: 31.42 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
BRIGHTON-WEST-8TH-STREET

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 02/05/2024  
Supervised By :Sohil Jodhani 02/05/2024