

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020323\
Data File : FG011361.D
Signal(s) : FID1A.ch
Acq On : 03 Feb 2023 07:38
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 00:19:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.998	168108	1.209 ug/ml
16) N-HEXATRIACONTANE	20.552	111820	0.964 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020323\
Data File : FG011361.D
Signal(s) : FID1A.ch
Acq On : 03 Feb 2023 07:38
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 00:19:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

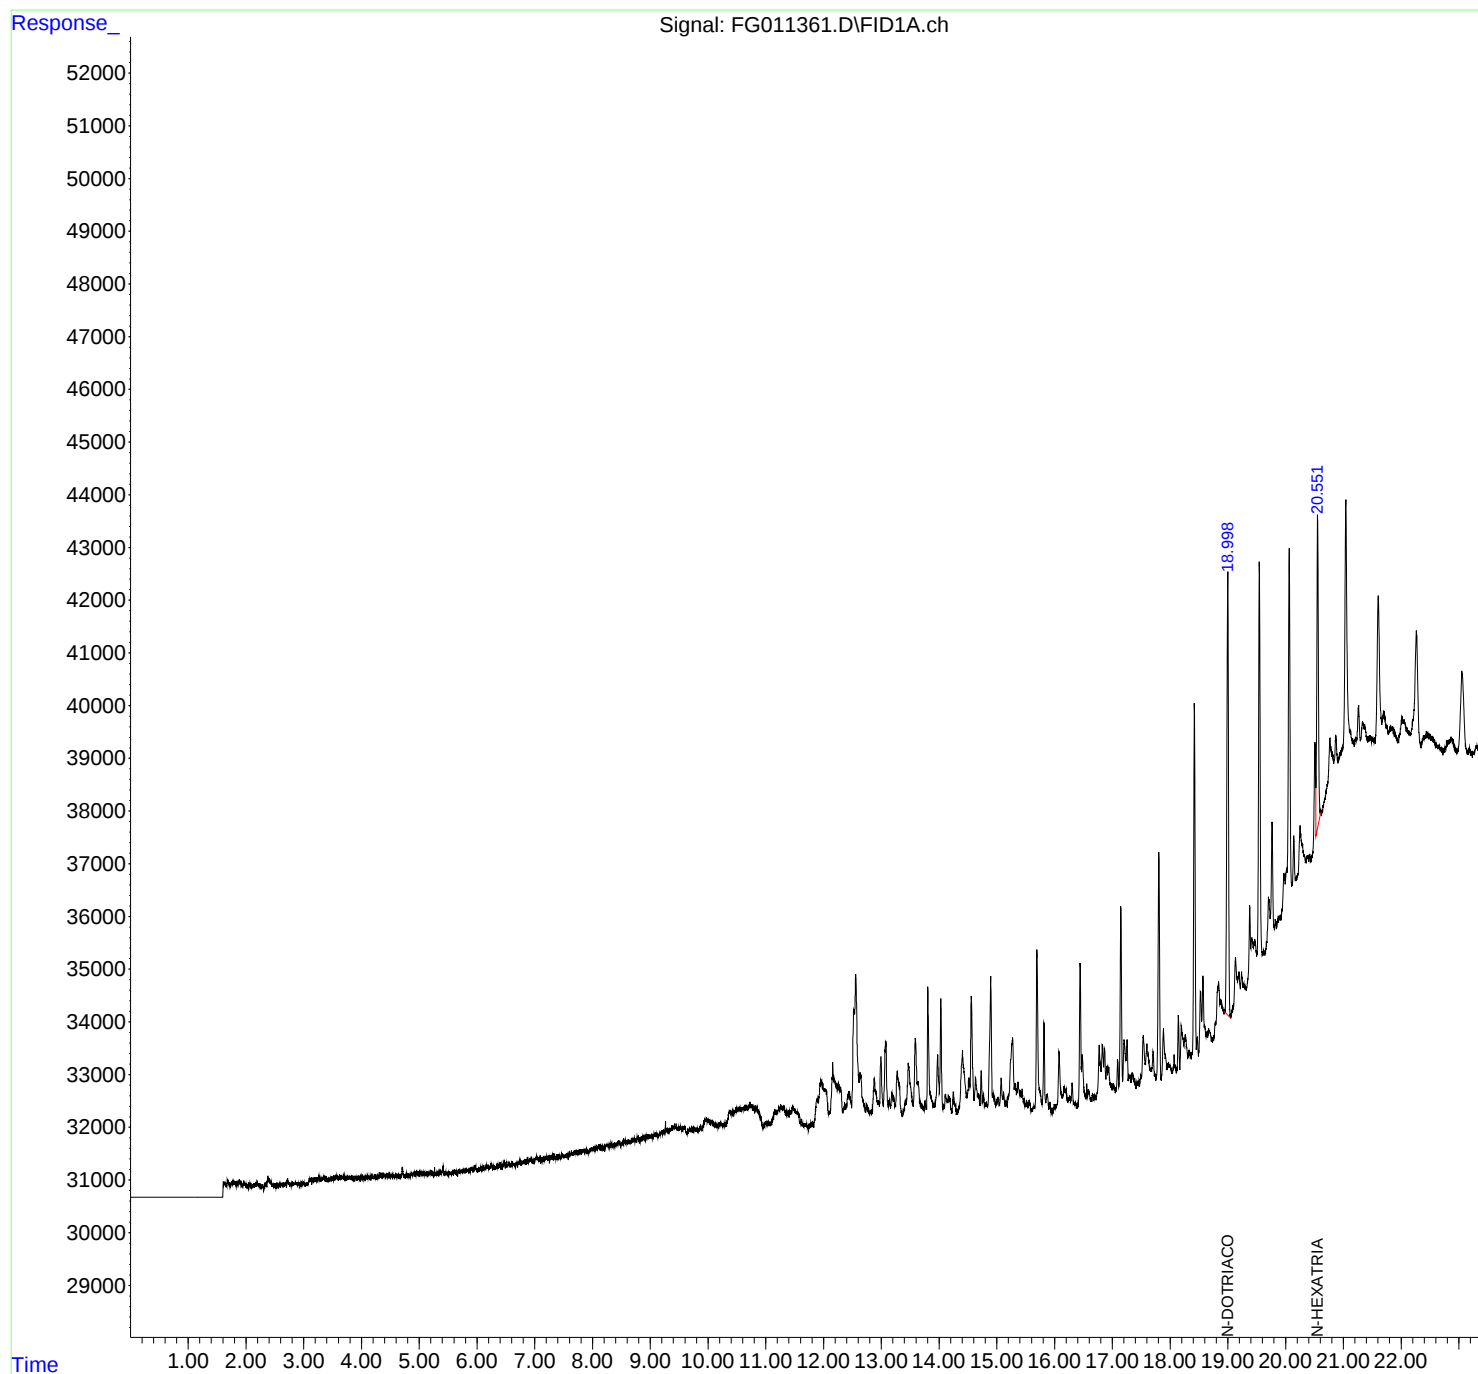


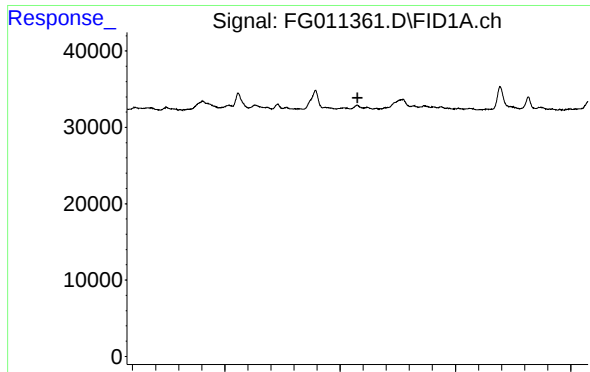

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

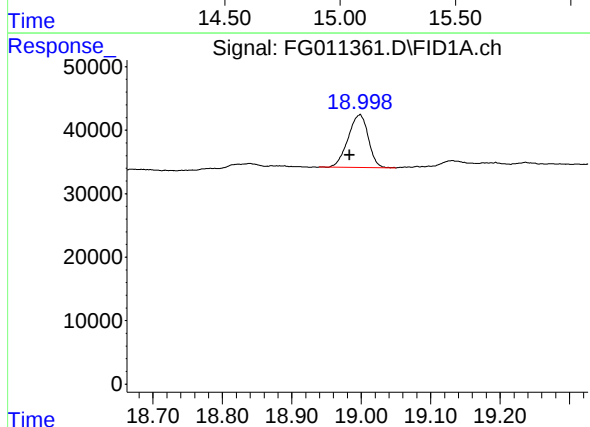

#14 N-DOTRIACONTANE

R.T.: 18.998 min
Delta R.T.: 0.015 min
Response: 168108
Conc: 1.21 ug/ml

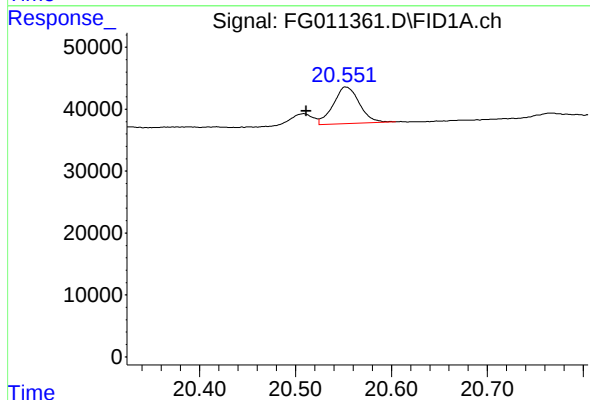

#16 N-HEXATRIACONTANE

R.T.: 20.552 min
Delta R.T.: 0.041 min
Response: 111820
Conc: 0.96 ug/ml