

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020323\
 Data File : FG011373.D
 Signal(s) : FID1A.ch
 Acq On : 03 Feb 2023 21:17
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 04 00:21:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
 Quant Title :
 QLast Update : Mon Jan 30 21:53:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.072	2059947	15.607 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.979	42086	0.303 ug/ml
16) N-HEXATRIACONTANE	20.508	80983	0.698 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020323\
Data File : FG011373.D
Signal(s) : FID1A.ch
Acq On : 03 Feb 2023 21:17
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 00:21:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

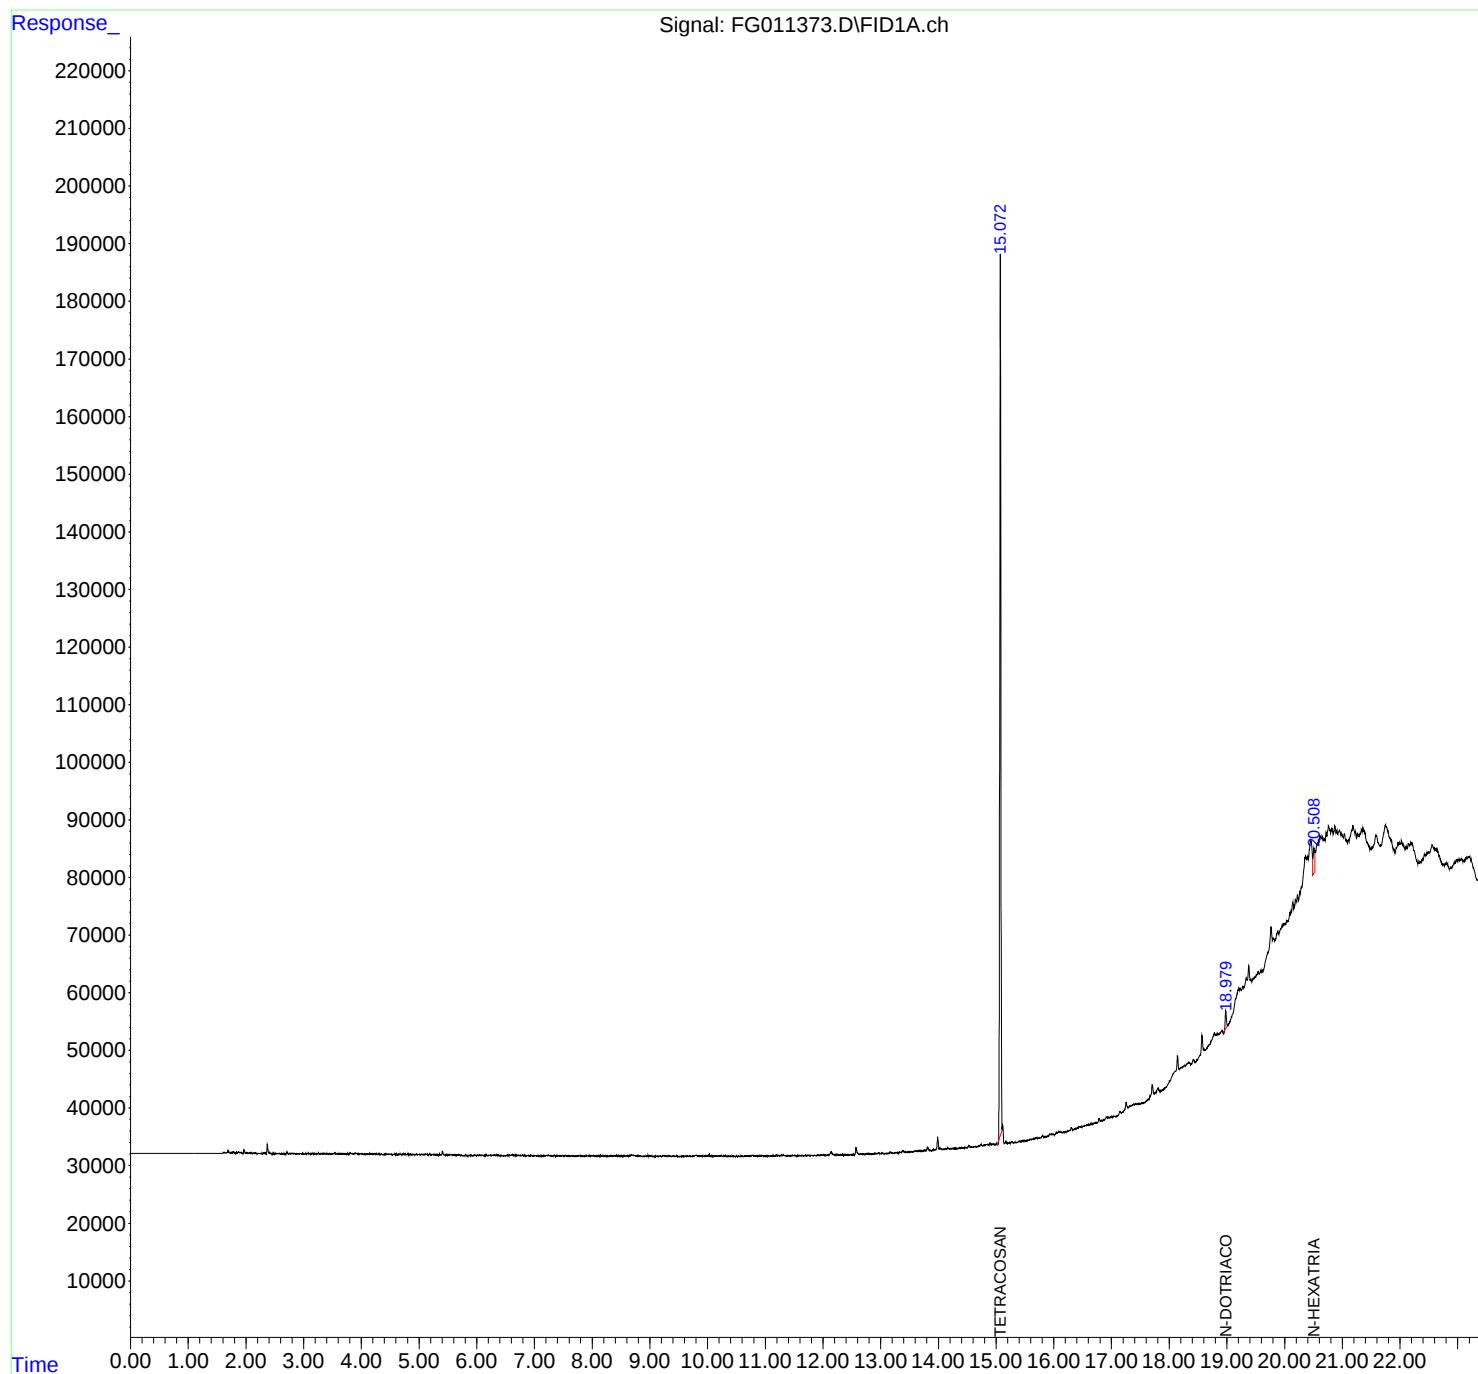

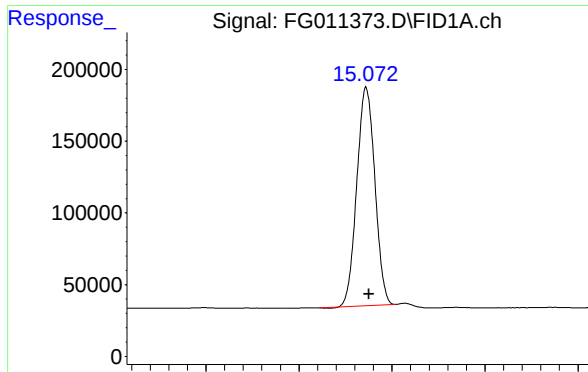


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.072 min
Delta R.T.: -0.003 min
Response: 2059947
Conc: 15.61 ug/ml

Instrument :


FID_G

ClientSampleId :

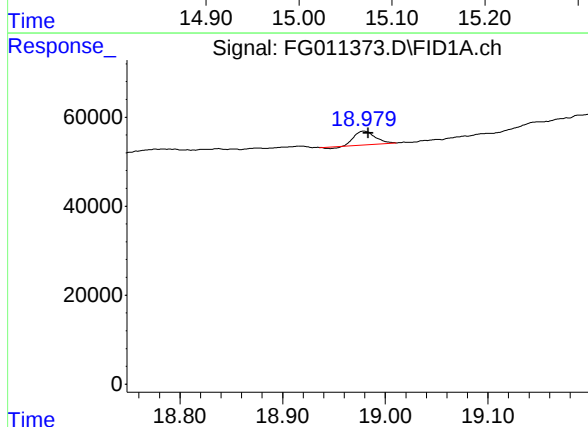

#14 N-DOTRIACONTANE

R.T.: 18.979 min
Delta R.T.: -0.004 min
Response: 42086
Conc: 0.30 ug/ml

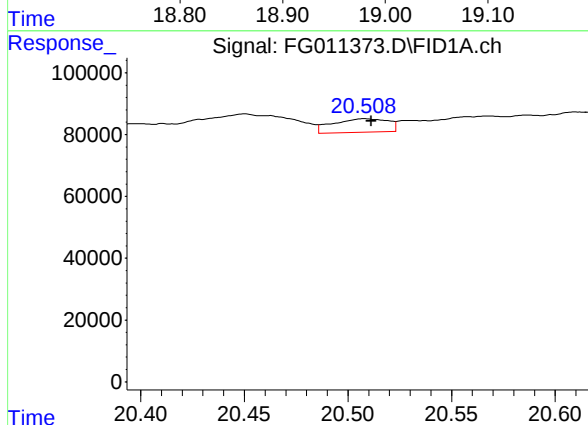

#16 N-HEXATRIACONTANE

R.T.: 20.508 min
Delta R.T.: -0.003 min
Response: 80983
Conc: 0.70 ug/ml