

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020323\
Data File : FG011366.D
Signal(s) : FID1A.ch
Acq On : 03 Feb 2023 16:52
Operator : YP\AJ
Sample : PB150674BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB150674BL

Integration File: autoint1.e
Quant Time: Feb 04 00:19:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.070	2228806	16.887 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020323\
Data File : FG011366.D
Signal(s) : FID1A.ch
Acq On : 03 Feb 2023 16:52
Operator : YP\AJ
Sample : PB150674BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB150674BL

Integration File: autoint1.e
Quant Time: Feb 04 00:19:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

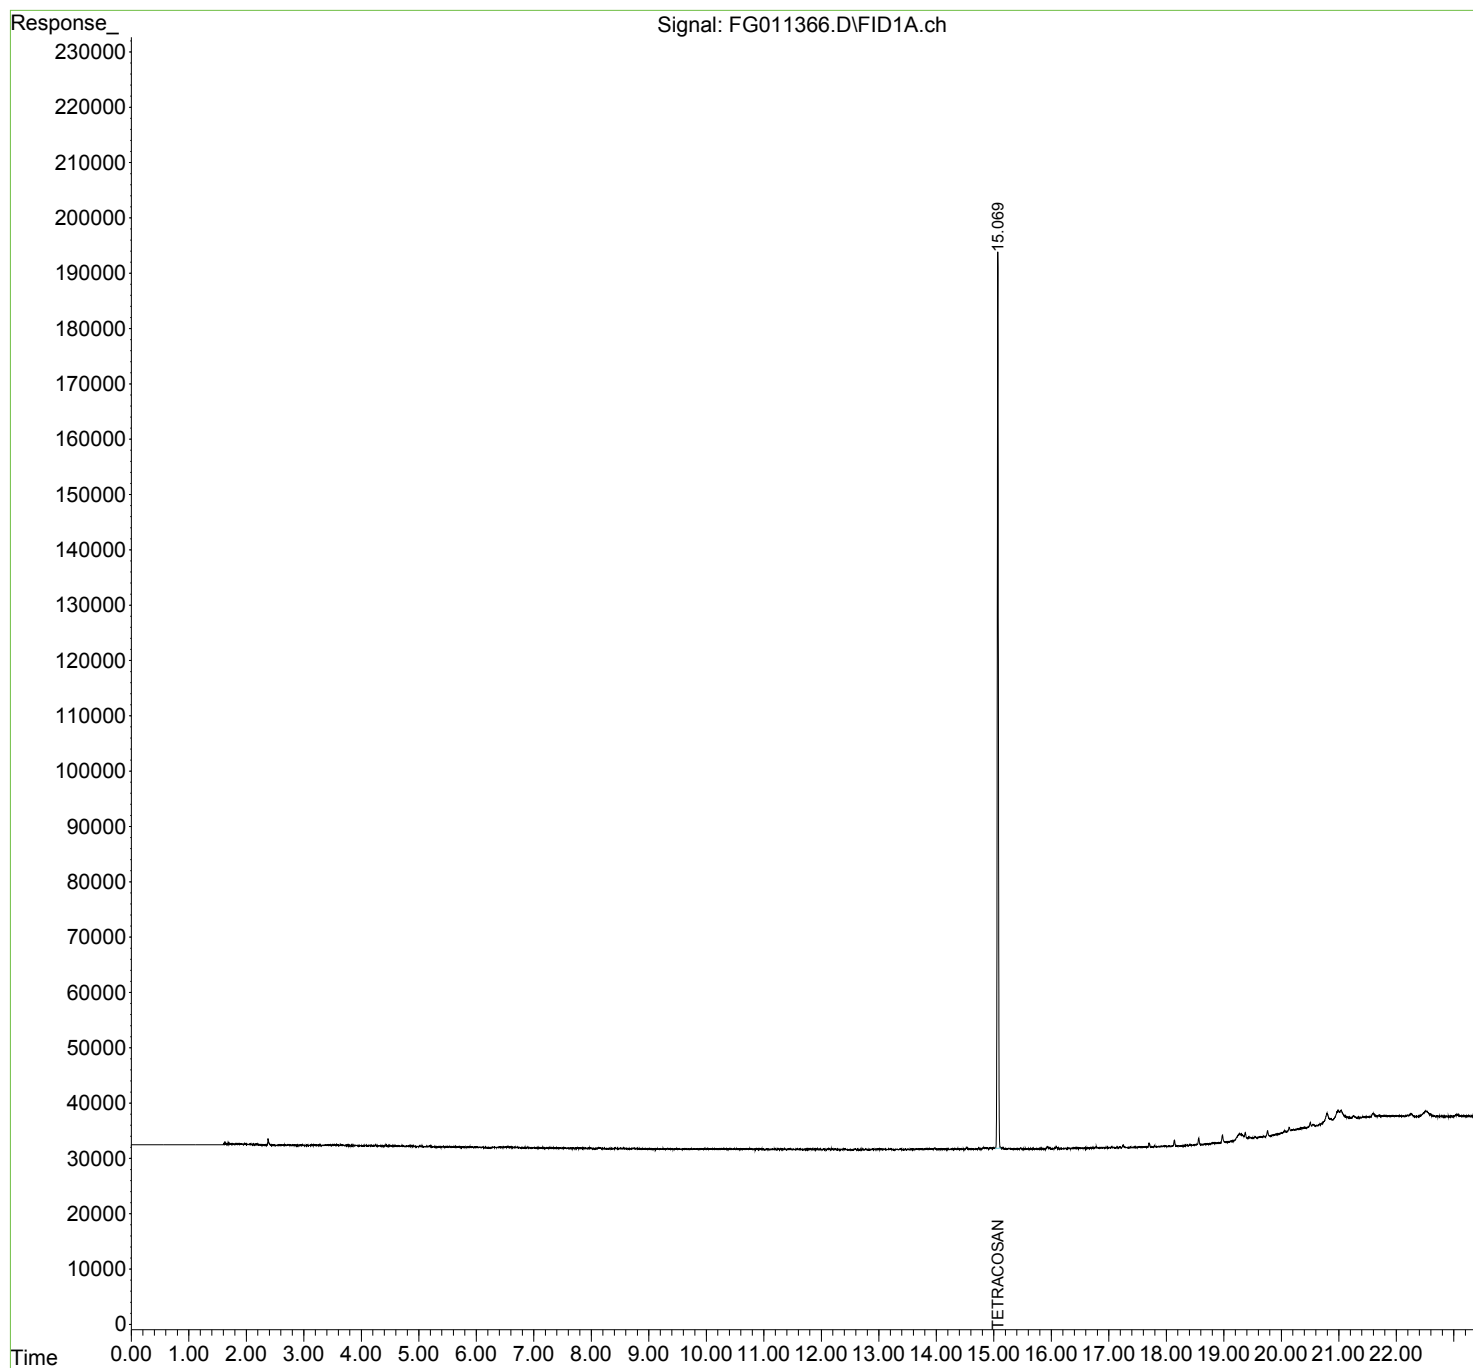

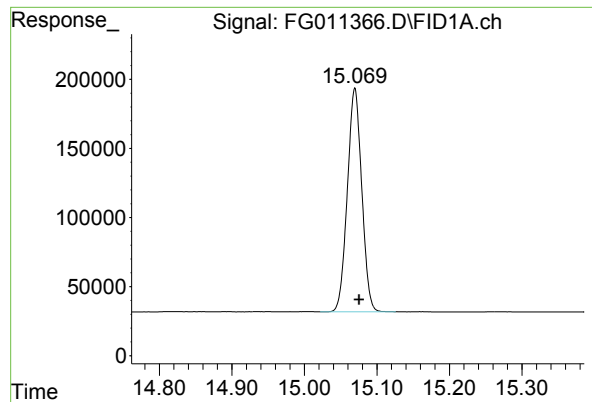

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.070 min
Delta R.T.: -0.006 min
Response: 2228806
Conc: 16.89 ug/ml

Instrument :
FID_G
ClientSampleId :
PB150674BL