

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020519\
 Data File : FG003664.D
 Signal(s) : FID1A.ch
 Acq On : 05 Feb 2019 14:47
 Operator : AJ\SJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 06 08:42:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:41:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.472	6209305	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.111	7326374	50.000 ug/ml
2) N-DECANE	4.196	7435506	50.000 ug/ml
3) N-DODECANE	6.221	7432944	50.000 ug/ml
4) N-TETRADECANE	8.016	7407439	50.000 ug/ml
5) N-HEXADECANE	9.618	7408169	50.000 ug/ml
6) N-OCTADECANE	11.062	7397386	50.000 ug/ml
7) N-EICOSANE	12.373	7272113	50.000 ug/ml
8) N-DOCOSANE	13.572	7109978	50.000 ug/ml
10) N-TETRACOSANE	14.678	6915540	50.000 ug/ml
11) N-HEXACOSANE	15.700	6737831	50.000 ug/ml
12) N-OCTACOSANE	16.651	6554433	50.000 ug/ml
13) N-TRIACONTANE	17.540	6340646	50.000 ug/ml
14) N-DOTRIACONTANE	18.375	5837441	50.000 ug/ml
15) N-TETRATRIACONTANE	19.159	5393132	50.000 ug/ml
16) N-HEXATRIACONTANE	19.903	4982440	50.000 ug/ml
17) N-OCTATRIACONTANE	20.619	4630537	50.000 ug/ml
18) N-TETRACONTANE	21.470	4664277	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020519\
Data File : FG003664.D
Signal(s) : FID1A.ch
Acq On : 05 Feb 2019 14:47
Operator : AJ\SJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 06 08:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:41:02 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

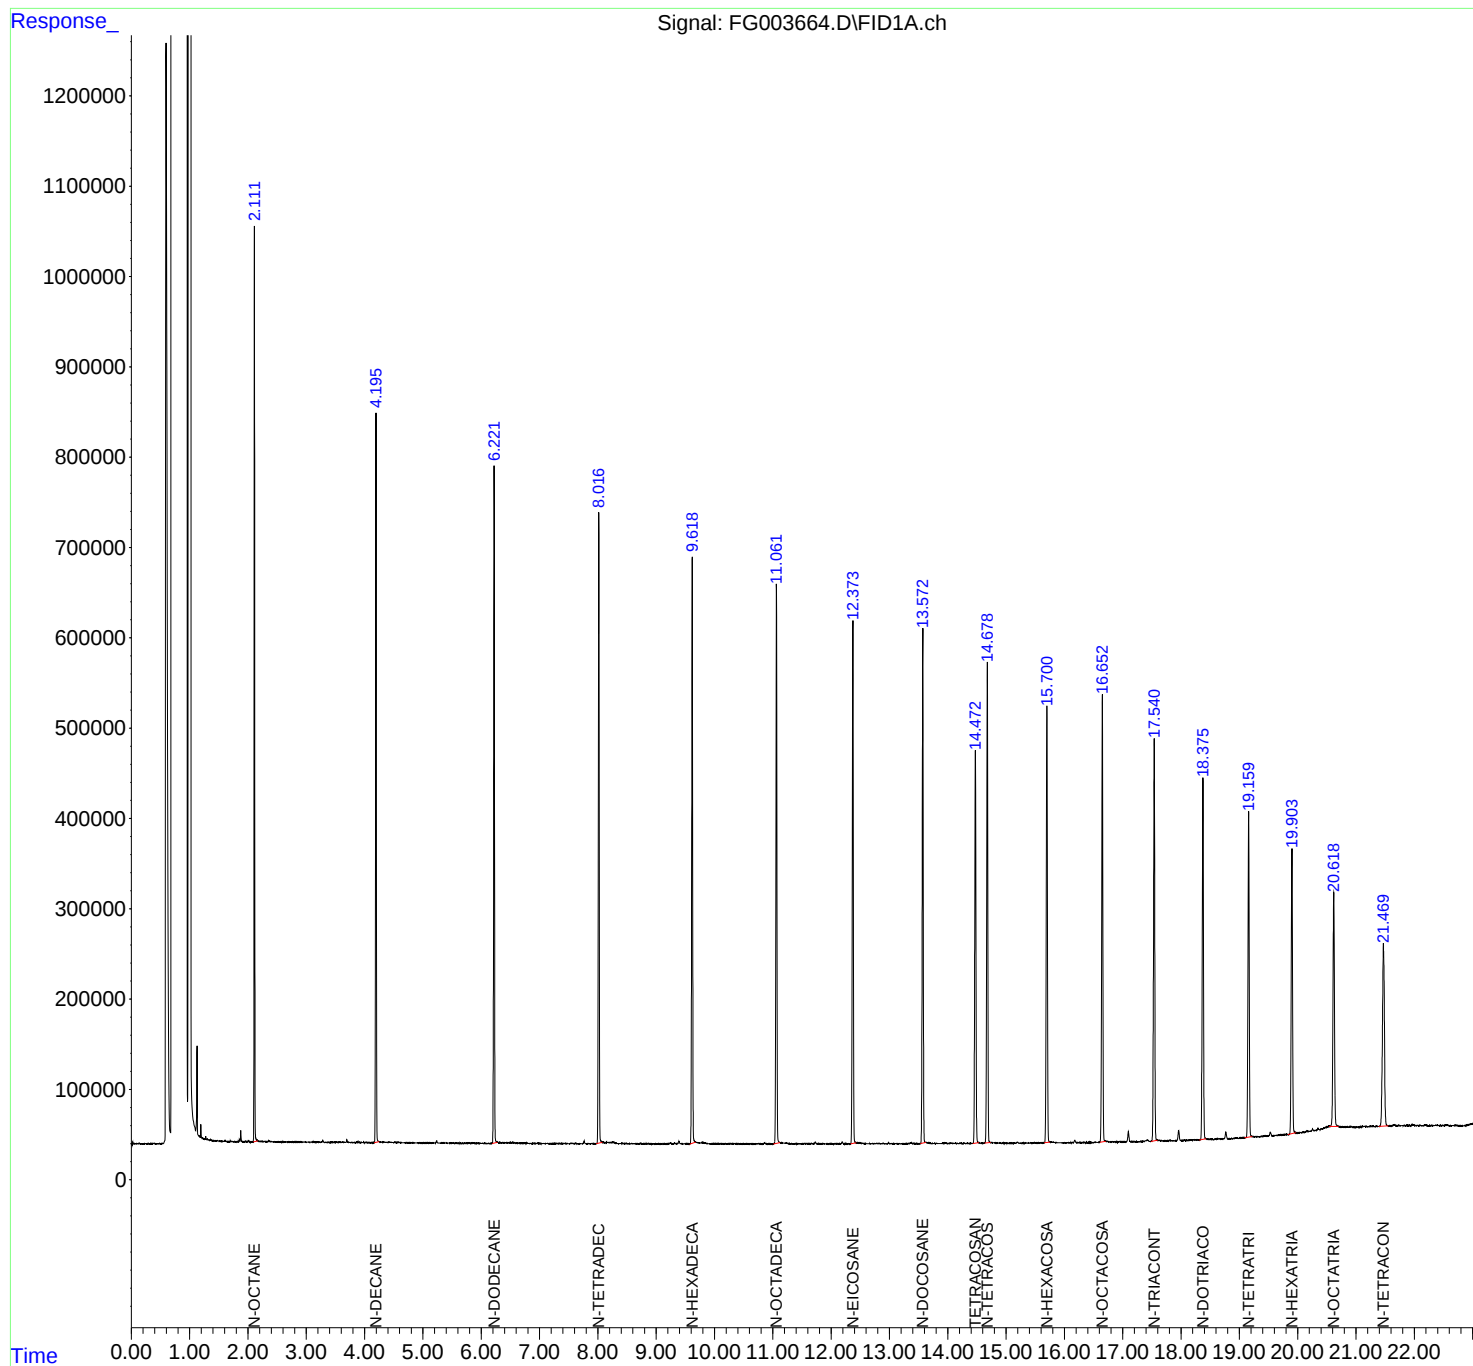

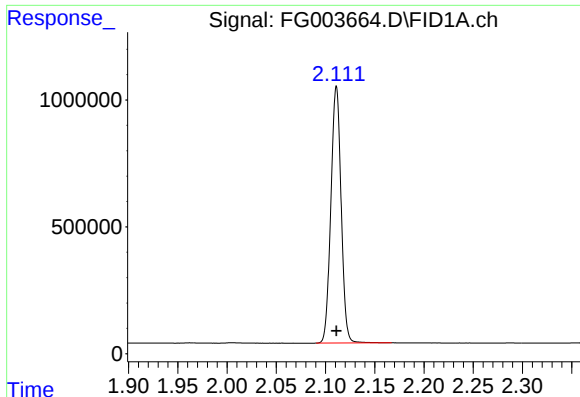


#1 N-OCTANE

R.T.: 2.111 min
Delta R.T.: 0.000 min
Response: 7326374
Conc: 50.00 ug/ml

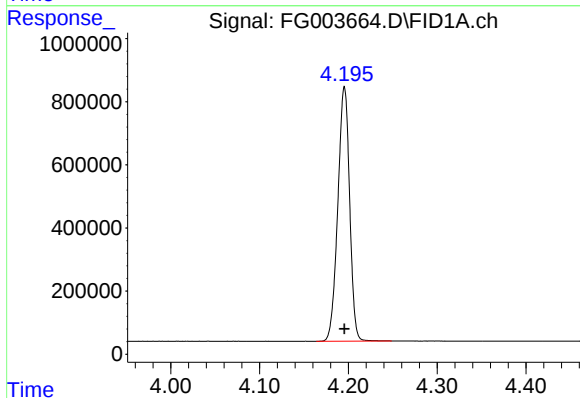


#2 N-DECANE

R.T.: 4.196 min
Delta R.T.: 0.000 min
Response: 7435506
Conc: 50.00 ug/ml

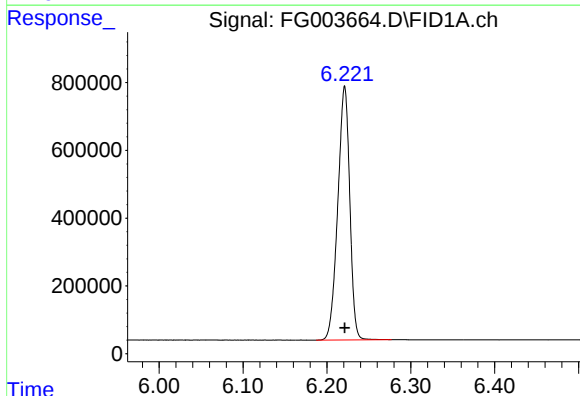


#3 N-DODECANE

R.T.: 6.221 min
Delta R.T.: 0.000 min
Response: 7432944
Conc: 50.00 ug/ml

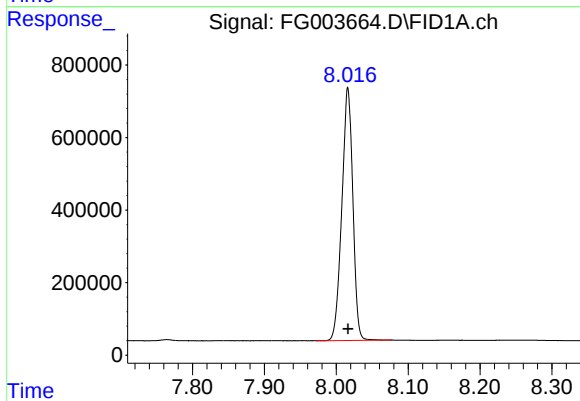


#4 N-TETRADECANE

R.T.: 8.016 min
Delta R.T.: 0.000 min
Response: 7407439
Conc: 50.00 ug/ml

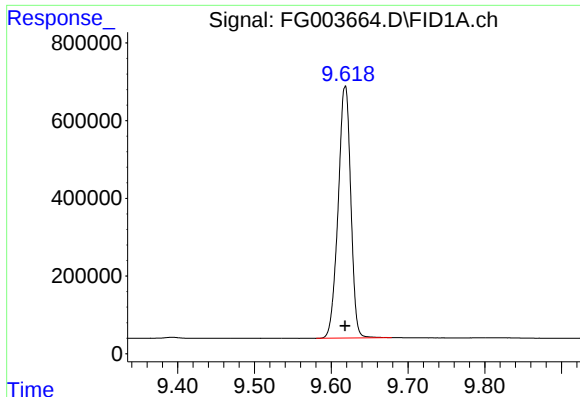


#5 N-HEXADECANE

R.T.: 9.618 min
Delta R.T.: 0.000 min
Response: 7408169
Conc: 50.00 ug/ml

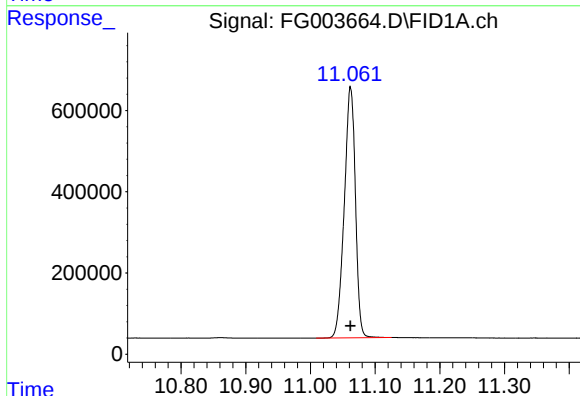


#6 N-OCTADECANE

R.T.: 11.062 min
Delta R.T.: 0.000 min
Response: 7397386
Conc: 50.00 ug/ml

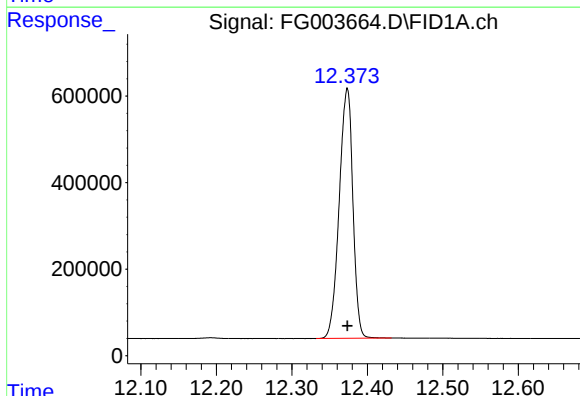


#7 N-EICOSANE

R.T.: 12.373 min
Delta R.T.: 0.000 min
Response: 7272113
Conc: 50.00 ug/ml

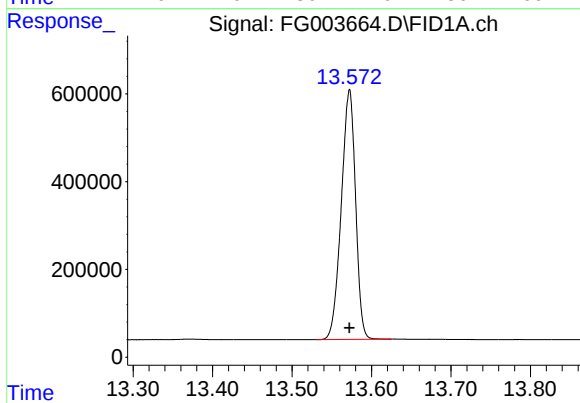


#8 N-DOCOSANE

R.T.: 13.572 min
Delta R.T.: 0.000 min
Response: 7109978
Conc: 50.00 ug/ml

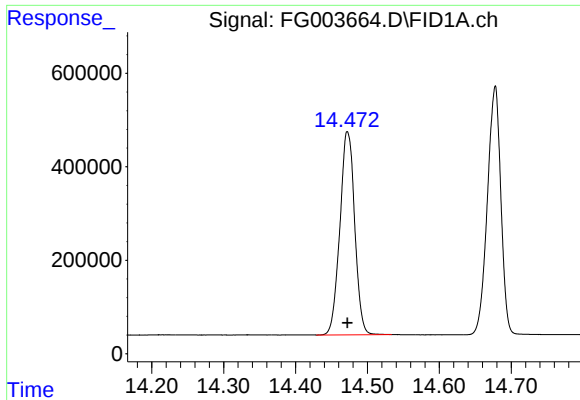


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.472 min
Delta R.T.: 0.000 min
Response: 6209305
Conc: 50.00 ug/ml

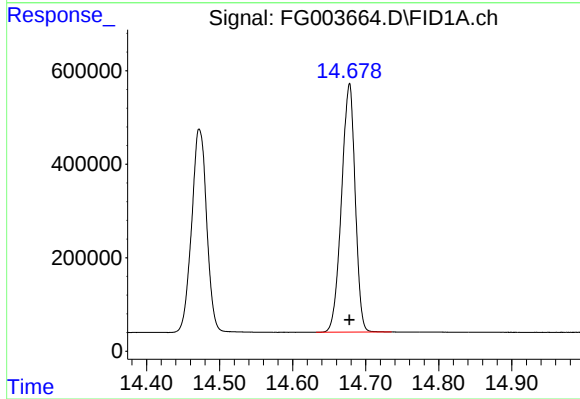


#10 N-TETRACOSANE

R.T.: 14.678 min
Delta R.T.: 0.000 min
Response: 6915540
Conc: 50.00 ug/ml

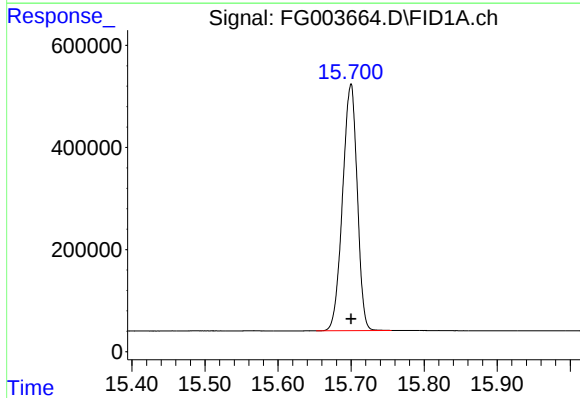


#11 N-HEXACOSANE

R.T.: 15.700 min
Delta R.T.: 0.000 min
Response: 6737831
Conc: 50.00 ug/ml

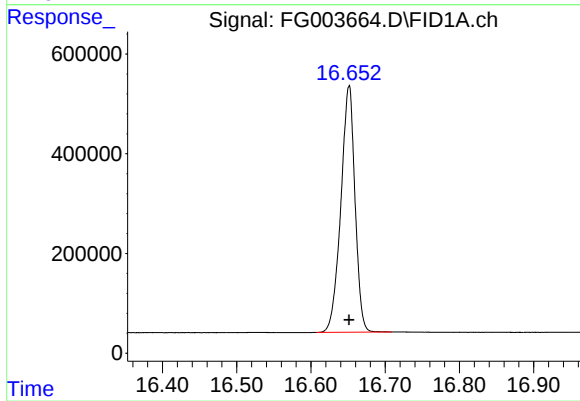


#12 N-OCTACOSANE

R.T.: 16.651 min
Delta R.T.: 0.000 min
Response: 6554433
Conc: 50.00 ug/ml

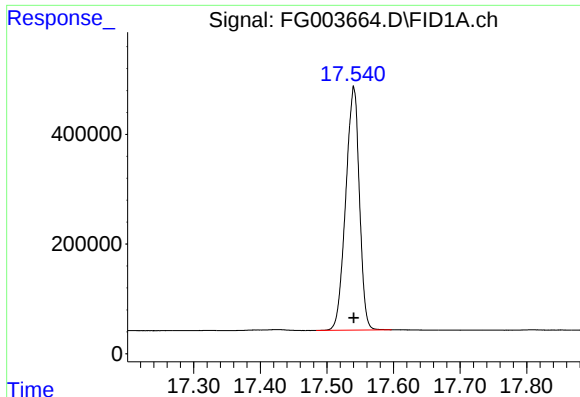


#13 N-TRIACONTANE

R.T.: 17.540 min
Delta R.T.: 0.000 min
Response: 6340646
Conc: 50.00 ug/ml

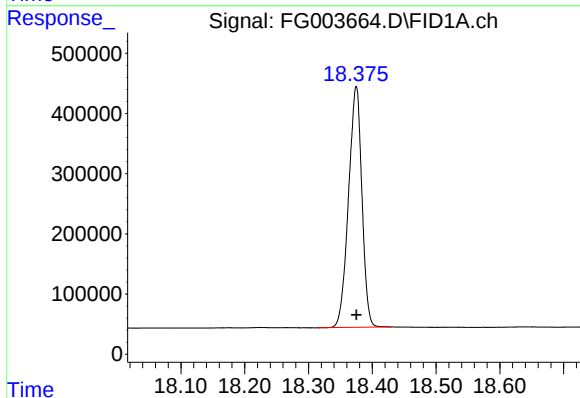


#14 N-DOTRIACONTANE

R.T.: 18.375 min
Delta R.T.: 0.000 min
Response: 5837441
Conc: 50.00 ug/ml

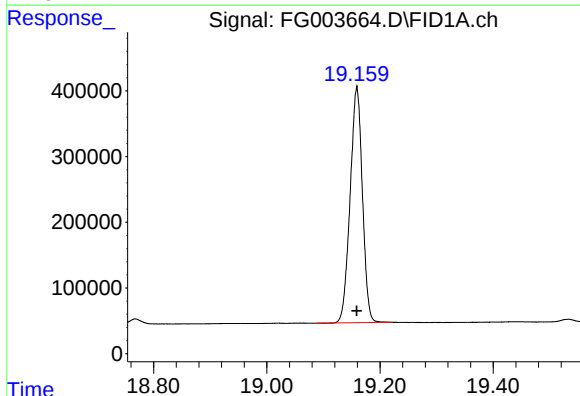


#15 N-TETRATRIACONTANE

R.T.: 19.159 min
Delta R.T.: 0.000 min
Response: 5393132
Conc: 50.00 ug/ml

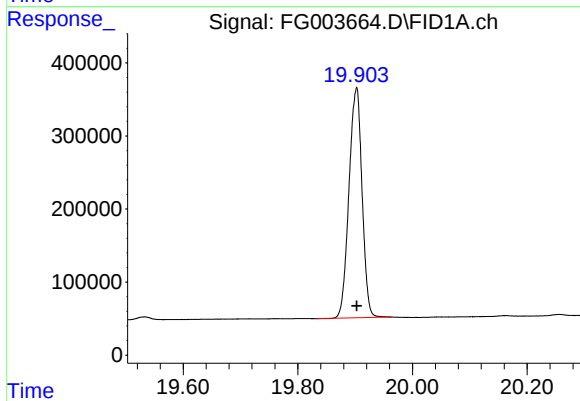


#16 N-HEXATRIACONTANE

R.T.: 19.903 min
Delta R.T.: 0.000 min
Response: 4982440
Conc: 50.00 ug/ml

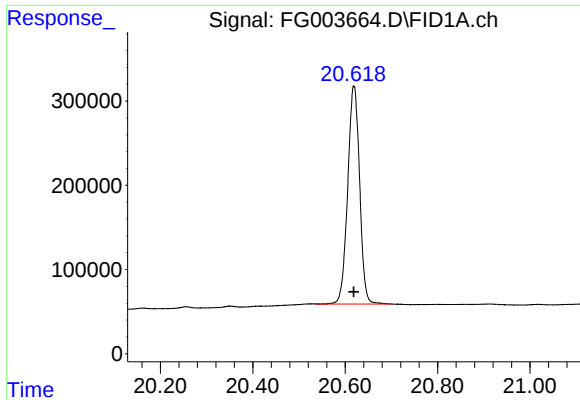

#17 N-OCTATRIACONTANE

R.T.: 20.619 min
Delta R.T.: 0.000 min
Response: 4630537
Conc: 50.00 ug/ml

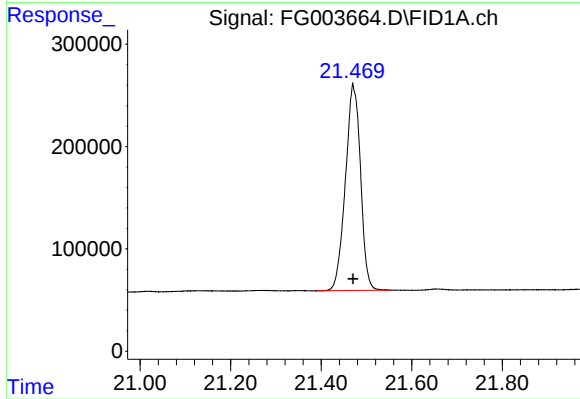

#18 N-TETRACONTANE

R.T.: 21.470 min
Delta R.T.: 0.000 min
Response: 4664277
Conc: 50.00 ug/ml