

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020525AR\
Data File : FG015311.D
Signal(s) : FID1A.ch
Acq On : 05 Feb 2025 20:58
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 06 03:07:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 020525.M
Quant Title : GC Extractables
QLast Update : Thu Feb 06 02:53:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

19) T	Indeno[1,2,3-cd]pyren...	18.540	84232	0.655 ug/ml
20) T	Dibenz[a,h]anthracene...	18.540	84232	0.623 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020525AR\
Data File : FG015311.D
Signal(s) : FID1A.ch
Acq On : 05 Feb 2025 20:58
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 06 03:07:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 020525.M
Quant Title : GC Extractables
QLast Update : Thu Feb 06 02:53:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

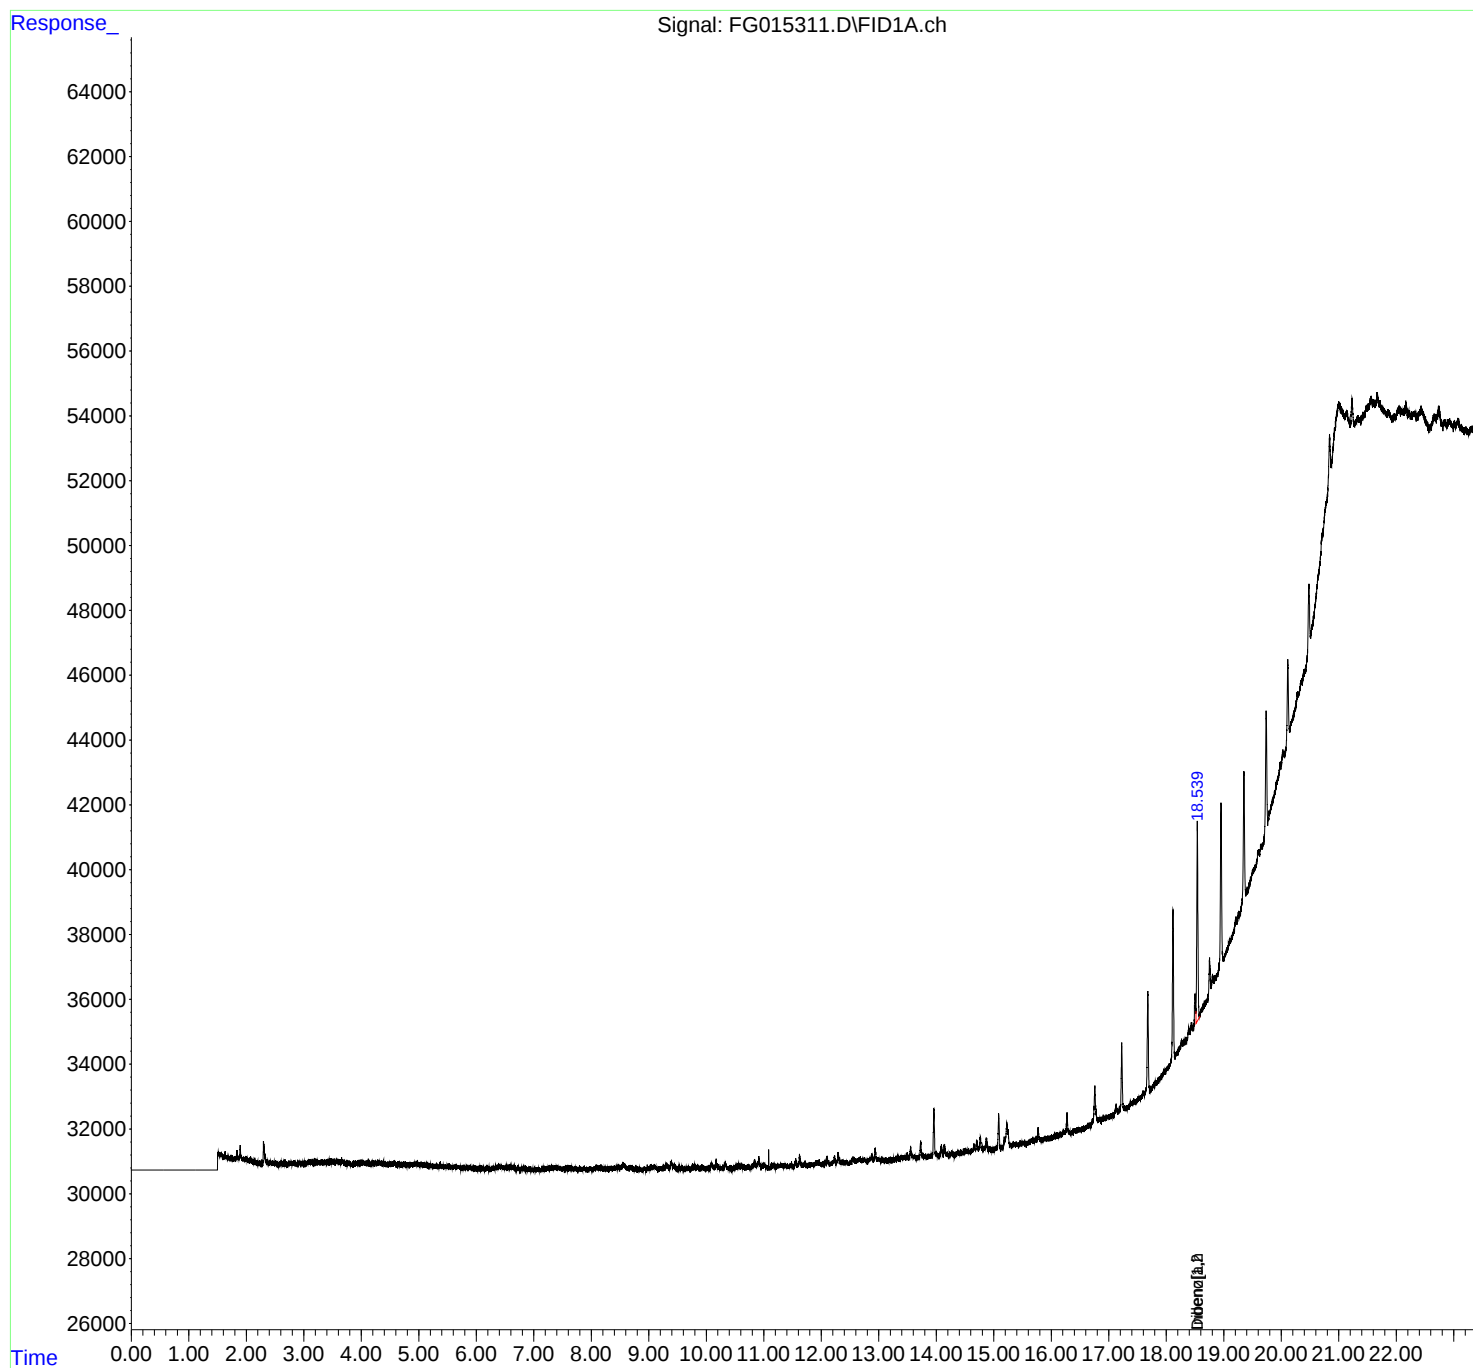


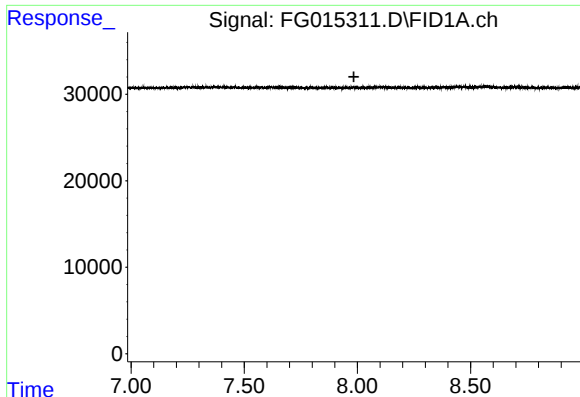

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.985 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

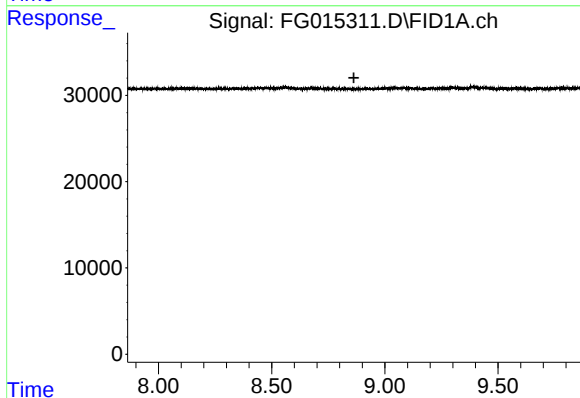


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.863 min
Response: 0
Conc: N.D.

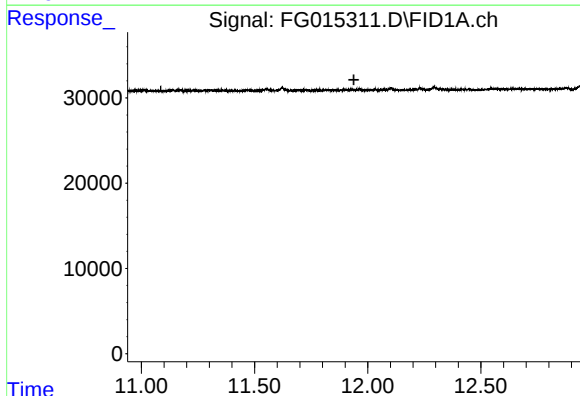


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.939 min
Response: 0
Conc: N.D.

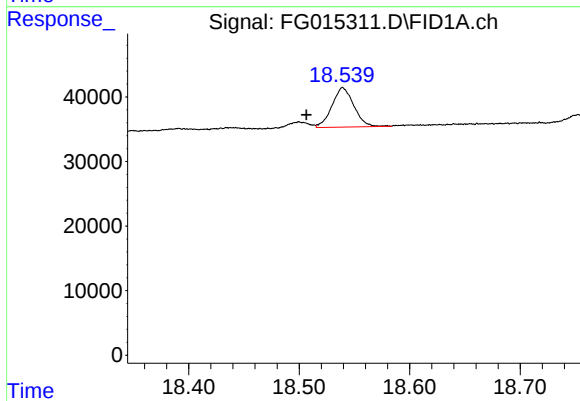

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.540 min
Delta R.T.: 0.033 min
Response: 84232
Conc: 0.66 ug/ml

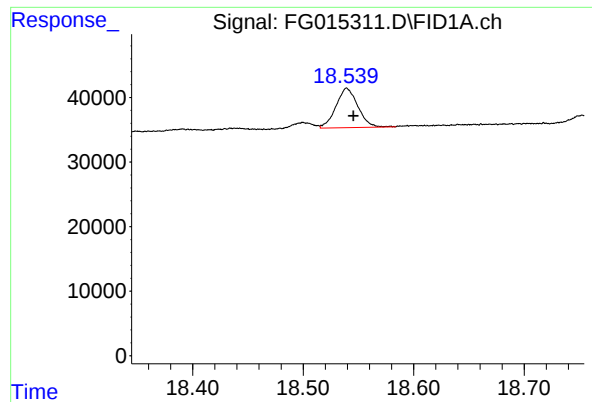

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.540 min
Delta R.T.: -0.006 min
Response: 84232
Conc: 0.62 ug/ml

Instrument :

FID_G

ClientSampleId :