

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020623\
Data File : FG011377.D
Signal(s) : FID1A.ch
Acq On : 06 Feb 2023 09:47
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 07 05:30:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.072	1960619	14.855 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.554	79451	0.685 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020623\
Data File : FG011377.D
Signal(s) : FID1A.ch
Acq On : 06 Feb 2023 09:47
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 07 05:30:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

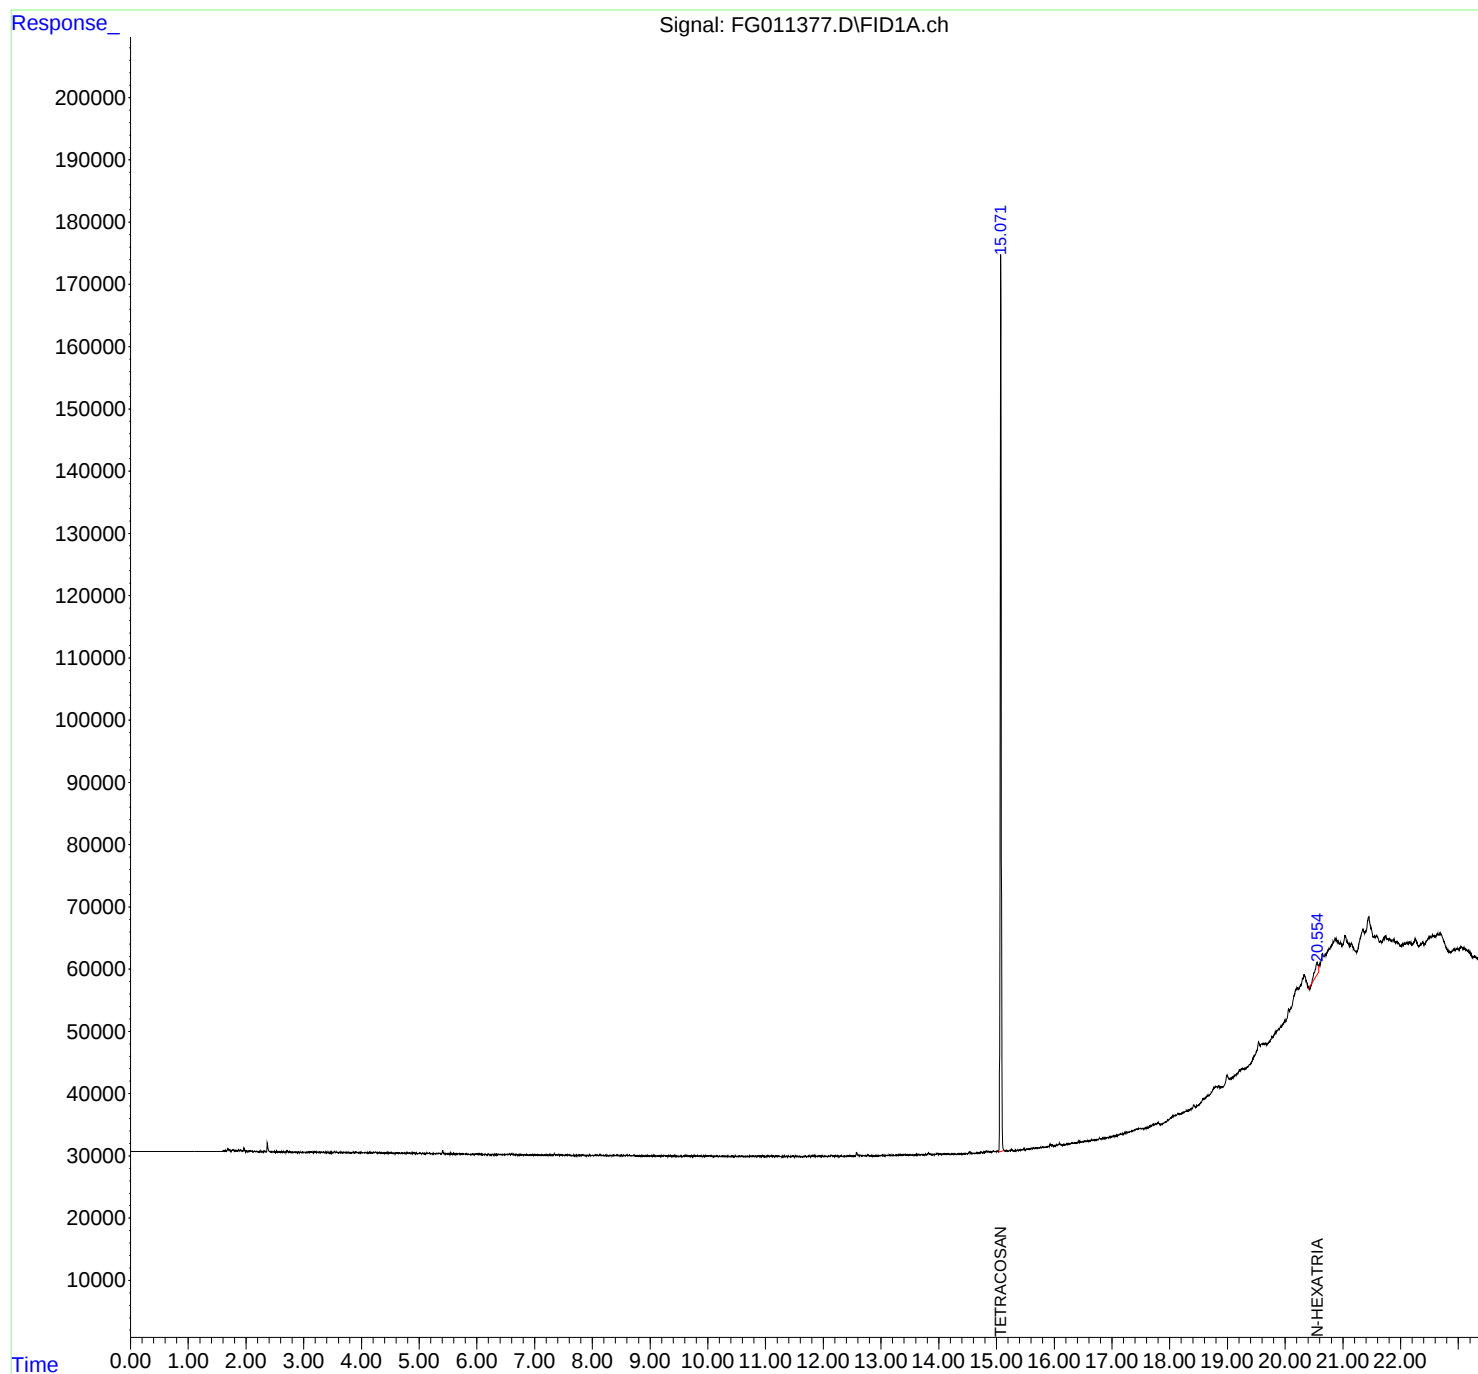


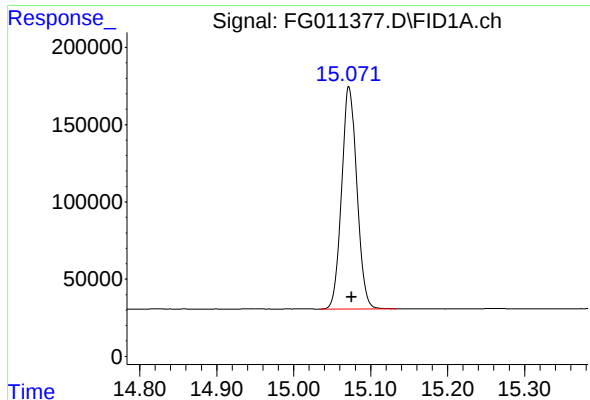

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.072 min
Delta R.T.: -0.004 min
Response: 1960619
Conc: 14.85 ug/ml

Instrument :
FID_G
ClientSampleId :

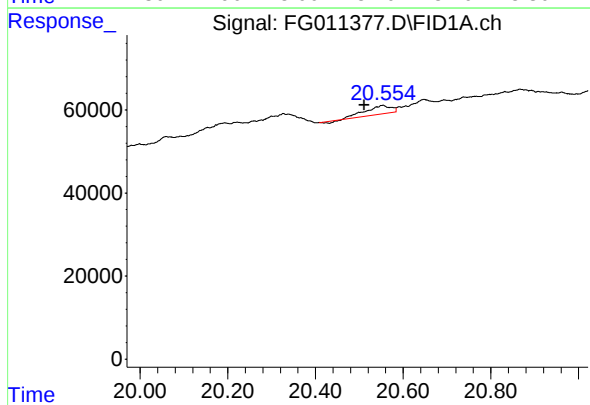

#16 N-HEXATRIACONTANE

R.T.: 20.554 min
Delta R.T.: 0.042 min
Response: 79451
Conc: 0.68 ug/ml