

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020623\
 Data File : FG011379.D
 Signal(s) : FID1A.ch
 Acq On : 06 Feb 2023 10:46
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 07 05:30:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
 Quant Title :
 QLast Update : Mon Jan 30 21:53:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.763	2497771	17.571 ug/ml
12) N-OCTACOSANE	17.256	2343932	16.491 ug/ml
14) N-DOTRIACONTANE	18.987	69047	0.497 ug/ml
15) N-TETRATRIACONTANE	19.766	38069	0.306 ug/ml
16) N-HEXATRIACONTANE	20.550	321637	2.772 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020623\
Data File : FG011379.D
Signal(s) : FID1A.ch
Acq On : 06 Feb 2023 10:46
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 07 05:30:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

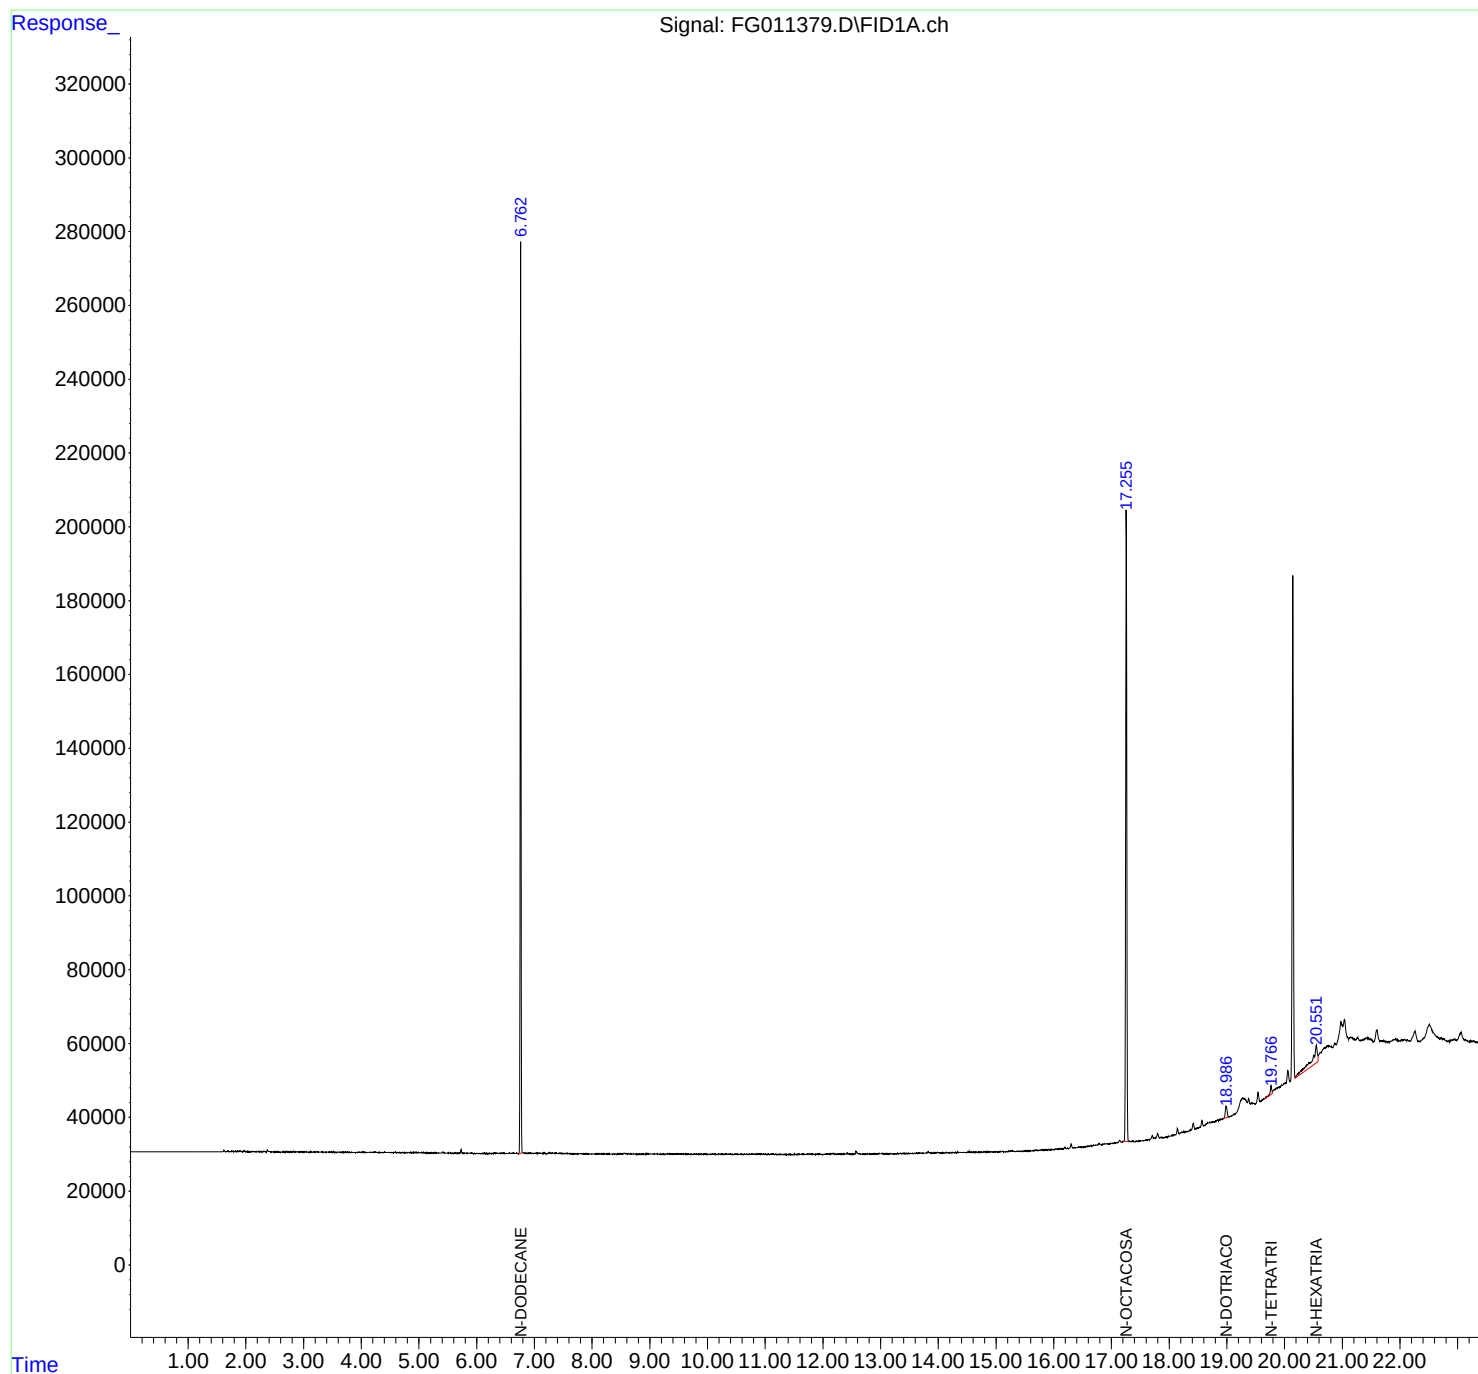


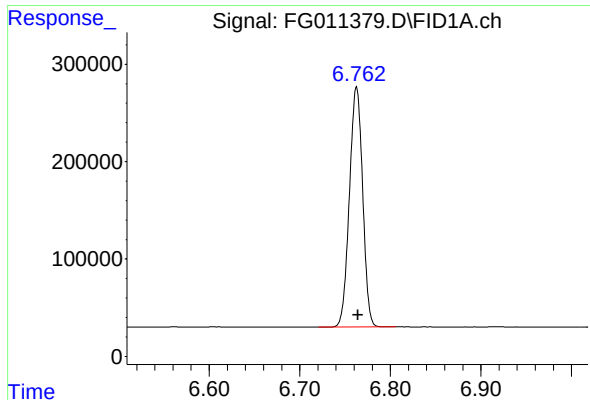

#3 N-DODECANE


R.T.: 6.763 min
Delta R.T.: -0.002 min
Response: 2497771
Conc: 17.57 ug/ml

Instrument :
FID_G
ClientSampleId :

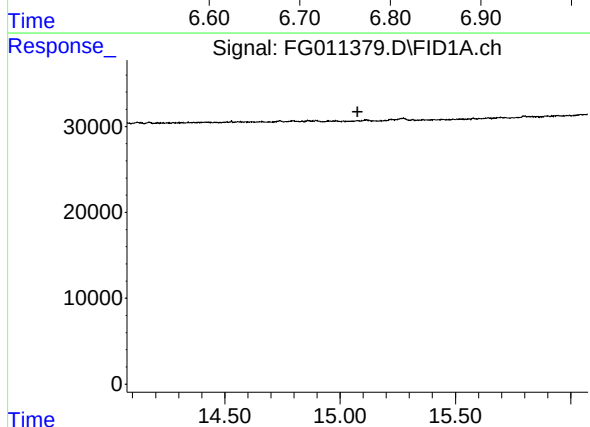


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

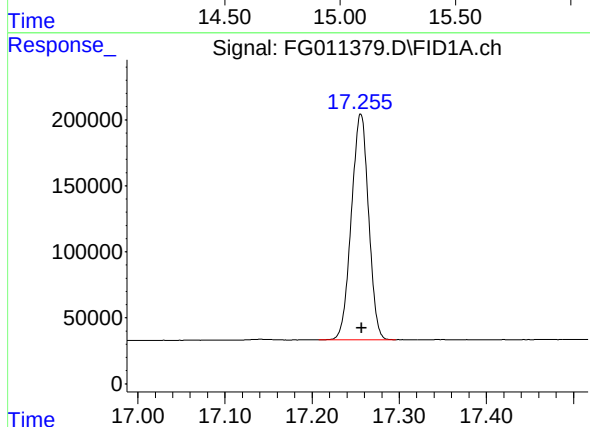


#12 N-OCTACOSANE

R.T.: 17.256 min
Delta R.T.: 0.000 min
Response: 2343932
Conc: 16.49 ug/ml

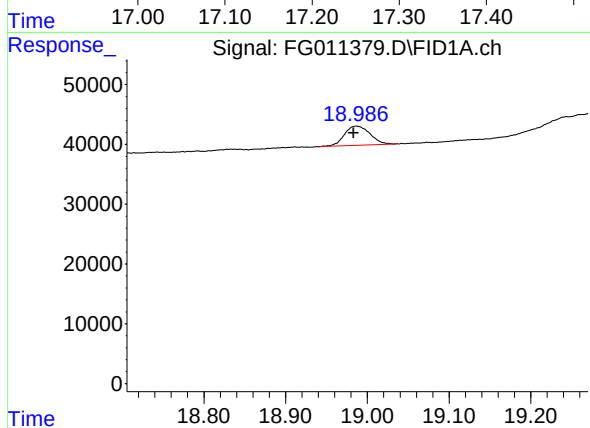

#14 N-DOTRIACONTANE

R.T.: 18.987 min
Delta R.T.: 0.004 min
Response: 69047
Conc: 0.50 ug/ml

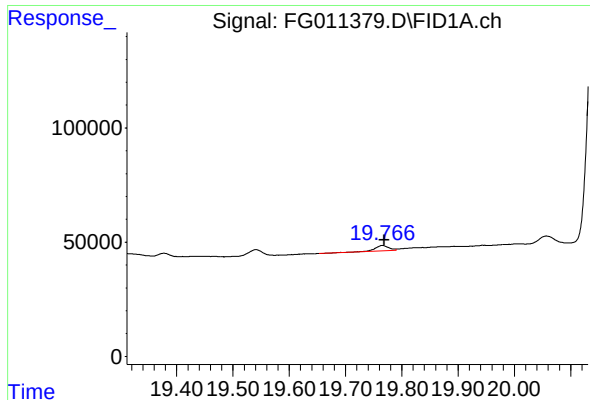


#15 N-TETRATRIACONTANE

R.T.: 19.766 min
Delta R.T.: -0.003 min
Response: 38069
Conc: 0.31 ug/ml

Instrument :

FID_G

ClientSampleId :

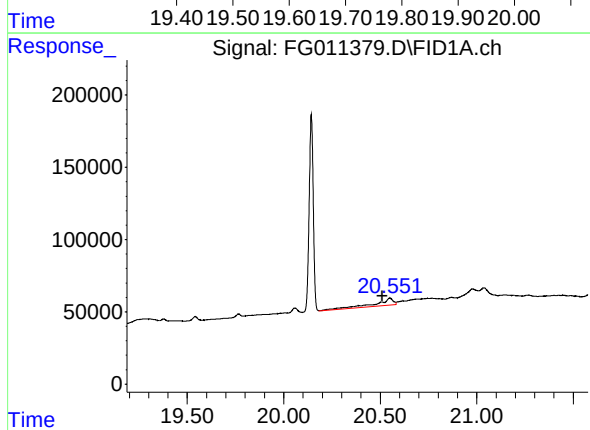

#16 N-HEXATRIACONTANE

R.T.: 20.550 min
Delta R.T.: 0.039 min
Response: 321637
Conc: 2.77 ug/ml