

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020623\
Data File : FG011382.D
Signal(s) : FID1A.ch
Acq On : 06 Feb 2023 12:46
Operator : YP\AJ
Sample : 01418-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
JPP-18A-020223

Integration File: autoint1.e
Quant Time: Feb 07 05:30:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.074	744563	5.641 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020623\
Data File : FG011382.D
Signal(s) : FID1A.ch
Acq On : 06 Feb 2023 12:46
Operator : YP\AJ
Sample : 01418-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
JPP-18A-020223

Integration File: autoint1.e
Quant Time: Feb 07 05:30:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG013023.M
Quant Title :
QLast Update : Mon Jan 30 21:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

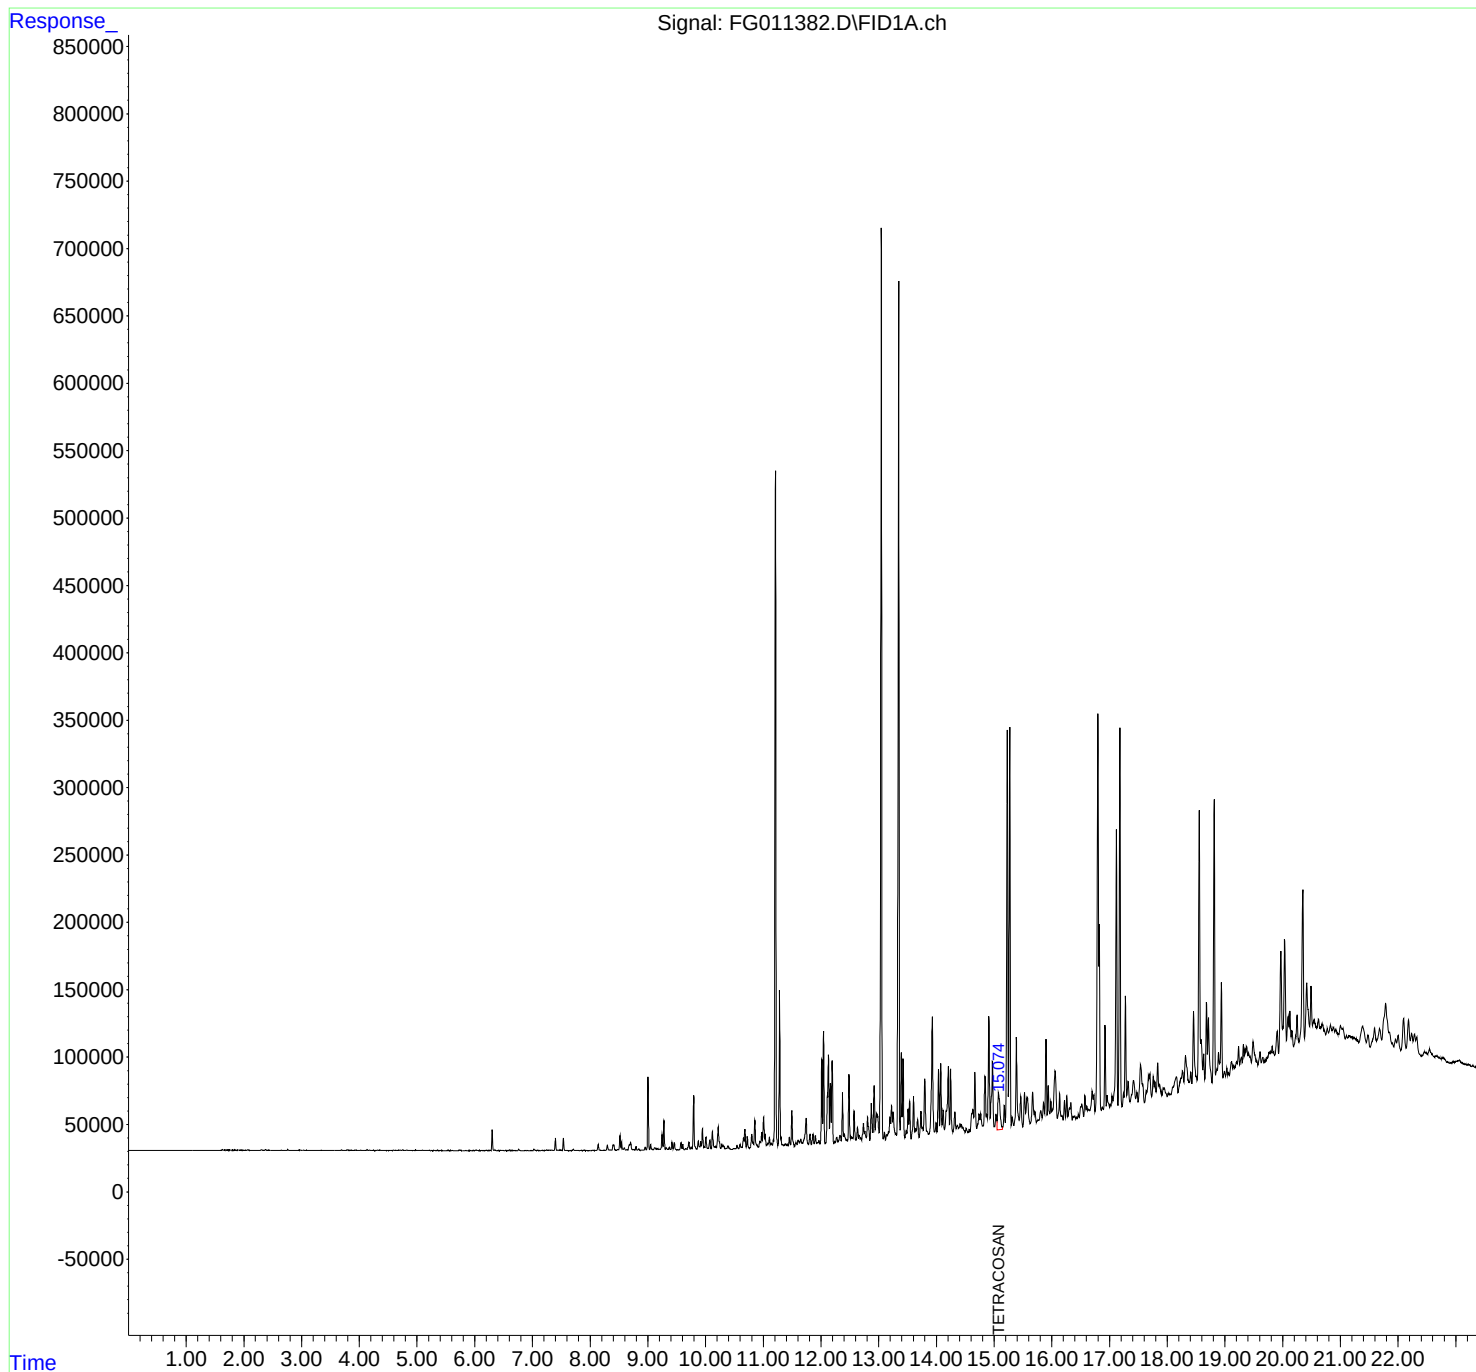

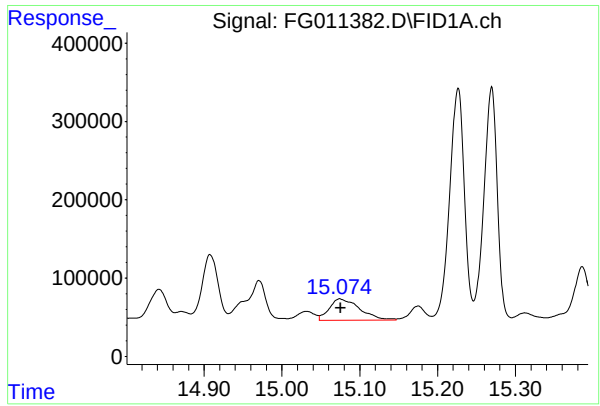

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.074 min
Delta R.T.: -0.001 min
Response: 744563
Conc: 5.64 ug/ml

Instrument :
FID_G
ClientSampleId :
JPP-18A-020223