

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020624\
 Data File : FG013473.D
 Signal(s) : FID1A.ch
 Acq On : 06 Feb 2024 14:09
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 07 04:26:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010824.M
 Quant Title :
 QLast Update : Mon Jan 08 14:52:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.071	6109805	49.970 ug/ml
Target Compounds			
2) N-DECANE	4.585	6543567	50.036 ug/ml
3) N-DODECANE	6.756	6780185	49.856 ug/ml
4) N-TETRADECANE	8.589	6655210	49.927 ug/ml
5) N-HEXADECANE	10.202	6812344	49.989 ug/ml
6) N-OCTADECANE	11.650	7040981	49.970 ug/ml
7) N-EICOSANE	12.966	6877572	49.910 ug/ml
8) N-DOCOSANE	14.168	6757214	49.839 ug/ml
10) N-TETRACOSANE	15.275	6687128	49.700 ug/ml
11) N-HEXACOSANE	16.300	6517054	49.473 ug/ml
12) N-OCTACOSANE	17.254	6371822	49.469 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020624\
Data File : FG013473.D
Signal(s) : FID1A.ch
Acq On : 06 Feb 2024 14:09
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 07 04:26:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG010824.M
Quant Title :
QLast Update : Mon Jan 08 14:52:14 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

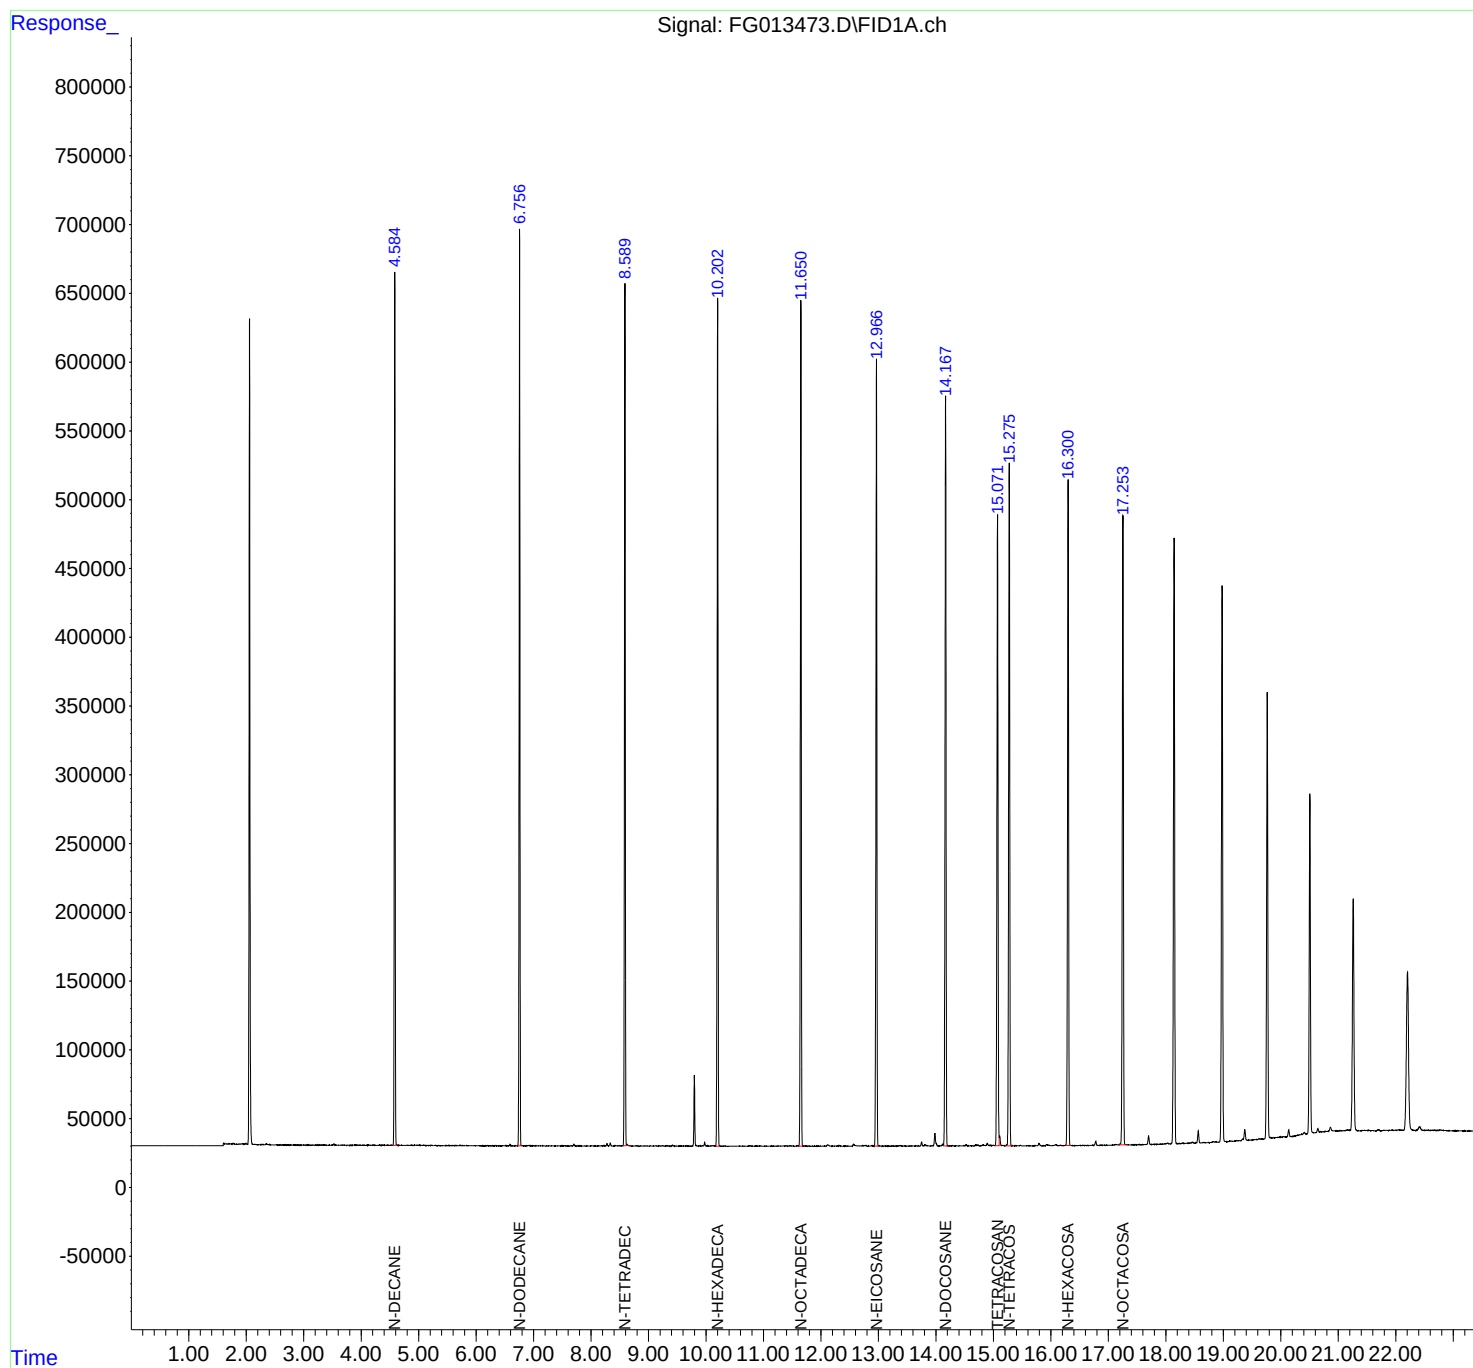

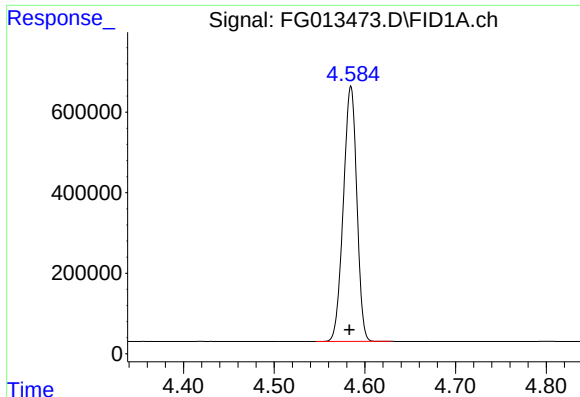


#2 N-DECANE

R.T.: 4.585 min
Delta R.T.: 0.002 min
Response: 6543567
Conc: 50.04 ug/ml

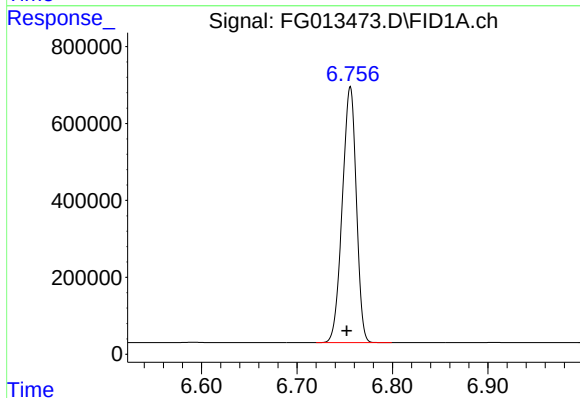


#3 N-DODECANE

R.T.: 6.756 min
Delta R.T.: 0.004 min
Response: 6780185
Conc: 49.86 ug/ml

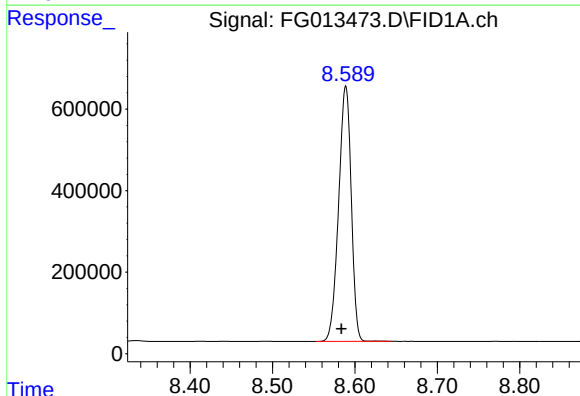


#4 N-TETRADECANE

R.T.: 8.589 min
Delta R.T.: 0.005 min
Response: 6655210
Conc: 49.93 ug/ml

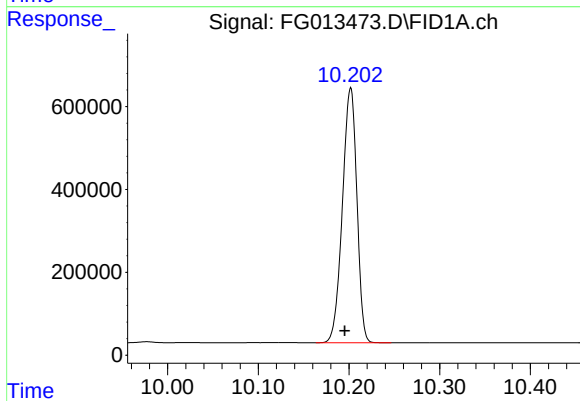


#5 N-HEXADECANE

R.T.: 10.202 min
Delta R.T.: 0.007 min
Response: 6812344
Conc: 49.99 ug/ml

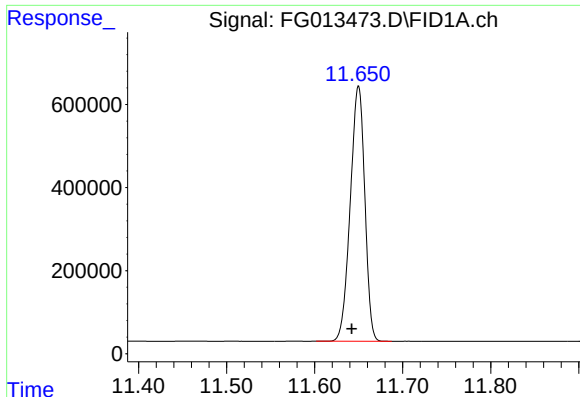


#6 N-OCTADECANE

R.T.: 11.650 min
Delta R.T.: 0.008 min
Response: 7040981
Conc: 49.97 ug/ml

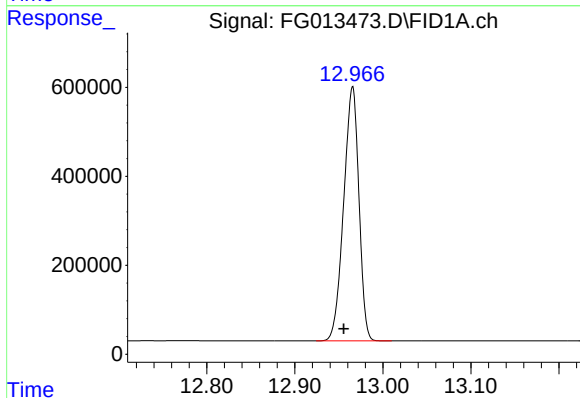


#7 N-EICOSANE

R.T.: 12.966 min
Delta R.T.: 0.010 min
Response: 6877572
Conc: 49.91 ug/ml

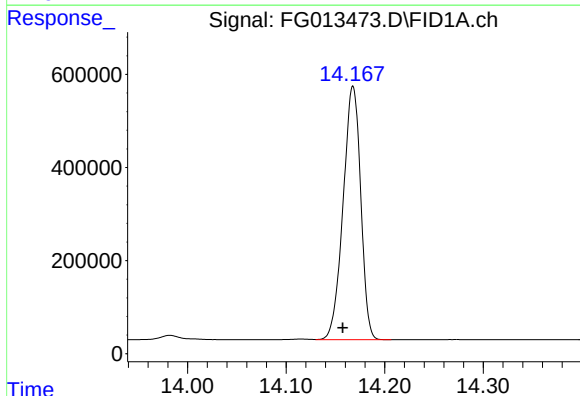


#8 N-DOCOSANE

R.T.: 14.168 min
Delta R.T.: 0.010 min
Response: 6757214
Conc: 49.84 ug/ml

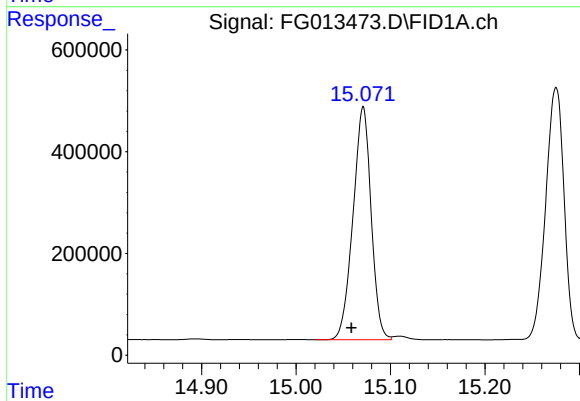


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.071 min
Delta R.T.: 0.012 min
Response: 6109805
Conc: 49.97 ug/ml

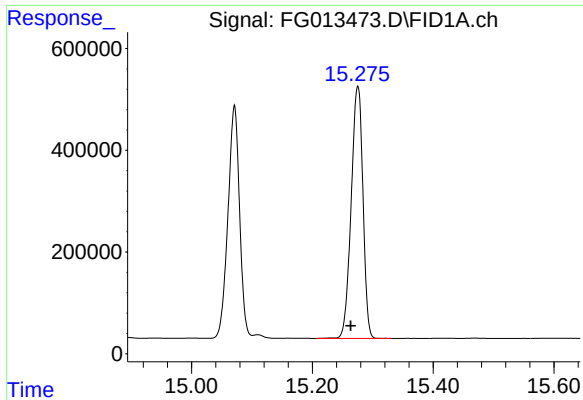


#10 N-TETRACOSANE

R.T.: 15.275 min
Delta R.T.: 0.012 min
Response: 6687128
Conc: 49.70 ug/ml

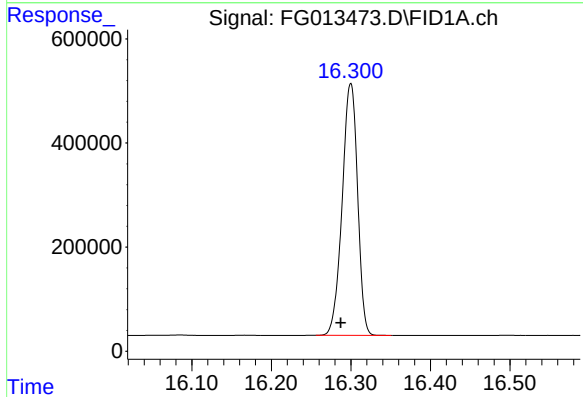

#11 N-HEXACOSANE

R.T.: 16.300 min
Delta R.T.: 0.013 min
Response: 6517054
Conc: 49.47 ug/ml

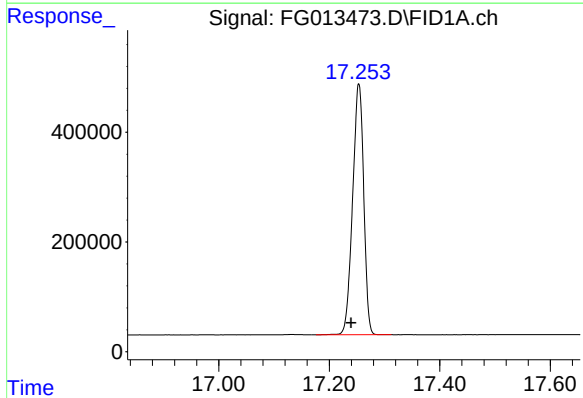

#12 N-OCTACOSANE

R.T.: 17.254 min
Delta R.T.: 0.014 min
Response: 6371822
Conc: 49.47 ug/ml